

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016753.D
 Acq On : 10 Jun 2020 06:18
 Operator : SY/MD
 Sample : L2914-14 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	63	69	82	rVB	151644	145034	10.84%	1.378%
2	1.556	138	145	156	rVB	105186	129358	9.67%	1.229%
3	2.116	309	319	346	rVB	234098	365065	27.28%	3.469%
4	2.248	358	360	366	rVB5	2172	1755	0.13%	0.017%
5	2.364	393	396	399	rBV5	1192	833	0.06%	0.008%
6	2.855	546	549	550	rBV3	1886	1086	0.08%	0.010%
7	2.958	576	581	584	rBV7	1886	2023	0.15%	0.019%
8	3.026	600	602	606	rBV4	1161	823	0.06%	0.008%
9	3.135	634	636	639	rVB3	1175	626	0.05%	0.006%
10	3.222	661	663	667	rBV4	1232	786	0.06%	0.007%
11	3.344	698	701	704	rBV5	1664	1074	0.08%	0.010%
12	3.460	735	737	738	rBV2	1759	767	0.06%	0.007%
13	3.550	763	765	766	rBV2	1243	633	0.05%	0.006%
14	3.592	776	778	780	rBV3	1124	643	0.05%	0.006%
15	3.640	792	793	796	rBV3	1278	684	0.05%	0.006%
16	3.736	817	823	825	rBV6	1215	1414	0.11%	0.013%
17	3.804	842	844	847	rVB3	1648	618	0.05%	0.006%
18	3.833	850	853	855	rBV2	1353	772	0.06%	0.007%
19	3.894	862	872	906	rBV	118696	330632	24.71%	3.142%
20	4.190	962	964	965	rBV2	1331	672	0.05%	0.006%
21	4.277	989	991	994	rBV3	1542	1026	0.08%	0.010%
22	4.373	1005	1021	1045	rBV	223582	547955	40.95%	5.207%
23	4.582	1084	1086	1090	rBV4	1121	664	0.05%	0.006%
24	4.659	1108	1110	1112	rBV4	1438	553	0.04%	0.005%
25	4.746	1134	1137	1138	rBV2	1464	679	0.05%	0.006%
26	4.916	1187	1190	1192	rBV3	1818	1072	0.08%	0.010%
27	4.929	1192	1194	1197	rVV3	1050	601	0.04%	0.006%
28	5.068	1221	1237	1247	rBV2	525115	1338217	100.00%	12.717%
29	5.572	1391	1394	1398	rVB5	2458	1569	0.12%	0.015%
30	5.640	1402	1415	1434	rBV	428073	853025	63.74%	8.106%
31	6.093	1542	1556	1578	rBV	309290	620490	46.37%	5.896%
32	6.559	1698	1701	1702	rBV2	1113	734	0.05%	0.007%
33	6.746	1757	1759	1762	rBV3	801	587	0.04%	0.006%
34	6.807	1776	1778	1781	rBV5	1561	1088	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016753.D
 Acq On : 10 Jun 2020 06:18
 Operator : SY/MD
 Sample : L2914-14 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.936	1815	1818	1819	rBV3	1279	666	0.05%	0.006%
36	7.006	1827	1840	1858	rBV	162940	293008	21.90%	2.784%
37	7.141	1879	1882	1884	rBV4	1519	1104	0.08%	0.010%
38	7.235	1907	1911	1914	rBV5	1806	1240	0.09%	0.012%
39	7.257	1915	1918	1922	rVB6	2129	1373	0.10%	0.013%
40	7.276	1922	1924	1929	rVB6	1229	731	0.05%	0.007%
41	7.338	1930	1943	1959	rBV	602315	1036356	77.44%	9.848%
42	7.643	2028	2038	2056	rVB	115602	193766	14.48%	1.841%
43	7.858	2103	2105	2107	rBV3	1334	654	0.05%	0.006%
44	7.871	2107	2109	2112	rVV4	1466	714	0.05%	0.007%
45	8.039	2159	2161	2164	rBV3	1299	907	0.07%	0.009%
46	8.106	2171	2182	2215	rBV	388675	743855	55.59%	7.069%
47	8.479	2295	2298	2299	rBV2	1197	669	0.05%	0.006%
48	8.569	2322	2326	2328	rBV6	1722	1339	0.10%	0.013%
49	8.582	2328	2330	2332	rBV2	1312	684	0.05%	0.006%
50	8.653	2348	2352	2354	rBV5	1182	1093	0.08%	0.010%
51	8.874	2409	2421	2445	rBV	646912	1058357	79.09%	10.057%
52	9.006	2460	2462	2463	rBV2	1469	685	0.05%	0.007%
53	9.225	2528	2530	2536	rVB5	1973	1965	0.15%	0.019%
54	9.267	2536	2543	2544	rBV6	3033	2751	0.21%	0.026%
55	9.392	2579	2582	2585	rBV5	2121	1744	0.13%	0.017%
56	9.572	2632	2638	2642	rBV8	2557	3422	0.26%	0.033%
57	9.653	2661	2663	2666	rBV3	1243	895	0.07%	0.009%
58	10.186	2825	2829	2832	rBV4	1342	1310	0.10%	0.012%
59	10.238	2833	2845	2863	rVV	427850	665453	49.73%	6.324%
60	10.350	2877	2880	2882	rBV4	1163	695	0.05%	0.007%
61	10.476	2916	2919	2920	rBV2	1321	730	0.05%	0.007%
62	10.678	2978	2982	2983	rBV2	1786	1100	0.08%	0.010%
63	10.868	3039	3041	3044	rVV4	1638	1142	0.09%	0.011%
64	11.132	3121	3123	3126	rBV4	1165	790	0.06%	0.008%
65	11.270	3155	3166	3182	rBV	672086	1028620	76.86%	9.775%
66	11.501	3234	3238	3240	rBV4	1004	789	0.06%	0.007%
67	11.646	3271	3283	3300	rBV	689652	1089603	81.42%	10.354%
68	11.765	3318	3320	3322	rBV3	1385	663	0.05%	0.006%
69	11.778	3322	3324	3328	rVB4	1853	921	0.07%	0.009%
70	11.990	3387	3390	3392	rBV4	1149	816	0.06%	0.008%
71	12.006	3393	3395	3397	rBV2	1300	766	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016753.D
 Acq On : 10 Jun 2020 06:18
 Operator : SY/MD
 Sample : L2914-14 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.061	3409	3412	3416	rBV5	1758	1623	0.12%	0.015%
73	12.099	3422	3424	3426	rVB2	1051	560	0.04%	0.005%
74	12.125	3426	3432	3435	rBV6	1837	2177	0.16%	0.021%
75	12.202	3449	3456	3459	rBV8	1550	2092	0.16%	0.020%
76	12.296	3483	3485	3489	rBV5	1451	873	0.07%	0.008%
77	12.353	3501	3503	3505	rBV3	1078	632	0.05%	0.006%
78	12.460	3534	3536	3539	rVB4	1766	810	0.06%	0.008%
79	12.556	3564	3566	3569	rBV4	743	576	0.04%	0.005%
80	12.579	3571	3573	3577	rVB4	1317	875	0.07%	0.008%
81	12.598	3577	3579	3582	rBV4	821	608	0.05%	0.006%
82	12.697	3607	3610	3611	rBV3	898	562	0.04%	0.005%
83	12.707	3611	3613	3615	rVV3	1252	592	0.04%	0.006%
84	12.800	3640	3642	3644	rBV3	1393	829	0.06%	0.008%
85	12.887	3667	3669	3671	rBV3	1382	843	0.06%	0.008%
86	12.990	3699	3701	3704	rBV4	1032	696	0.05%	0.007%
87	13.466	3846	3849	3853	rBV5	1246	1012	0.08%	0.010%
88	13.585	3883	3886	3889	rBV4	1353	913	0.07%	0.009%
89	13.604	3889	3892	3894	rBV3	1320	975	0.07%	0.009%
90	13.762	3939	3941	3944	rBV4	1325	1018	0.08%	0.010%
91	13.800	3951	3953	3956	rBV2	1686	1158	0.09%	0.011%
92	13.858	3966	3971	3973	rBV5	1233	1160	0.09%	0.011%
93	13.968	4001	4005	4007	rBV5	1500	1383	0.10%	0.013%
94	13.987	4009	4011	4014	rVB3	1375	760	0.06%	0.007%
95	14.041	4025	4028	4033	rBV7	1526	1539	0.12%	0.015%
96	14.672	4222	4224	4228	rVB4	1905	1184	0.09%	0.011%
97	14.804	4263	4265	4269	rVB4	1442	841	0.06%	0.008%
98	15.180	4380	4382	4384	rBV2	1307	554	0.04%	0.005%
99	15.270	4408	4410	4415	rVB5	1687	1040	0.08%	0.010%
100	15.517	4485	4487	4489	rBV3	1321	617	0.05%	0.006%


Sum of corrected areas: 10523436

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016753.D
Acq On : 10 Jun 2020 06:18
Operator : SY/MD
Sample : L2914-14 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

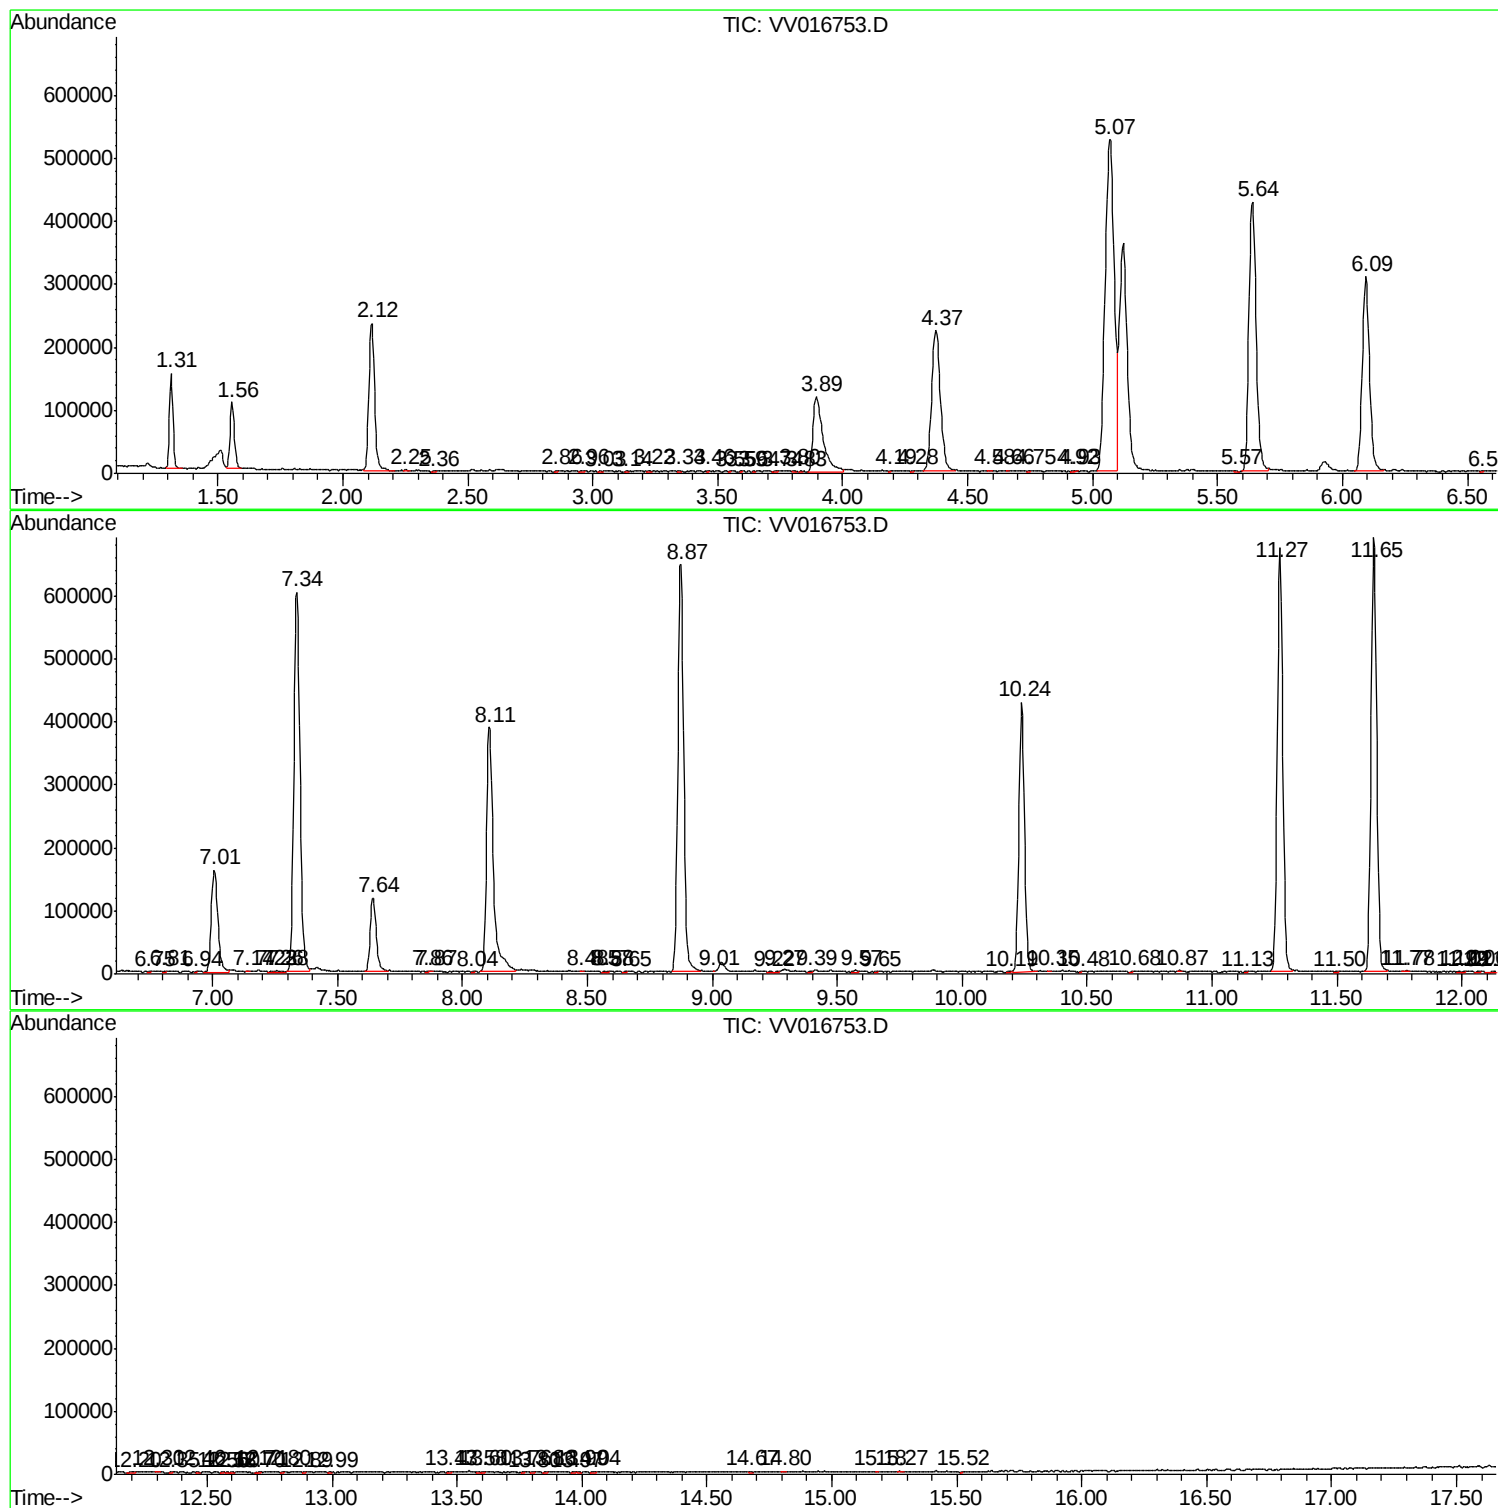

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016753.D
Acq On : 10 Jun 2020 06:18
Operator : SY/MD
Sample : L2914-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016753.D
Acq On : 10 Jun 2020 06:18
Operator : SY/MD
Sample : L2914-14 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 60 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc