

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016754.D
 Acq On : 10 Jun 2020 06:42
 Operator : SY/MD
 Sample : L2914-15 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.312	64	69	78	rVB	146509	146858	10.20%	1.387%
2	1.557	139	145	161	rVB	113681	135894	9.44%	1.283%
3	2.116	309	319	334	rBV	243996	363060	25.23%	3.428%
4	2.631	472	479	491	rBV	4067	9600	0.67%	0.091%
5	2.875	551	555	557	rBV3	1155	889	0.06%	0.008%
6	2.891	557	560	564	rVB2	1481	1104	0.08%	0.010%
7	3.328	693	696	699	rBV4	1449	1031	0.07%	0.010%
8	3.354	701	704	708	rVB3	1650	1263	0.09%	0.012%
9	3.380	708	712	713	rBV4	1409	1065	0.07%	0.010%
10	3.412	718	722	724	rBV3	1550	914	0.06%	0.009%
11	3.434	725	729	735	rVB8	1344	1528	0.11%	0.014%
12	3.470	735	740	742	rBV5	1532	1113	0.08%	0.011%
13	3.524	753	757	760	rBV5	1025	616	0.04%	0.006%
14	3.553	762	766	769	rVV5	1409	963	0.07%	0.009%
15	3.740	821	824	826	rVV4	1508	919	0.06%	0.009%
16	3.846	855	857	861	rVB4	1416	1052	0.07%	0.010%
17	3.894	861	872	901	rBV	116123	325870	22.64%	3.077%
18	4.151	950	952	954	rBV3	1102	768	0.05%	0.007%
19	4.245	978	981	983	rBV4	885	595	0.04%	0.006%
20	4.373	1008	1021	1041	rVB	223561	536372	37.27%	5.065%
21	4.663	1109	1111	1113	rBV2	1582	770	0.05%	0.007%
22	4.756	1138	1140	1145	rVB4	2176	1312	0.09%	0.012%
23	4.778	1145	1147	1152	rBV4	1439	1320	0.09%	0.012%
24	4.801	1152	1154	1156	rBV3	1146	586	0.04%	0.006%
25	4.846	1165	1168	1170	rBV4	1333	929	0.06%	0.009%
26	5.068	1217	1237	1278	rBV2	529399	1439219	100.00%	13.590%
27	5.502	1367	1372	1375	rBV7	2001	1778	0.12%	0.017%
28	5.640	1401	1415	1433	rBV	419458	844933	58.71%	7.979%
29	5.926	1496	1504	1521	rVB5	16714	34114	2.37%	0.322%
30	6.094	1542	1556	1575	rBV	306930	623897	43.35%	5.891%
31	6.312	1620	1624	1625	rBV3	1289	894	0.06%	0.008%
32	6.447	1664	1666	1669	rBV3	1147	620	0.04%	0.006%
33	6.576	1703	1706	1708	rBV3	1099	562	0.04%	0.005%
34	6.769	1763	1766	1773	rVB6	1417	1780	0.12%	0.017%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016754.D
 Acq On : 10 Jun 2020 06:42
 Operator : SY/MD
 Sample : L2914-15 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	6.942	1818	1820	1821	rBV	1433	638	0.04%	0.006%
36	7.007	1829	1840	1861	rBV	161375	289087	20.09%	2.730%
37	7.338	1931	1943	1962	rBV	607855	1047497	72.78%	9.891%
38	7.640	2028	2037	2055	rBV	117922	195613	13.59%	1.847%
39	7.888	2110	2114	2118	rBV7	1728	1843	0.13%	0.017%
40	8.106	2169	2182	2213	rBV	374857	730980	50.79%	6.903%
41	8.434	2282	2284	2287	rBV3	1588	953	0.07%	0.009%
42	8.614	2337	2340	2341	rBV3	1027	706	0.05%	0.007%
43	8.650	2347	2351	2355	rBV6	1668	1763	0.12%	0.017%
44	8.810	2399	2401	2403	rBV2	1225	683	0.05%	0.006%
45	8.872	2409	2420	2439	rBV	623998	1027343	71.38%	9.701%
46	9.042	2469	2473	2479	rBV8	2533	2475	0.17%	0.023%
47	9.164	2507	2511	2515	rVB7	1689	1401	0.10%	0.013%
48	9.238	2531	2534	2537	rBV4	1708	1216	0.08%	0.011%
49	9.309	2553	2556	2557	rBV3	1182	632	0.04%	0.006%
50	9.492	2610	2613	2615	rBV4	1913	1071	0.07%	0.010%
51	9.595	2642	2645	2648	rBV4	1290	896	0.06%	0.008%
52	9.611	2648	2650	2652	rBV3	1415	756	0.05%	0.007%
53	9.682	2670	2672	2678	rVB6	1448	1206	0.08%	0.011%
54	9.711	2678	2681	2685	rBV3	1222	892	0.06%	0.008%
55	9.743	2685	2691	2697	rBV9	2540	3129	0.22%	0.030%
56	10.029	2777	2780	2782	rBV4	1229	695	0.05%	0.007%
57	10.109	2801	2805	2808	rBV5	2285	1228	0.09%	0.012%
58	10.238	2833	2845	2863	rBV	421250	660712	45.91%	6.239%
59	10.347	2875	2879	2880	rBV4	1388	956	0.07%	0.009%
60	10.701	2985	2989	2994	rBV6	1674	1414	0.10%	0.013%
61	10.727	2994	2997	3000	rBV4	1193	986	0.07%	0.009%
62	10.794	3014	3018	3019	rBV3	1296	870	0.06%	0.008%
63	11.019	3085	3088	3092	rBV6	1020	1016	0.07%	0.010%
64	11.109	3114	3116	3120	rVB4	1636	957	0.07%	0.009%
65	11.145	3120	3127	3128	rBV7	1549	1462	0.10%	0.014%
66	11.170	3133	3135	3139	rVV4	1137	743	0.05%	0.007%
67	11.270	3155	3166	3182	rBV	654462	1008576	70.08%	9.524%
68	11.428	3209	3215	3216	rBV5	1652	1369	0.10%	0.013%
69	11.560	3252	3256	3258	rBV5	1742	1211	0.08%	0.011%
70	11.646	3272	3283	3302	rBV	692187	1081937	75.18%	10.217%
71	11.955	3378	3379	3382	rBV3	1087	591	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016754.D
 Acq On : 10 Jun 2020 06:42
 Operator : SY/MD
 Sample : L2914-15 50X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E27

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.039	3402	3405	3407	rBV2	872	586	0.04%	0.006%
73	12.061	3407	3412	3413	rBV4	1062	569	0.04%	0.005%
74	12.074	3414	3416	3420	rVB6	1557	963	0.07%	0.009%
75	12.196	3451	3454	3457	rBV4	1794	1102	0.08%	0.010%
76	12.354	3498	3503	3506	rBV7	1647	1229	0.09%	0.012%
77	12.495	3544	3547	3550	rBV3	1288	895	0.06%	0.008%
78	12.598	3576	3579	3581	rBV3	1612	733	0.05%	0.007%
79	12.698	3605	3610	3611	rBV3	1854	1558	0.11%	0.015%
80	12.804	3639	3643	3646	rBV5	1014	1009	0.07%	0.010%
81	12.997	3701	3703	3707	rVB5	1440	728	0.05%	0.007%
82	13.071	3722	3726	3727	rBV4	1381	805	0.06%	0.008%
83	13.109	3736	3738	3741	rBV3	1116	767	0.05%	0.007%
84	13.238	3776	3778	3781	rBV3	1314	927	0.06%	0.009%
85	13.254	3781	3783	3788	rVV6	1544	1165	0.08%	0.011%
86	13.277	3788	3790	3792	rVV3	1560	661	0.05%	0.006%
87	13.675	3910	3914	3916	rBV4	1101	937	0.07%	0.009%
88	13.791	3947	3950	3954	rVB3	1740	1069	0.07%	0.010%
89	13.855	3967	3970	3972	rBV3	1033	611	0.04%	0.006%
90	13.907	3984	3986	3989	rBV4	1288	900	0.06%	0.008%
91	13.945	3995	3998	3999	rBV3	1348	766	0.05%	0.007%
92	13.994	4011	4013	4016	rVV3	1848	1199	0.08%	0.011%
93	14.032	4022	4025	4028	rBV4	1824	1694	0.12%	0.016%
94	14.222	4079	4084	4085	rBV5	1560	1515	0.11%	0.014%
95	14.440	4150	4152	4158	rVB4	1421	1425	0.10%	0.013%
96	14.617	4204	4207	4208	rBV3	1573	907	0.06%	0.009%
97	14.704	4232	4234	4241	rBV6	1090	960	0.07%	0.009%
98	14.756	4245	4250	4254	rBV7	2022	1908	0.13%	0.018%
99	14.881	4286	4289	4296	rVB7	1675	1589	0.11%	0.015%
100	14.948	4307	4310	4314	rBV3	1397	1199	0.08%	0.011%


Sum of corrected areas: 10590067

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016754.D
Acq On : 10 Jun 2020 06:42
Operator : SY/MD
Sample : L2914-15 50X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E27

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

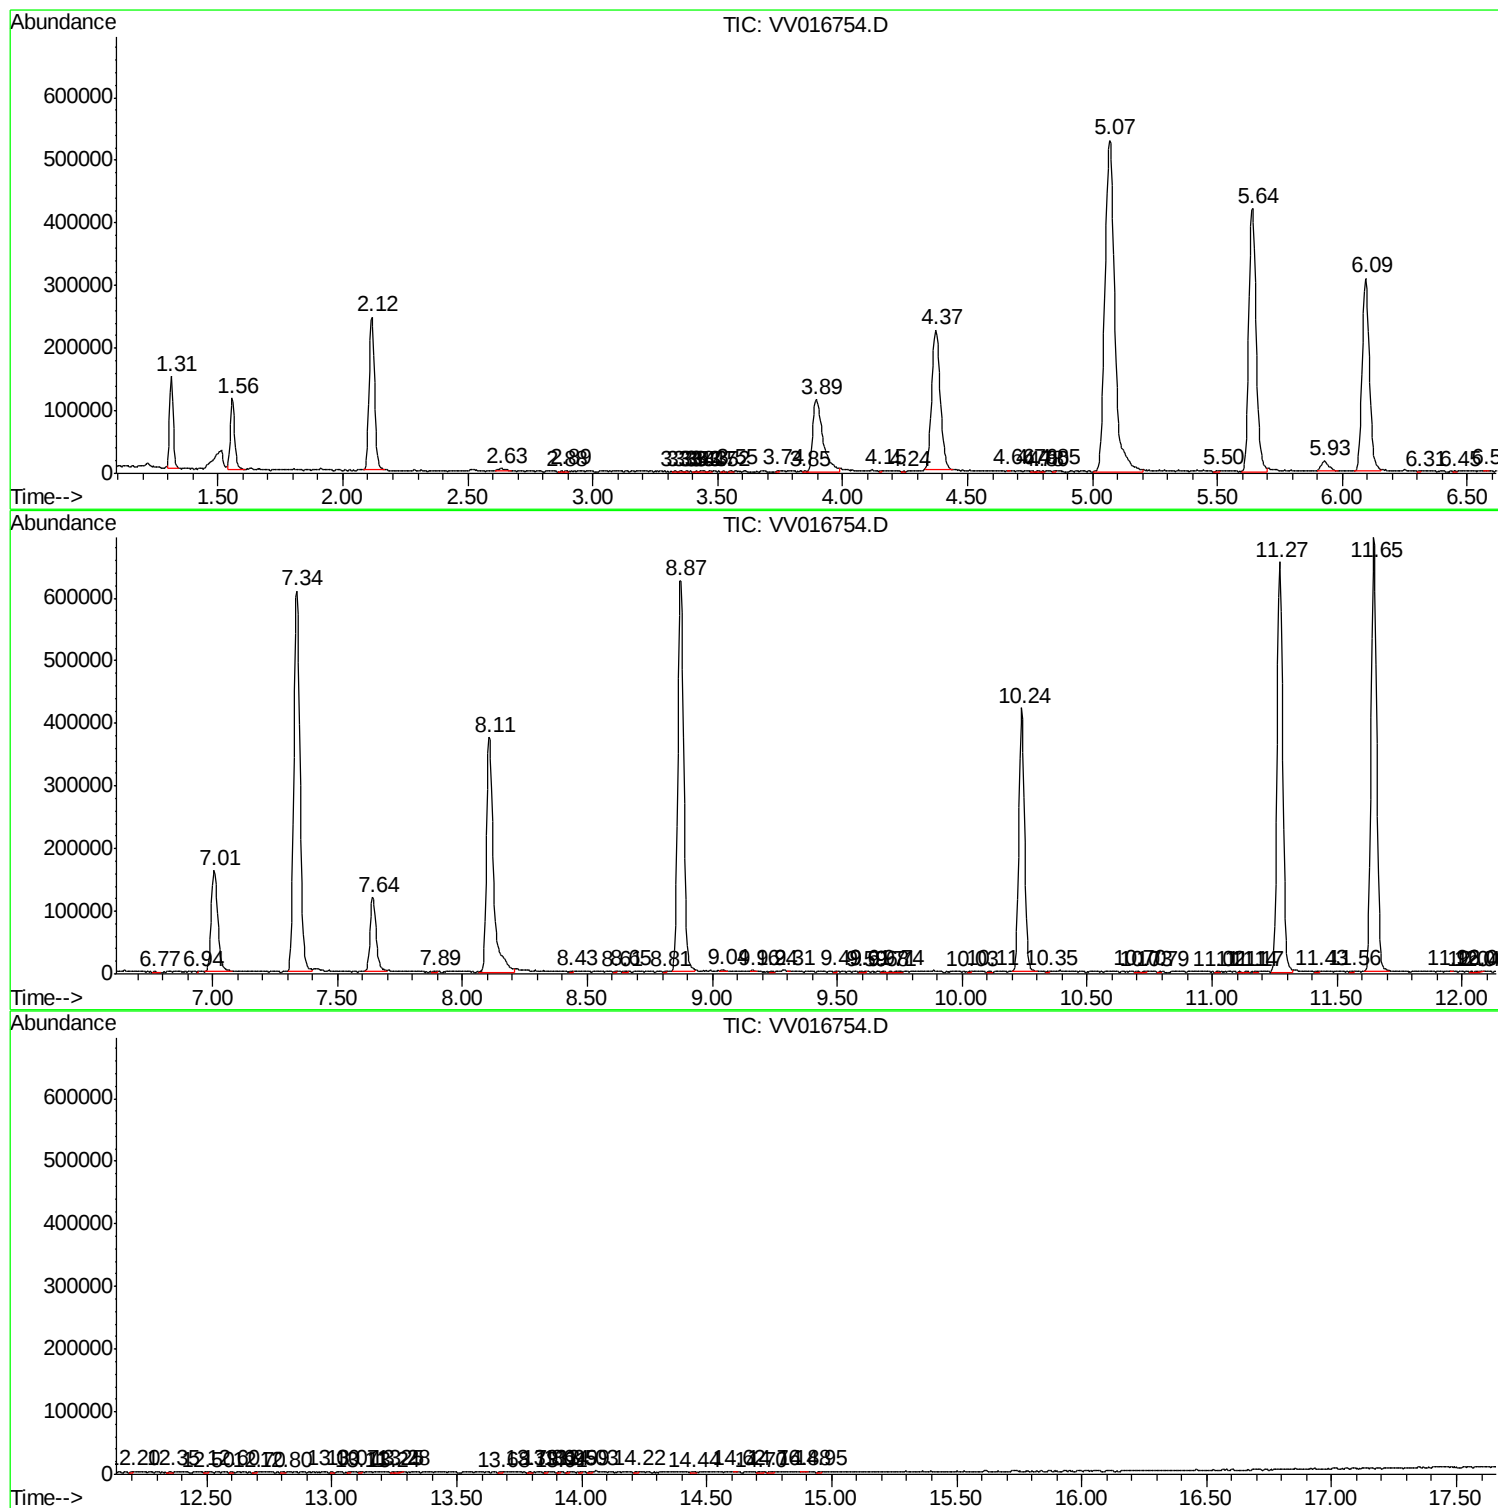

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016754.D
Acq On : 10 Jun 2020 06:42
Operator : SY/MD
Sample : L2914-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E27

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016754.D
Acq On : 10 Jun 2020 06:42
Operator : SY/MD
Sample : L2914-15 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 61 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E27

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc