

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016755.D
 Acq On : 10 Jun 2020 08:59
 Operator : SY/MD
 Sample : L2914-09DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E12DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	79	rVB	182620	190127	13.16%	1.641%
2	1.566	141	148	158	rVB	123241	144584	10.01%	1.248%
3	2.116	310	319	335	rBV	276975	408134	28.25%	3.524%
4	2.897	560	562	567	rVB4	1234	703	0.05%	0.006%
5	2.936	570	574	575	rBV3	1387	936	0.06%	0.008%
6	3.110	626	628	632	rVB3	1605	1126	0.08%	0.010%
7	3.216	656	661	663	rBV6	1953	2000	0.14%	0.017%
8	3.434	723	729	731	rBV6	2755	2101	0.15%	0.018%
9	3.695	809	810	814	rVB5	1441	791	0.05%	0.007%
10	3.765	829	832	833	rBV3	2323	1334	0.09%	0.012%
11	3.891	860	871	906	rBV	119099	329524	22.80%	2.845%
12	4.148	949	951	953	rBV3	1345	865	0.06%	0.007%
13	4.315	1001	1003	1004	rBV2	1310	578	0.04%	0.005%
14	4.370	1004	1020	1039	rVV	249267	601562	41.63%	5.194%
15	4.640	1101	1104	1107	rBV5	1693	939	0.06%	0.008%
16	4.782	1146	1148	1151	rBV4	1295	870	0.06%	0.008%
17	4.839	1162	1166	1169	rBV6	1295	917	0.06%	0.008%
18	5.064	1218	1236	1244	rBV2	581150	1444977	100.00%	12.475%
19	5.637	1401	1414	1434	rBV	466710	926807	64.14%	8.002%
20	6.039	1536	1539	1540	rBV4	1484	840	0.06%	0.007%
21	6.090	1542	1555	1578	rVV	337503	683330	47.29%	5.900%
22	6.431	1657	1661	1662	rBV4	1169	735	0.05%	0.006%
23	6.627	1718	1722	1724	rBV4	2031	1545	0.11%	0.013%
24	6.875	1797	1799	1803	rVB5	1463	861	0.06%	0.007%
25	6.945	1819	1821	1823	rBV2	1440	882	0.06%	0.008%
26	7.003	1828	1839	1856	rVV	189424	341059	23.60%	2.945%
27	7.238	1910	1912	1913	rBV2	1455	536	0.04%	0.005%
28	7.334	1927	1942	1956	rBV	682889	1166906	80.76%	10.074%
29	7.408	1958	1965	1980	rVB	101652	176878	12.24%	1.527%
30	7.640	2026	2037	2053	rBV	135938	232548	16.09%	2.008%
31	7.804	2086	2088	2091	rBV3	1124	557	0.04%	0.005%
32	7.945	2127	2132	2135	rBV6	1401	1692	0.12%	0.015%
33	8.103	2171	2181	2211	rBV	384974	730263	50.54%	6.305%
34	8.630	2342	2345	2347	rBV4	1815	1199	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016755.D
 Acq On : 10 Jun 2020 08:59
 Operator : SY/MD
 Sample : L2914-09DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E12DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

35	8.656	2351	2353	2358	rBV3	1121	681	0.05%	0.006%
36	8.707	2366	2369	2370	rBV3	2016	1211	0.08%	0.010%
37	8.736	2376	2378	2381	rBV3	1321	769	0.05%	0.007%
38	8.772	2386	2389	2391	rBV3	1524	879	0.06%	0.008%
39	8.797	2394	2397	2400	rBV4	1338	1227	0.08%	0.011%
40	8.871	2408	2420	2446	rBV	695209	1131501	78.31%	9.769%
41	9.032	2461	2470	2482	rVB	65190	99411	6.88%	0.858%
42	9.392	2579	2582	2583	rBV3	1410	830	0.06%	0.007%
43	9.630	2654	2656	2659	rVB4	1123	577	0.04%	0.005%
44	9.791	2705	2706	2709	rVB4	1457	584	0.04%	0.005%
45	9.813	2709	2713	2717	rVB7	1227	851	0.06%	0.007%
46	9.932	2747	2750	2753	rBV4	2189	1931	0.13%	0.017%
47	10.051	2783	2787	2789	rBV5	2026	1307	0.09%	0.011%
48	10.190	2828	2830	2831	rBV2	1403	664	0.05%	0.006%
49	10.238	2833	2845	2861	rVV	425904	671302	46.46%	5.796%
50	10.338	2874	2876	2877	rBV2	1279	551	0.04%	0.005%
51	10.431	2901	2905	2909	rBV6	2523	2256	0.16%	0.019%
52	10.553	2940	2943	2944	rBV3	1407	919	0.06%	0.008%
53	10.649	2970	2973	2974	rBV3	904	532	0.04%	0.005%
54	10.704	2986	2990	2992	rBV5	1357	1056	0.07%	0.009%
55	11.026	3086	3090	3091	rBV3	1380	873	0.06%	0.008%
56	11.112	3111	3117	3119	rBV7	1768	1726	0.12%	0.015%
57	11.129	3119	3122	3125	rVV5	942	625	0.04%	0.005%
58	11.270	3155	3166	3180	rBV	713646	1089471	75.40%	9.406%
59	11.482	3230	3232	3237	rVB3	1327	609	0.04%	0.005%
60	11.508	3237	3240	3242	rBV4	1401	901	0.06%	0.008%
61	11.553	3249	3254	3259	rBV9	2942	3138	0.22%	0.027%
62	11.588	3263	3265	3268	rBV4	1627	944	0.07%	0.008%
63	11.604	3268	3270	3271	rBV2	1152	561	0.04%	0.005%
64	11.646	3271	3283	3300	rBV	719190	1129495	78.17%	9.752%
65	11.903	3361	3363	3367	rVB4	1774	978	0.07%	0.008%
66	11.990	3388	3390	3393	rVB4	1255	555	0.04%	0.005%
67	12.006	3393	3395	3397	rBV3	1095	639	0.04%	0.006%
68	12.055	3408	3410	3414	rVB3	2382	1688	0.12%	0.015%
69	12.087	3414	3420	3423	rBV6	1633	1948	0.13%	0.017%
70	12.109	3423	3427	3428	rBV3	1528	1123	0.08%	0.010%
71	12.190	3450	3452	3454	rBV2	996	610	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060920\
 Data File : VV016755.D
 Acq On : 10 Jun 2020 08:59
 Operator : SY/MD
 Sample : L2914-09DL 500X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9E12DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis

72	12.318	3489	3492	3494	rBV3	1412	759	0.05%	0.007%
73	12.444	3525	3531	3532	rBV5	1028	972	0.07%	0.008%
74	12.501	3547	3549	3553	rVB5	1497	695	0.05%	0.006%
75	12.588	3573	3576	3581	rVB7	1473	1235	0.09%	0.011%
76	12.672	3599	3602	3607	rBV6	987	1098	0.08%	0.009%
77	12.723	3616	3618	3623	rVB4	1455	861	0.06%	0.007%
78	12.746	3623	3625	3627	rBV3	1056	771	0.05%	0.007%
79	12.813	3640	3646	3648	rBV5	1133	1249	0.09%	0.011%
80	12.977	3694	3697	3701	rBV3	741	676	0.05%	0.006%
81	13.000	3701	3704	3709	rVB6	1598	1378	0.10%	0.012%
82	13.022	3709	3711	3714	rBV3	1447	766	0.05%	0.007%
83	13.106	3734	3737	3742	rVB5	2229	1883	0.13%	0.016%
84	13.132	3742	3745	3750	rBV5	1844	1783	0.12%	0.015%
85	13.170	3754	3757	3758	rBV4	1297	620	0.04%	0.005%
86	13.209	3767	3769	3772	rVB4	1631	805	0.06%	0.007%
87	13.231	3772	3776	3780	rVB5	1148	905	0.06%	0.008%
88	13.344	3808	3811	3816	rVB5	1380	1259	0.09%	0.011%
89	13.624	3896	3898	3900	rBV3	1008	569	0.04%	0.005%
90	13.743	3933	3935	3938	rVB4	1386	672	0.05%	0.006%
91	13.765	3938	3942	3945	rBV5	1258	1320	0.09%	0.011%
92	13.813	3954	3957	3959	rBV3	829	542	0.04%	0.005%
93	13.855	3967	3970	3973	rBV4	1177	1055	0.07%	0.009%
94	14.013	4016	4019	4023	rBV5	1515	1284	0.09%	0.011%
95	14.167	4064	4067	4071	rBV4	1268	1261	0.09%	0.011%
96	14.331	4116	4118	4120	rBV3	1060	593	0.04%	0.005%
97	14.566	4188	4191	4193	rBV4	960	712	0.05%	0.006%
98	14.710	4233	4236	4239	rVB3	1812	1202	0.08%	0.010%
99	14.730	4239	4242	4245	rBV3	1551	747	0.05%	0.006%
100	15.215	4390	4393	4396	rBV5	1880	1470	0.10%	0.013%


Sum of corrected areas: 11582771

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060920\
Data File : VV016755.D
Acq On : 10 Jun 2020 08:59
Operator : SY/MD
Sample : L2914-09DL 500X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E12DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

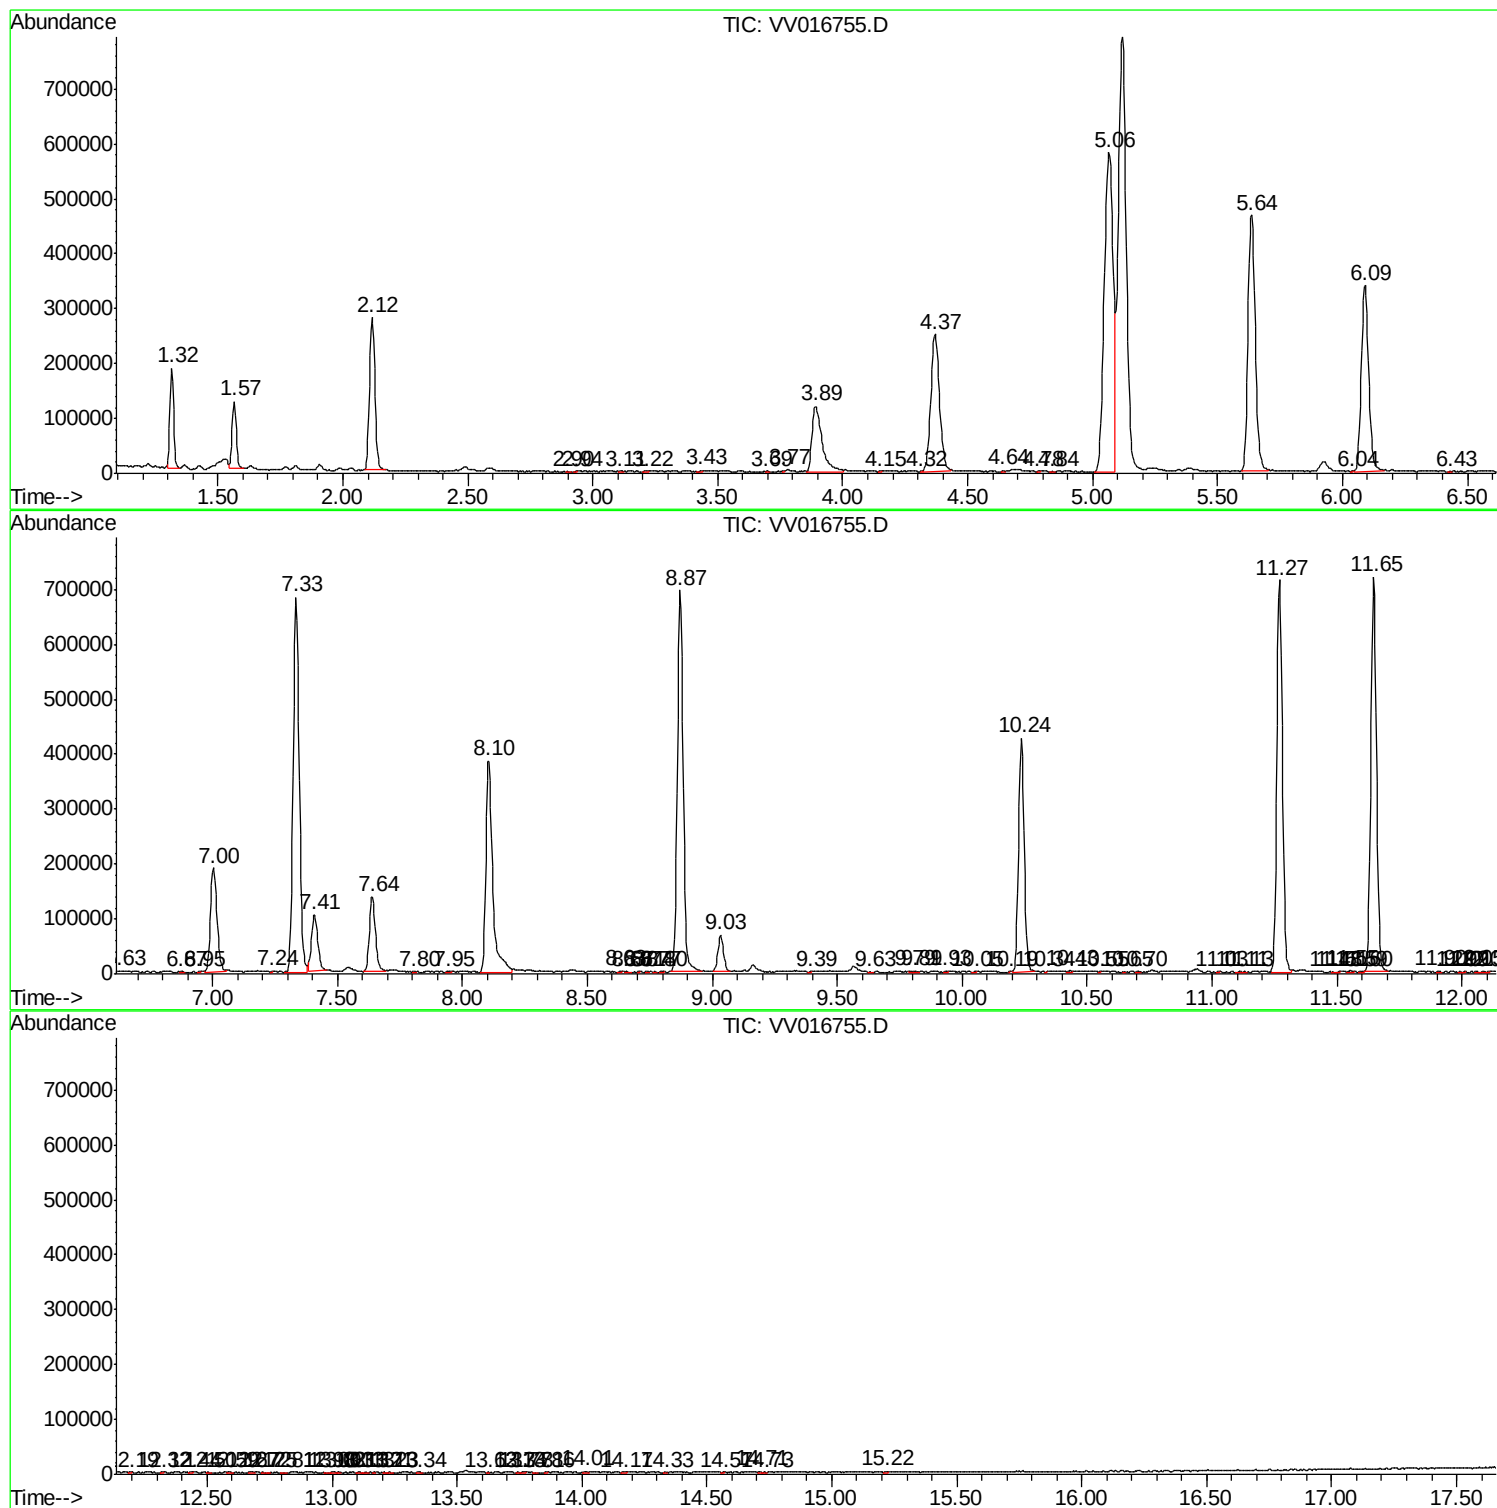

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016755.D
Acq On : 10 Jun 2020 08:59
Operator : SY/MD
Sample : L2914-09DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E12DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV060920\
Data File : VV016755.D
Acq On : 10 Jun 2020 08:59
Operator : SY/MD
Sample : L2914-09DL 500X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 62 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9E12DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc