


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV060920\
 Data File : VV016697.D
 Acq On : 09 Jun 2020 06:52
 Operator : SY/MD
 Sample : BFB84
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB84

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
 Title : VOC Analysis
 Last Update : Wed Jun 10 06:10:57 2020

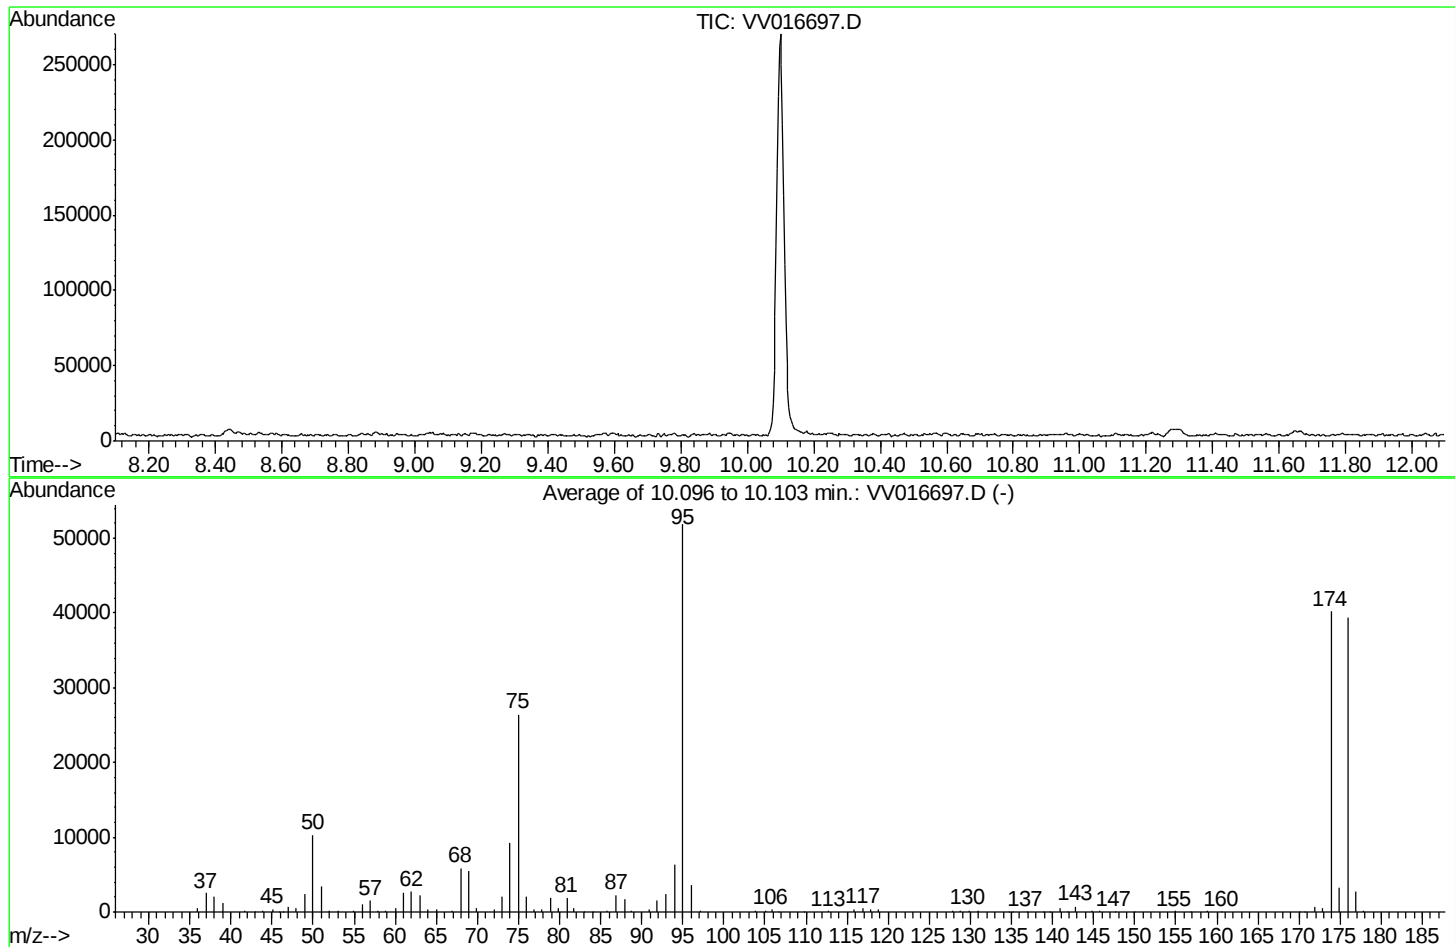

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	10290	PASS
75	95	30	80	50.9	26380	PASS
95	95	100	100	100.0	51874	PASS
96	95	5	9	6.9	3603	PASS
173	174	0.00	2	1.5	590	PASS
174	95	50	120	77.6	40245	PASS
175	174	5	9	8.1	3252	PASS
176	174	95	101	97.8	39368	PASS
177	176	5	9	6.9	2735	PASS

m/z	Abundance
36.00	680.0
37.00	2732.0
38.00	2290.0
39.00	1212.0
40.00	450.0
41.80	157.0
42.90	200.0
44.00	619.0
45.10	565.0
46.90	821.0
48.00	493.0
49.00	2628.0
50.00	10694.0
51.00	3248.0
52.00	203.0
53.00	134.0
54.90	216.0
55.20	195.0
55.90	1047.0
57.00	1638.0
58.00	144.0
58.70	114.0
60.00	611.0
61.00	2581.0
62.00	2862.0
63.00	2245.0
64.00	369.0
65.00	469.0
66.90	275.0
68.00	6005.0
69.00	5382.0
70.00	647.0
72.10	319.0
72.90	2219.0
74.00	9614.0
75.00	26144.0
76.00	2223.0
76.90	438.0
77.70	323.0
78.90	1867.0
79.90	538.0
80.90	1960.0
81.70	517.0
85.80	172.0
86.90	2321.0
88.00	1668.0
88.70	193.0
90.80	281.0
91.90	1671.0
93.00	2523.0
94.00	6716.0
95.00	52640.0
96.00	3702.0
97.10	217.0
103.80	233.0
105.10	129.0
105.80	240.0
106.70	118.0
112.70	143.0
115.90	263.0
116.90	427.0
117.80	312.0
118.80	351.0
127.80	197.0
128.80	237.0
129.80	261.0
131.00	133.0
135.10	136.0
136.80	150.0
140.90	484.0
141.80	116.0
142.80	807.0
144.70	194.0
145.80	147.0
147.60	115.0
150.00	121.0
154.90	129.0
160.60	108.0
170.70	118.0
171.90	703.0
173.00	592.0
173.90	39904.0
174.90	3240.0
175.90	38760.0
176.90	2701.0
177.80	147.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
36.00	738.0
37.00	2783.0
38.00	2216.0
39.00	1330.0
40.00	388.0
41.70	175.0
42.90	234.0
44.00	586.0
45.10	541.0
45.90	101.0
46.30	133.0
46.90	785.0
47.90	443.0
49.00	2507.0
50.00	10564.0
51.00	3571.0
51.90	240.0
53.00	121.0
54.00	135.0
54.90	235.0
56.00	996.0
57.00	1613.0
57.90	138.0
58.80	118.0
60.00	594.0
61.00	2619.0
62.00	2758.0
63.00	2268.0
64.00	400.0
65.00	416.0
66.90	295.0
68.00	6124.0
69.00	5773.0
69.90	641.0
72.10	331.0
72.90	2385.0
74.00	9650.0
75.00	27512.0
76.00	2172.0
76.80	439.0
77.80	282.0
78.90	1885.0
79.80	551.0
80.90	2037.0
81.80	496.0
85.80	180.0
86.90	2414.0
87.90	1827.0
88.70	290.0
90.90	305.0
91.90	1602.0
93.00	2468.0
94.00	6545.0
95.00	53888.0
96.00	3785.0
97.10	261.0
103.80	258.0
105.00	146.0
105.80	283.0
106.70	125.0
112.80	146.0
115.80	302.0
116.90	473.0
117.80	334.0
118.80	415.0
127.70	244.0
128.80	242.0
129.80	264.0
131.00	146.0
134.70	106.0
136.80	112.0
138.90	112.0
139.60	124.0
140.90	556.0
141.90	103.0
142.80	766.0
144.70	175.0
145.70	167.0
147.60	110.0
150.00	102.0
154.90	178.0
156.80	128.0
158.90	119.0
170.70	110.0
171.90	669.0
172.80	581.0
173.90	41656.0
174.90	3396.0
175.90	40632.0
176.90	2853.0
177.80	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.20	111.0
36.00	704.0
37.00	2539.0
38.00	2053.0
39.00	1239.0
40.00	359.0
41.70	213.0
42.90	253.0
43.90	585.0
45.00	490.0
45.90	121.0
46.90	666.0
47.90	392.0
49.00	2176.0
50.00	9614.0
51.00	3392.0
51.80	249.0
53.10	120.0
54.00	160.0
54.90	231.0
56.00	906.0
57.00	1363.0
57.90	175.0
58.80	146.0
60.00	536.0
61.00	2486.0
62.00	2386.0
63.00	1982.0
64.00	367.0
65.00	361.0
67.00	217.0
68.00	5413.0
69.00	5511.0
70.00	519.0
72.00	331.0
73.00	2393.0
74.00	8607.0
75.00	25832.0
76.00	1926.0
76.80	381.0
77.90	248.0
78.90	1720.0
79.80	531.0
80.90	1888.0
81.80	448.0
82.90	133.0
84.10	114.0
85.70	156.0
86.90	2159.0
87.90	1830.0
88.70	248.0
90.90	315.0
91.90	1389.0
93.00	2191.0
94.00	5781.0
95.00	49096.0
96.00	3322.0
97.10	210.0
103.80	281.0
105.00	151.0
105.80	338.0
109.70	108.0
112.80	125.0
115.80	306.0
117.00	527.0
117.80	292.0
118.80	416.0
127.70	251.0
128.70	179.0
129.80	221.0
130.90	134.0
134.70	130.0
138.90	103.0
139.60	139.0
140.90	600.0
142.80	696.0
144.80	157.0
145.80	138.0
154.90	171.0
156.90	138.0
158.70	170.0
170.10	103.0
171.90	466.0
172.80	597.0
173.90	39176.0
174.90	3122.0
175.90	38712.0
176.90	2653.0
177.80	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84

m/z	Abundance
35.00	126.0
35.80	176.0
36.90	156.0
37.90	144.0
38.50	126.0
39.30	176.0
39.90	488.0
41.30	183.0
42.80	185.0
43.90	350.0
45.10	153.0
47.10	130.0
47.70	113.0
49.70	138.0
53.90	115.0
55.20	103.0
57.40	128.0
59.20	127.0
61.50	103.0
67.20	114.0
73.10	193.0
74.30	111.0
75.20	116.0
98.70	100.0
235.40	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB84