




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026073.D
 Acq On : 09 Jun 2022 23:20
 Operator : SY/MD
 Sample : N3272-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B54

Manual IntegrationsAPPROVED

Quant Time: Jun 10 05:45:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

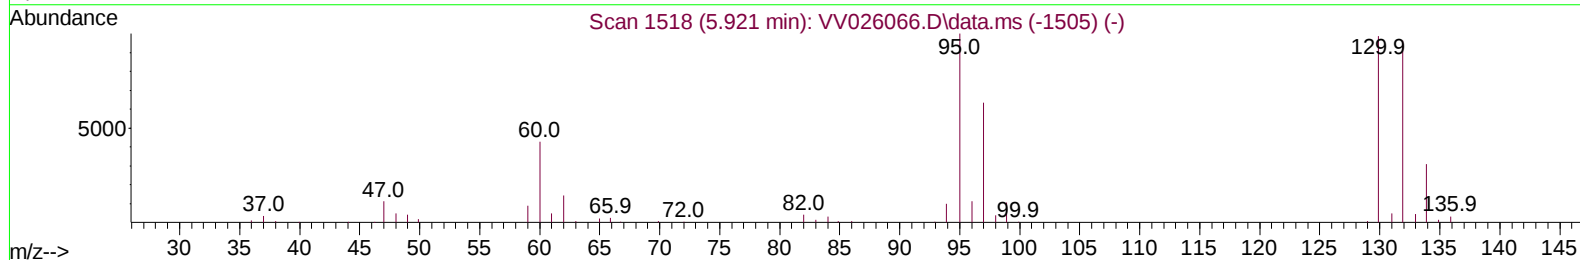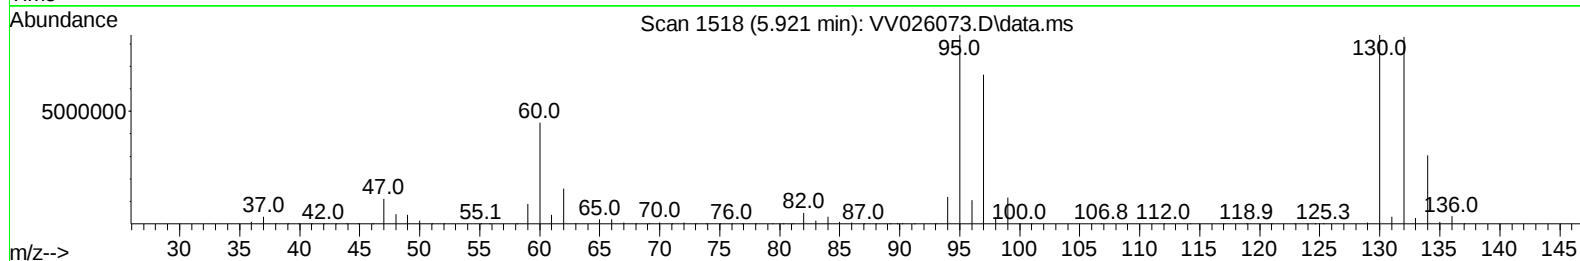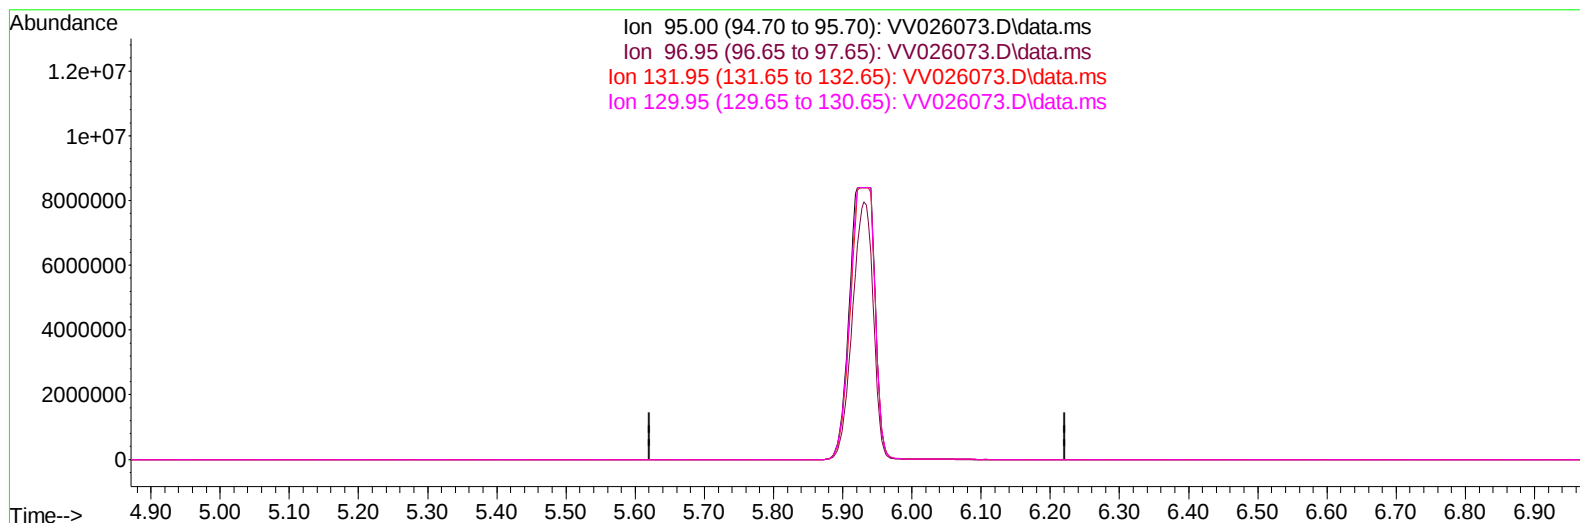

TIC: VV026073.D\data.ms

(34) Trichloroethene (T)

5.921min (-5.921) 0.00 ug/L

response 0

Ion	Exp%	Act%
95.00	100.00	0.00
96.95	62.80	0.00#
131.95	96.50	0.00#
129.95	99.60	0.00#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026073.D
 Acq On : 09 Jun 2022 23:20
 Operator : SY/MD
 Sample : N3272-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B54

Manual IntegrationsAPPROVED

Quant Time: Jun 10 05:45:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

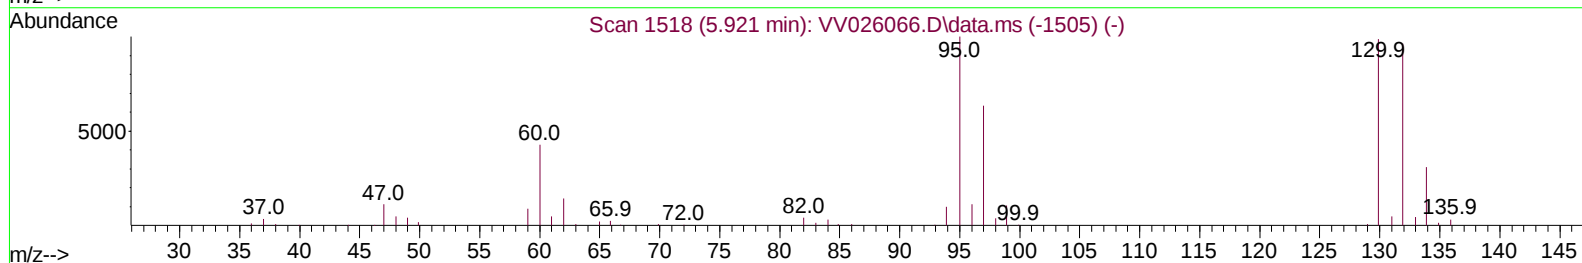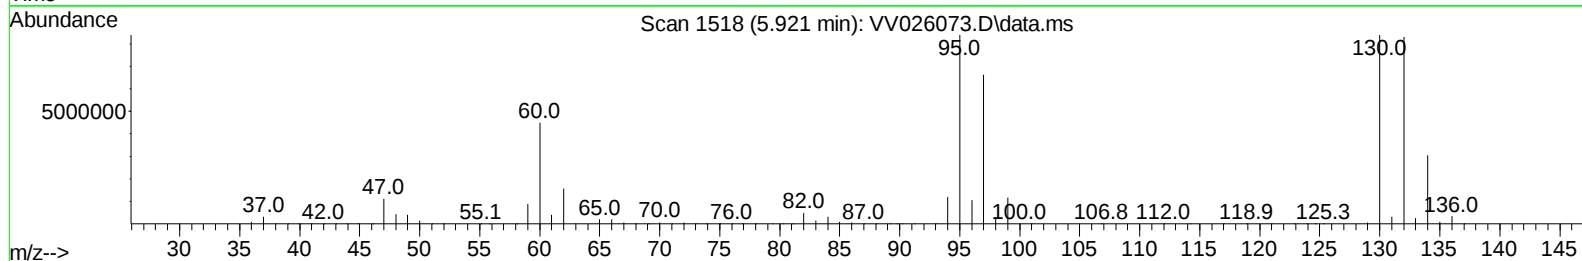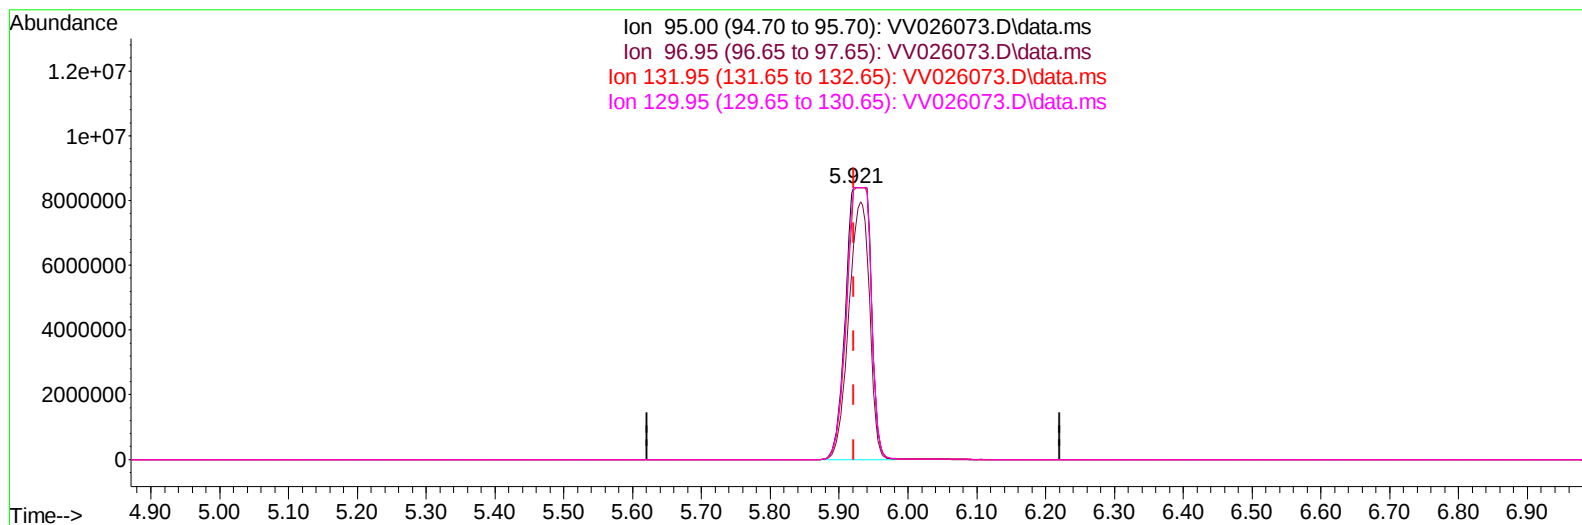

TIC: VV026073.D\data.ms

(34) Trichloroethene (T)

5.921min (+ 0.000) 1598.30 ug/L m

response 21410941

Ion	Exp%	Act%
95.00	100.00	100.00
96.95	62.80	79.00
131.95	96.50	99.05
129.95	99.60	100.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026073.D
 Acq On : 09 Jun 2022 23:20
 Operator : SY/MD
 Sample : N3272-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B54

Manual IntegrationsAPPROVED

Quant Time: Jun 10 05:45:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.625	114		171283	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117		163161	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152		66634	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.320	65		37694	3.749	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.000%	
7) Chloroethane-d5	1.581	69		46273	4.402	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	2.121	63		62847	2.706	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.200%#	
20) 2-Butanone-d5	3.918	46		85714	57.638	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.280%	
24) Chloroform-d	4.362	84		103637	4.863	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.200%	
26) 1,2-Dichloroethane-d4	5.043	65		46878	5.393	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.800%	
32) Benzene-d6	5.063	84		180667	4.582	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	6.079	67		62311	5.108	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%	
41) Toluene-d8	7.320	98		133089	3.820	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.400%	
43) trans-1,3-Dichloroprop...	7.632	79		14756	4.109	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%	
46) 2-Hexanone-d5	8.092	63		95997	60.745	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	121.480%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84		42644	5.185	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	103.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152		54002	5.297	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.000%	
Target Compounds							
						Qvalue	
9) Trichlorofluoromethane	1.767	101		1749892	69.641	ug/L	99
18) trans-1,2-Dichloroethene	2.780	96		2141	0.165	ug/L	88
22) cis-1,2-Dichloroethene	3.928	96		21757	1.699	ug/L	96
25) Chloroform	4.397	83		12316	0.508	ug/L	96
29) 1,1,1-Trichloroethane	4.619	97		2252	0.105	ug/L	97
31) Carbon tetrachloride	4.841	117		36464	2.074	ug/L	96
34) Trichloroethene	5.921	95		21410941m	1598.300	ug/L	
45) 1,1,2-Trichloroethane	7.850	97		2714	0.336	ug/L	90
47) Tetrachloroethene	7.982	164		5911577	570.099	ug/L	97
51) Chlorobenzene	8.886	112		15935	0.457	ug/L	100
52) Ethylbenzene	9.021	91		2073	0.037	ug/L	95
53) m,p-Xylene	9.143	106		3435	0.158	ug/L	97
63) 1,2,4-Trimethylbenzene	10.918	105		2627	0.075	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Manual IntegrationsAPPROVED

Quant Time: Jun 10 05:45:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 10 05:25:55 2022
Response via : Initial Calibration

