




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026089.D
 Acq On : 10 Jun 2022 05:41
 Operator : SY/MD
 Sample : N3272-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 07:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

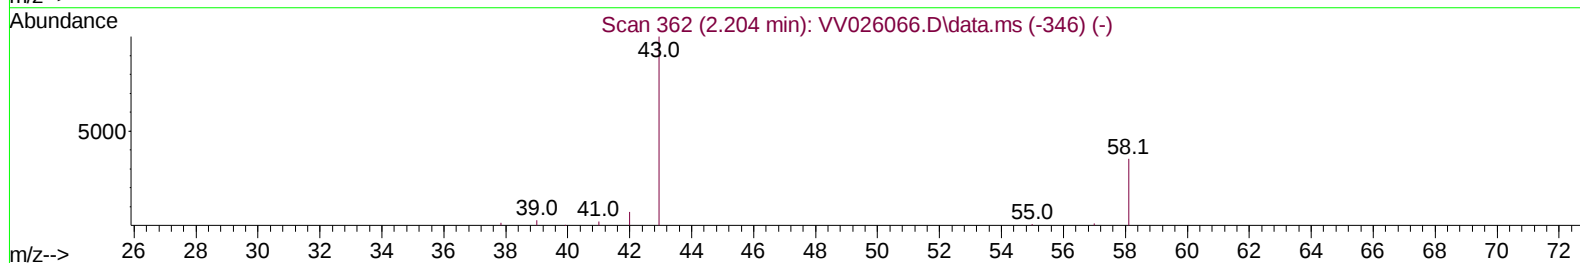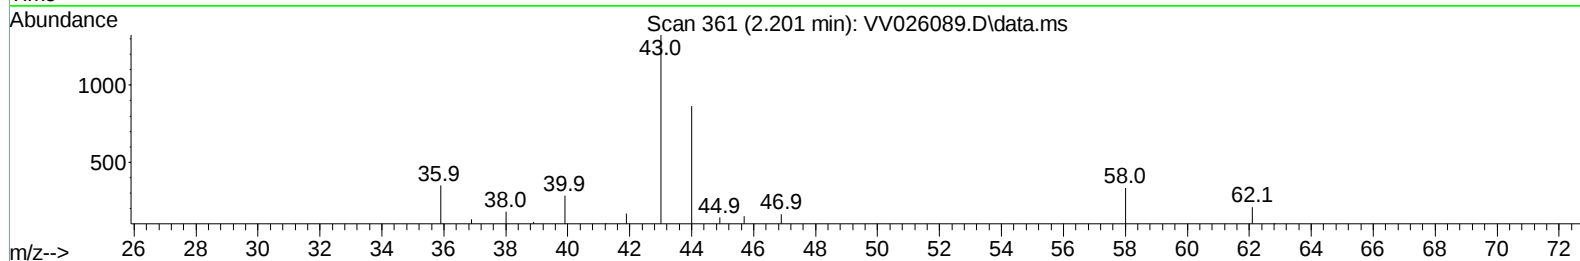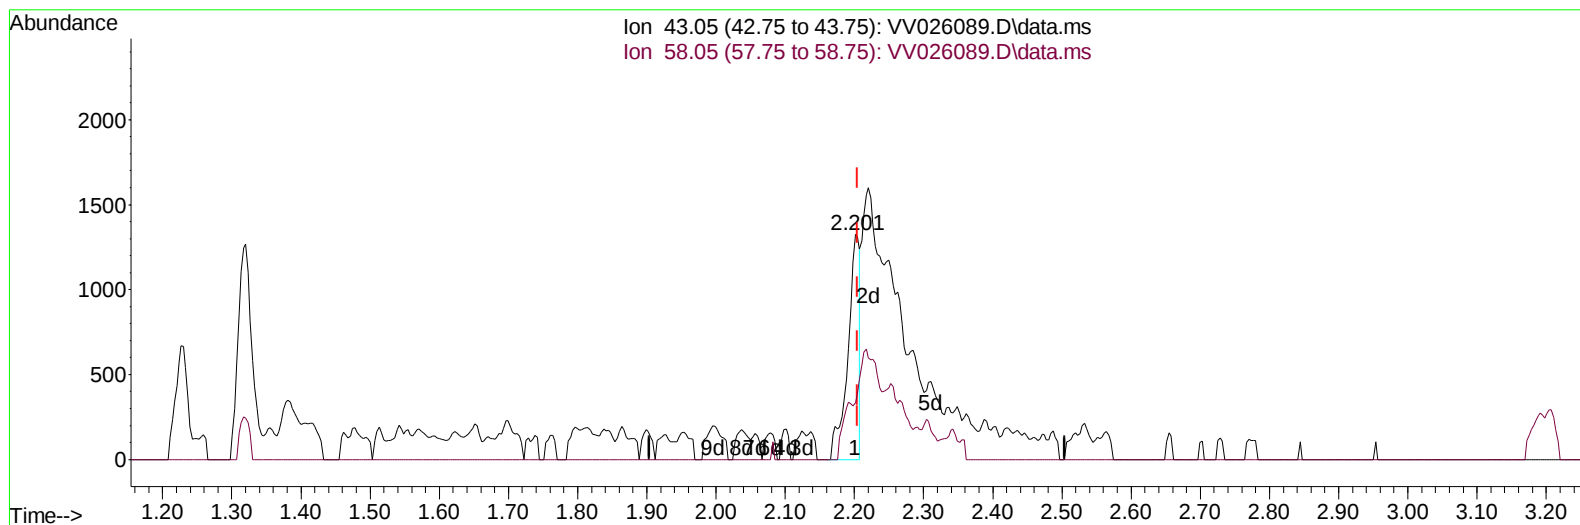

TIC: VV026089.D\data.ms

(13) Acetone (T)

2.201min (-0.003) 1.31 ug/L

response 1615

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	23.80	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026089.D
 Acq On : 10 Jun 2022 05:41
 Operator : SY/MD
 Sample : N3272-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 07:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

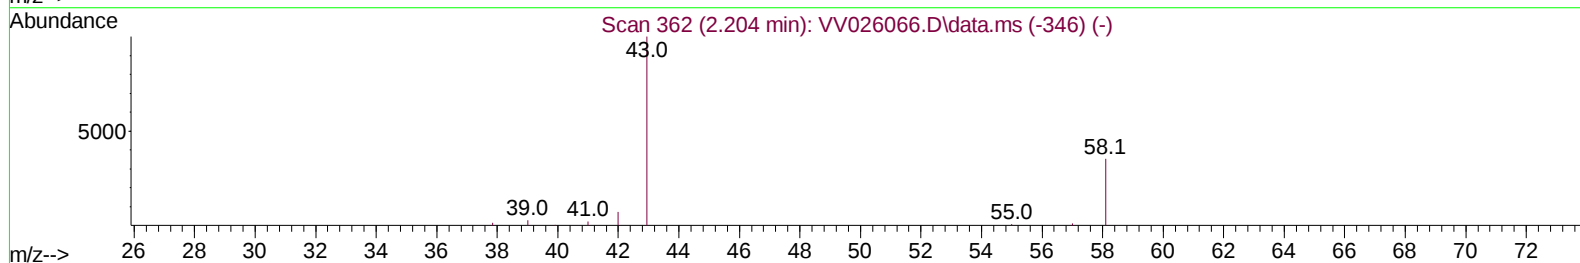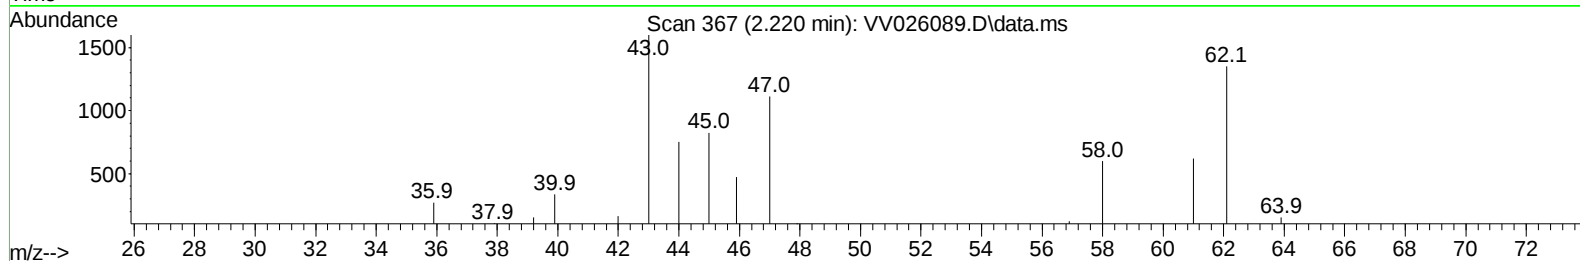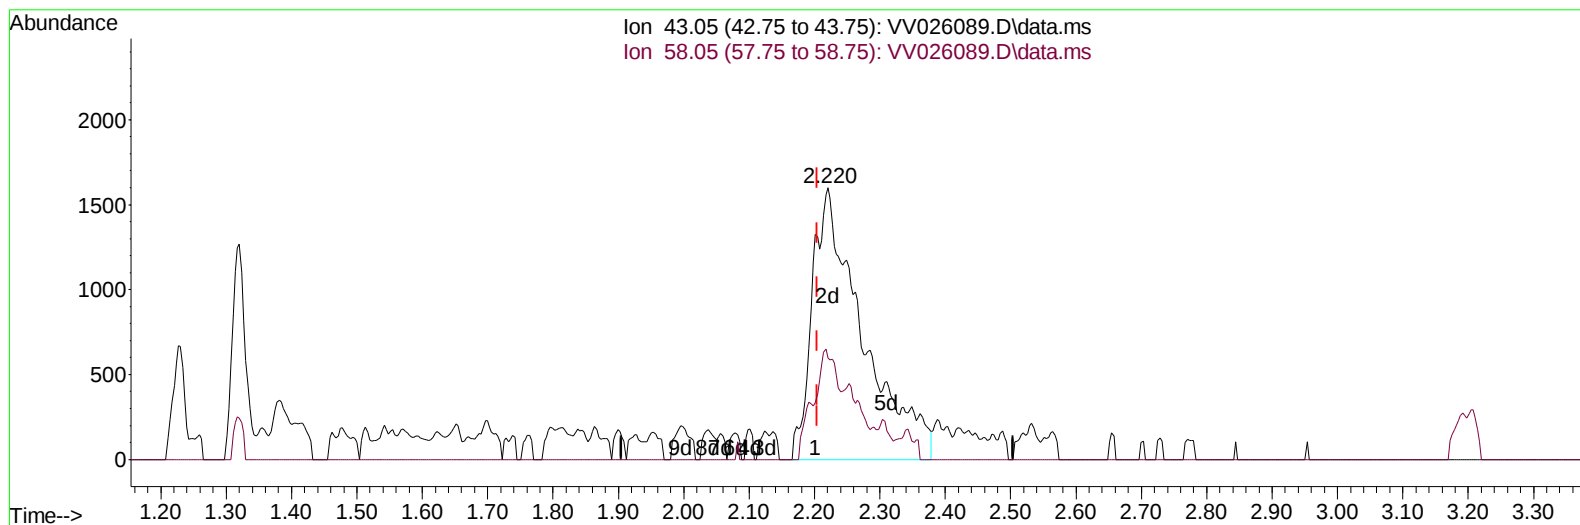

TIC: VV026089.D\data.ms

(13) Acetone (T)

2.220min (+ 0.016) 6.92 ug/L m

response 8497

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	23.80	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026089.D
 Acq On : 10 Jun 2022 05:41
 Operator : SY/MD
 Sample : N3272-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 07:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

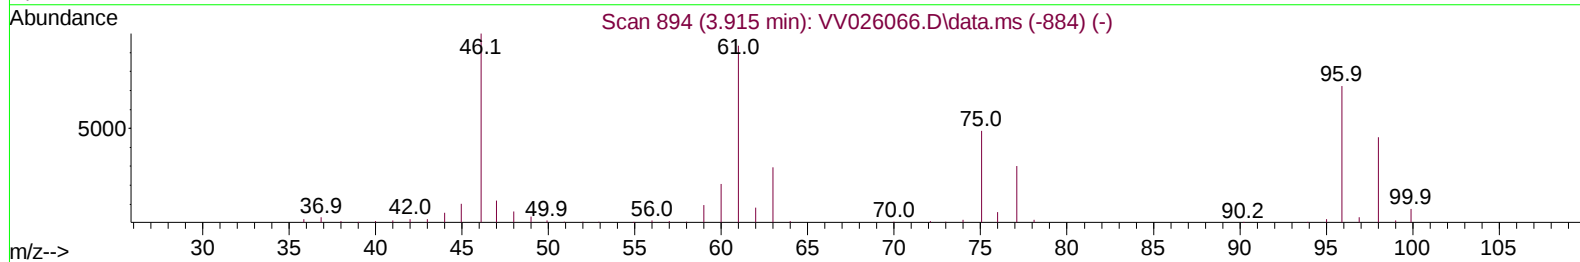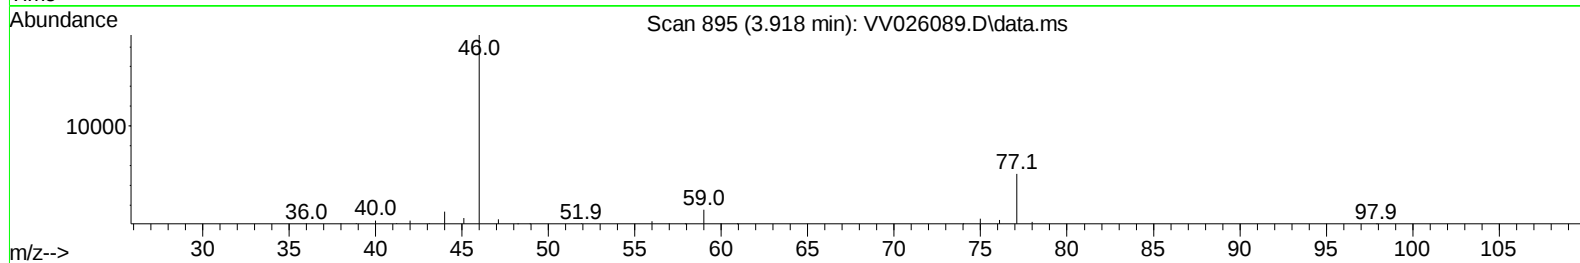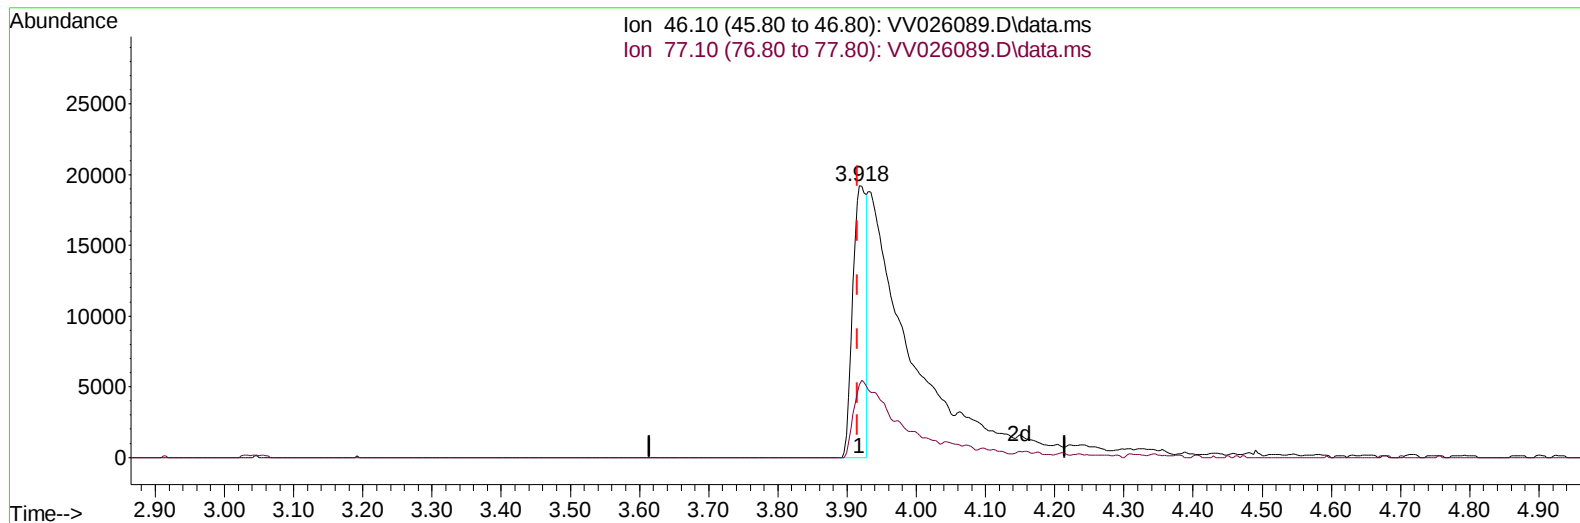

TIC: VV026089.D\data.ms

(20) 2-Butanone-d5 (S)

3.918min (+ 0.003) 17.07 ug/L

response 26287

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	26.10	87.02#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026089.D
 Acq On : 10 Jun 2022 05:41
 Operator : SY/MD
 Sample : N3272-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 07:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

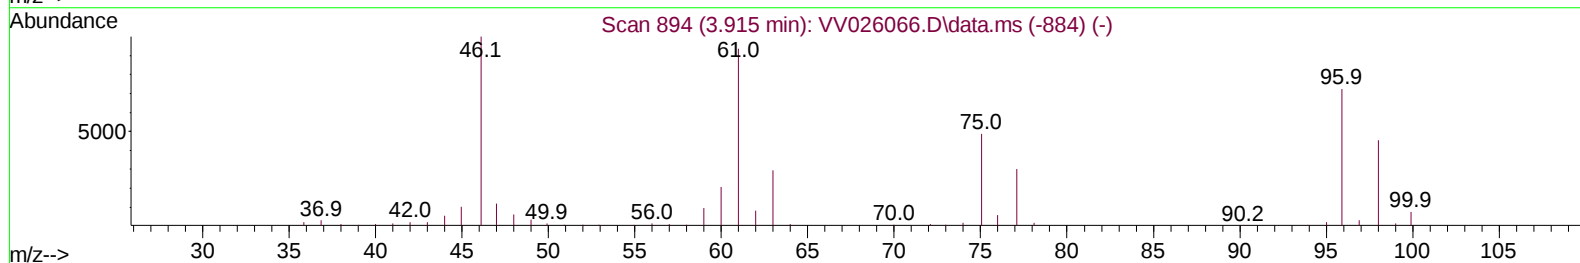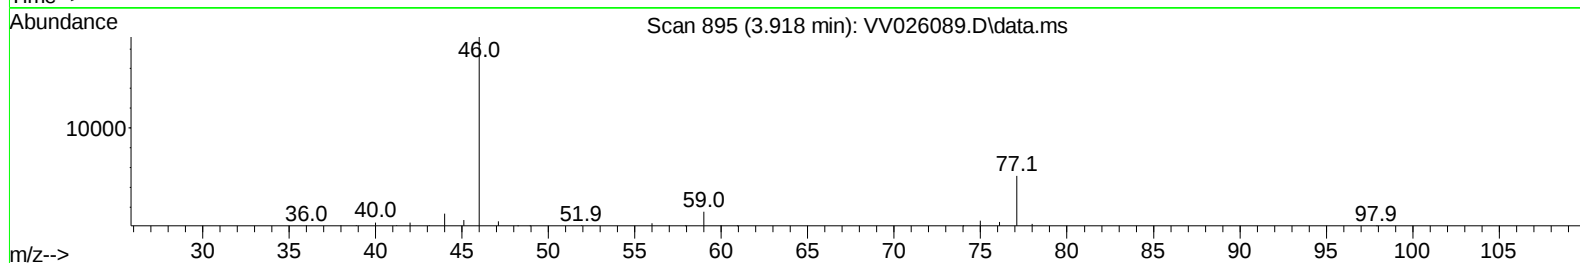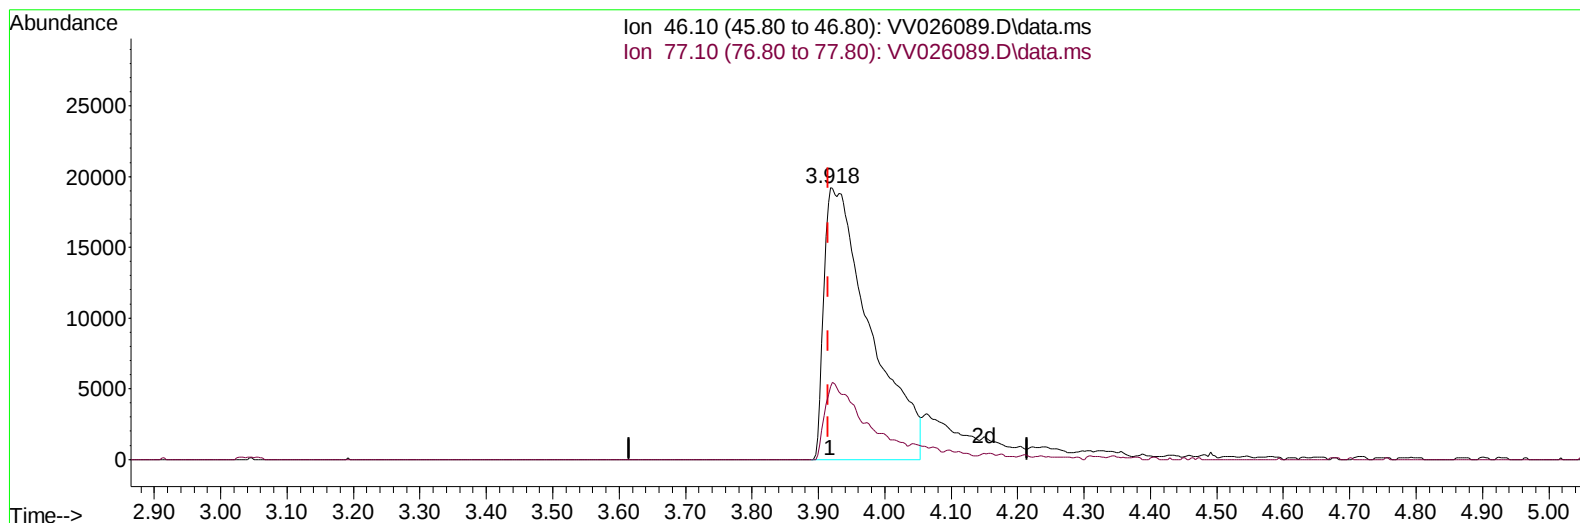

TIC: VV026089.D\data.ms

(20) 2-Butanone-d5 (S)

3.918min (+ 0.003) 60.05 ug/L m

response 92480

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	26.10	24.74
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026089.D
 Acq On : 10 Jun 2022 05:41
 Operator : SY/MD
 Sample : N3272-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 07:13:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
 Supervised By :Mahesh Dadoda 06/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	177387	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	172890	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	70486	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	38692	3.716	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	74.400%	
7) Chloroethane-d5	1.581	69	48269	4.434	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	88.600%	
11) 1,1-Dichloroethene-d2	2.121	63	63315	2.632	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	52.600%#	
20) 2-Butanone-d5	3.918	46	92480m	60.048	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130	Recovery	=	120.100%	
24) Chloroform-d	4.359	84	107080	4.852	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	97.000%	
26) 1,2-Dichloroethane-d4	5.043	65	44811	4.978	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	99.600%	
32) Benzene-d6	5.060	84	180441	4.319	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.400%	
36) 1,2-Dichloropropane-d6	6.076	67	64774	5.012	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	100.200%	
41) Toluene-d8	7.320	98	134852	3.653	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	73.000%	
43) trans-1,3-Dichloroprop...	7.629	79	13394	3.520	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	70.400%	
46) 2-Hexanone-d5	8.092	63	71217	42.529	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	85.060%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42284	4.852	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	97.000%	
66) 1,2-Dichlorobenzene-d4	11.622	152	52486	4.867	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	97.400%	
Target Compounds						
					Qvalue	
5) vinyl chloride	1.323	62	4648	0.228	ug/L	89
13) Acetone	2.220	43	8497m	6.918	ug/L	
14) Carbon disulfide	2.310	76	3394	0.083	ug/L #	93
34) Trichloroethene	5.921	95	30029	2.115	ug/L	98
47) Tetrachloroethene	7.982	164	1399	0.127	ug/L	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026089.D
Acq On : 10 Jun 2022 05:41
Operator : SY/MD
Sample : N3272-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B50

Manual IntegrationsAPPROVED

Quant Time: Jun 10 07:13:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 10 05:25:55 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 06/10/2022
Supervised By :Mahesh Dadoda 06/13/2022

