

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026047.D
 Acq On : 09 Jun 2022 11:36
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK364

Quant Time: Jun 10 02:50:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 02:49:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	250287	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	245609	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	103427	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.317	65	63919	4.350	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.000%	
7) Chloroethane-d5	1.577	69	73630	4.793	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	95.800%	
11) 1,1-Dichloroethene-d2	2.118	63	105287	3.102	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	62.000%	
20) 2-Butanone-d5	3.899	46	97791	45.002	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	90.000%	
24) Chloroform-d	4.352	84	157935	5.072	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.400%	
26) 1,2-Dichloroethane-d4	5.037	65	67945	5.350	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	107.000%	
32) Benzene-d6	5.053	84	284400	4.792	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.800%	
36) 1,2-Dichloropropane-d6	6.069	67	97257	5.297	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	106.000%	
41) Toluene-d8	7.317	98	216079	4.120	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.400%	
43) trans-1,3-Dichloroprop...	7.625	79	23223	4.296	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	86.000%	
46) 2-Hexanone-d5	8.088	63	119172	50.095	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.200%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	59946	4.842	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	84242	5.324	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.400%	
Target Compounds						
16) Methylene chloride	2.516	84	6532	0.326	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026047.D
Acq On : 09 Jun 2022 11:36
Operator : SY/MD
Sample : VV0609WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364


Quant Time: Jun 10 02:50:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 10 02:49:22 2022
Response via : Initial Calibration

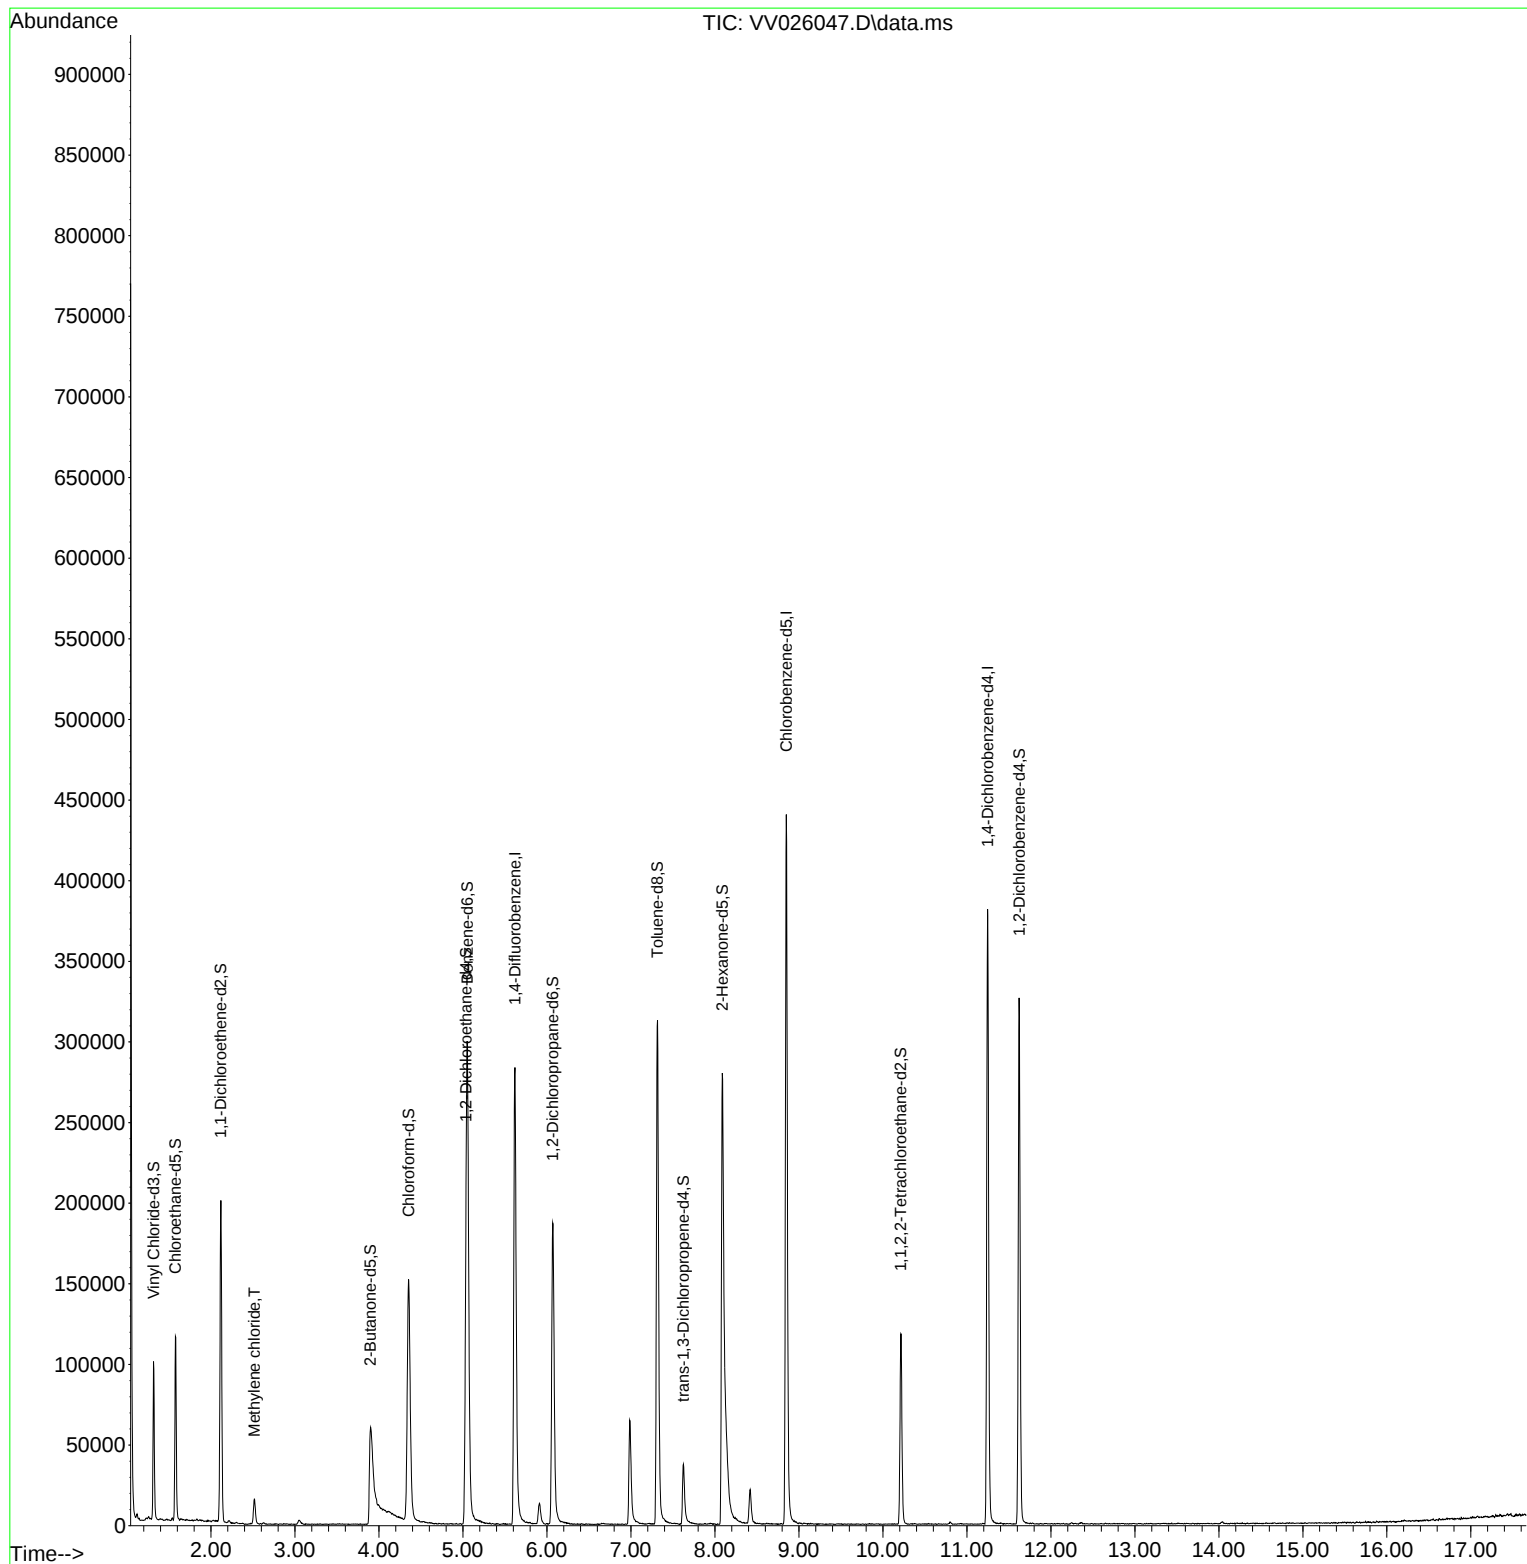

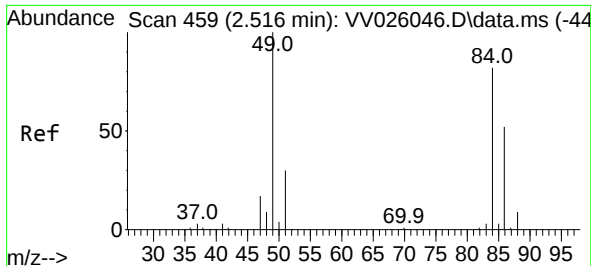

#16
Methylene chloride
Concen: 0.326 ug/L
RT: 2.516 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV026047.D
Acq: 09 Jun 2022 11:36

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

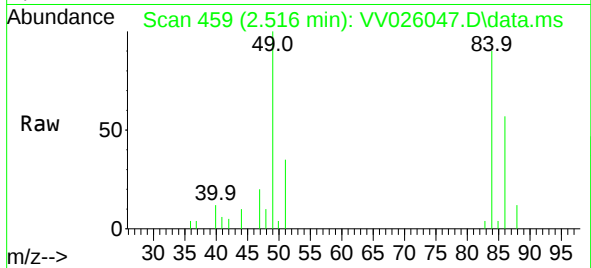

Tgt Ion: 84 Resp: 6532

Ion	Ratio	Lower	Upper
84	100		
86	62.9	45.6	84.6
49	110.8	82.9	153.9

