

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060922\
 Data File : VW026052.D
 Acq On : 09 Jun 2022 13:36
 Operator : SY/MD
 Sample : N3247-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS3

Quant Time: Jun 10 02:51:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 02:49:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	171223	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	168693	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69144	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	44625	4.440	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.800%	
7) Chloroethane-d5	1.581	69	50910	4.845	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	96.800%	
11) 1,1-Dichloroethene-d2	2.121	63	71114	3.063	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.200%	
20) 2-Butanone-d5	3.915	46	70267	47.268	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	94.540%	
24) Chloroform-d	4.362	84	109116	5.122	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.400%	
26) 1,2-Dichloroethane-d4	5.043	65	48153	5.542	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	110.800%	
32) Benzene-d6	5.059	84	191822	4.706	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.200%	
36) 1,2-Dichloropropane-d6	6.075	67	66221	5.251	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.000%	
41) Toluene-d8	7.320	98	145306	4.034	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	80.600%	
43) trans-1,3-Dichloroprop...	7.632	79	16635	4.480	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	89.600%	
46) 2-Hexanone-d5	8.091	63	77627	47.510	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.020%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	41594	4.892	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	58095	5.492	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.800%	
Target Compounds						
					Qvalue	
13) Acetone	2.198	43	11227	9.470	ug/L	85
25) Chloroform	4.397	83	6542	0.270	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026052.D
Acq On : 09 Jun 2022 13:36
Operator : SY/MD
Sample : N3247-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS3

Quant Time: Jun 10 02:51:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 10 02:49:22 2022
Response via : Initial Calibration

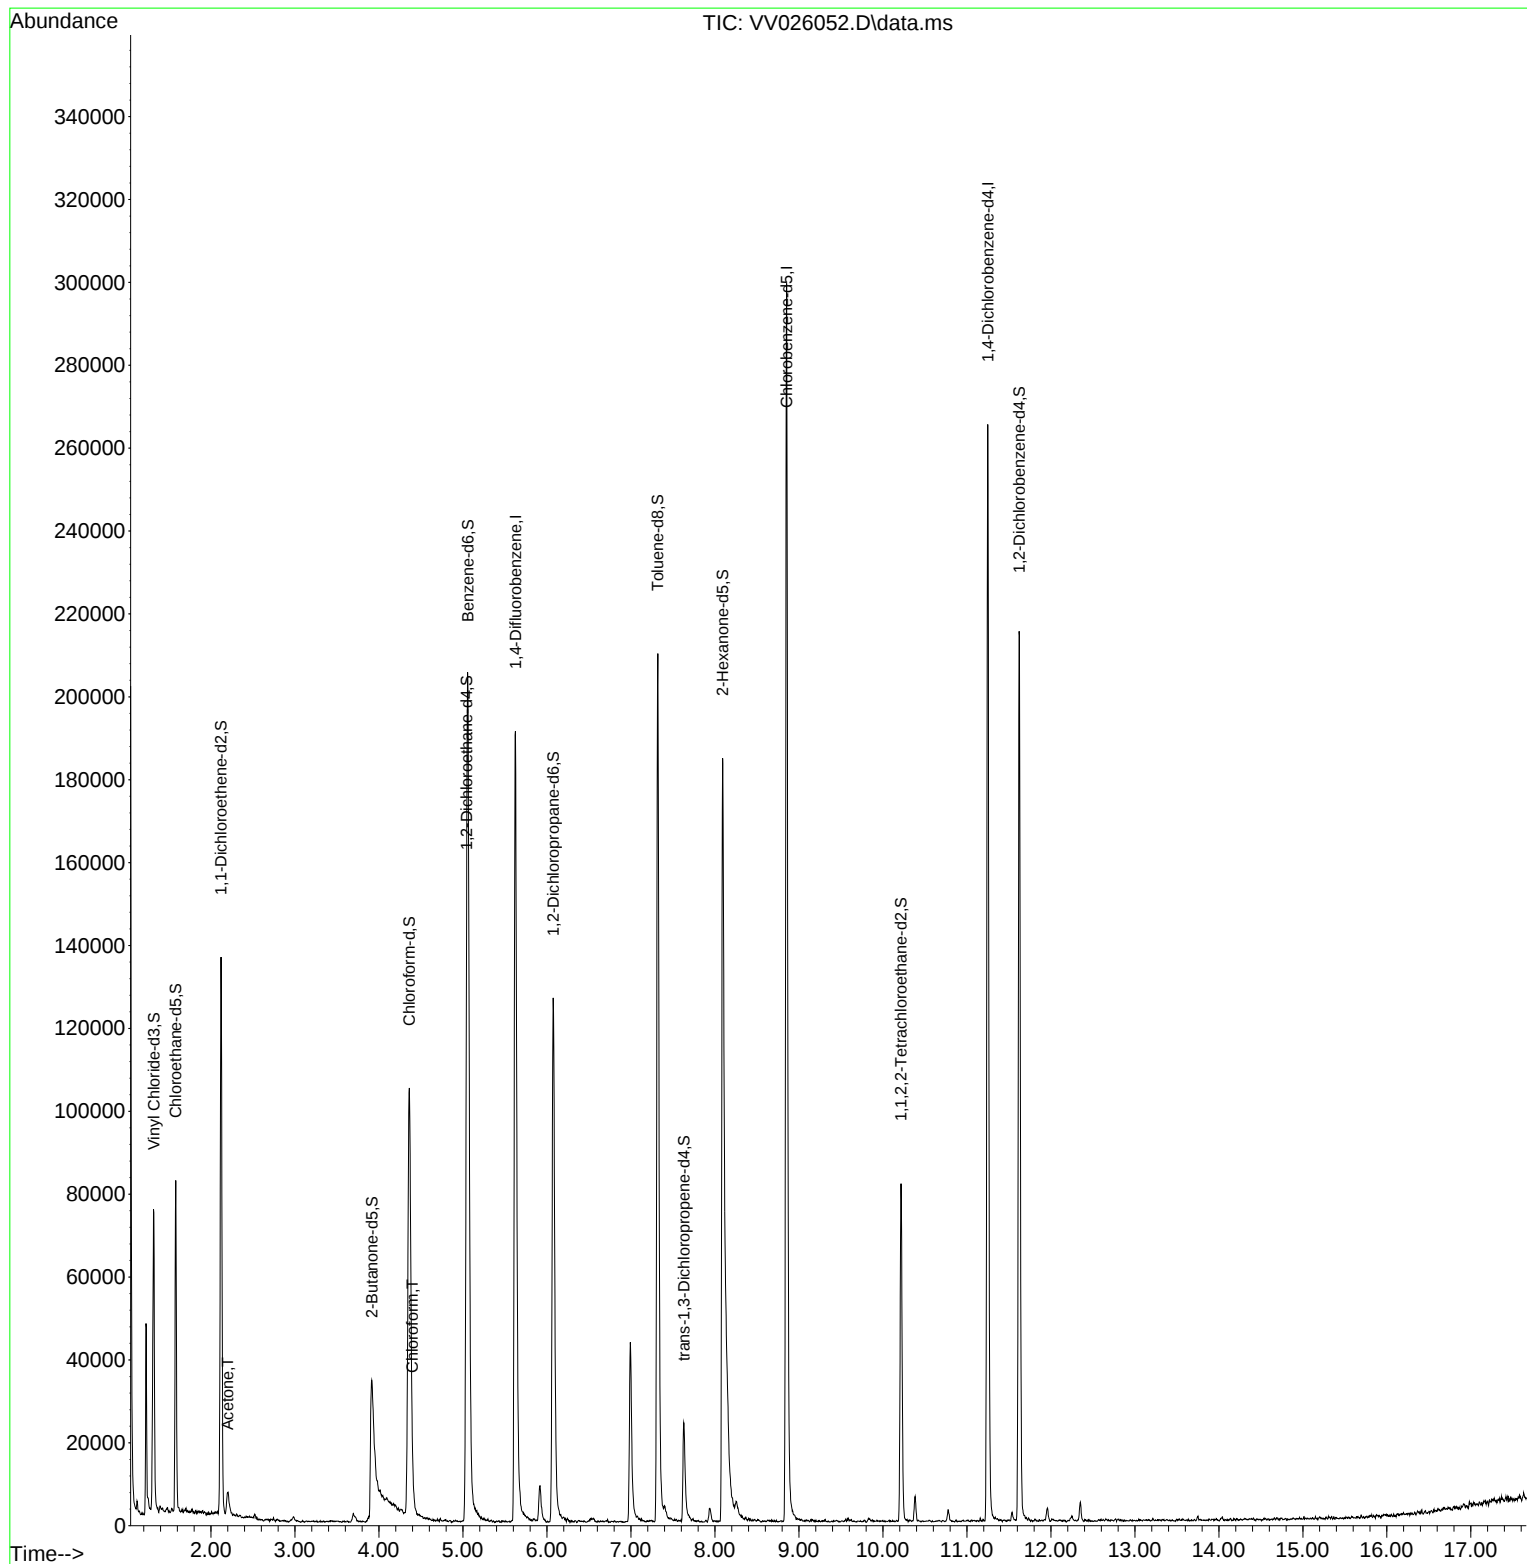

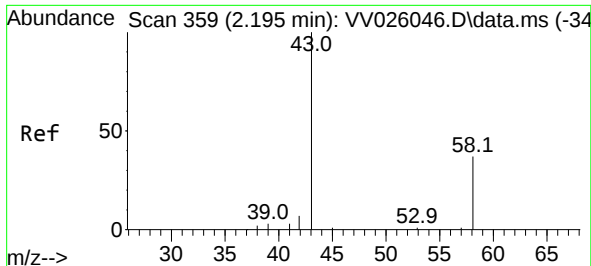

#13

Acetone

Concen: 9.470 ug/L

RT: 2.198 min Scan# 3

Delta R.T. 0.003 min

Lab File: VV026052.D

Acq: 09 Jun 2022 13:36

Instrument :

MSVOA_V

ClientSampleId :





EXYS3

Tgt Ion: 43 Resp: 11227

Ion Ratio Lower Upper

43 100

58 31.4 0.0 47.6

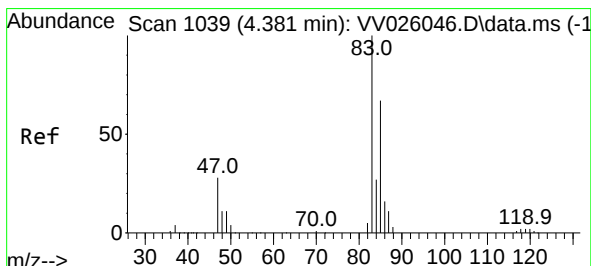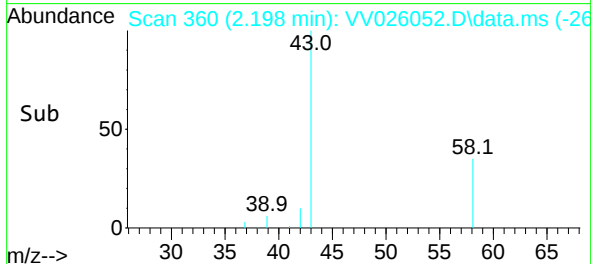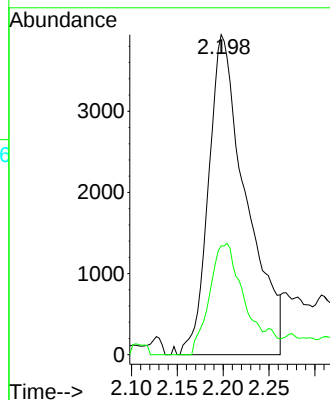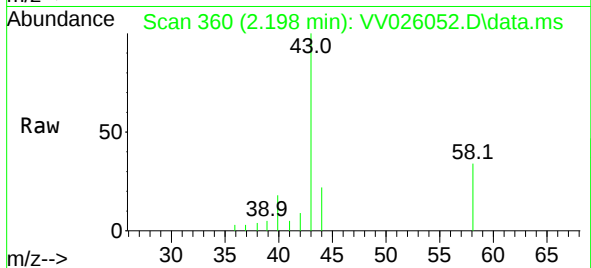

#25

Chloroform

Concen: 0.270 ug/L

RT: 4.397 min Scan# 1044

Delta R.T. 0.016 min

Lab File: VV026052.D

Acq: 09 Jun 2022 13:36

Tgt Ion: 83 Resp: 6542

Ion Ratio Lower Upper

83 100

85 57.6 45.2 84.0

