

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060922\
 Data File : VW026061.D
 Acq On : 09 Jun 2022 17:45
 Operator : SY/MD
 Sample : N3272-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B44

Quant Time: Jun 10 02:53:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 02:49:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	201496	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	199270	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	80250	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	44598	3.770	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.400%
7) Chloroethane-d5	1.581	69	54079	4.373	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.400%
11) 1,1-Dichloroethene-d2	2.121	63	73149	2.677	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.600%#
20) 2-Butanone-d5	3.908	46	101618	58.087	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.180%
24) Chloroform-d	4.362	84	122162	4.873	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.400%
26) 1,2-Dichloroethane-d4	5.043	65	53864	5.268	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.400%
32) Benzene-d6	5.059	84	206150	4.281	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.600%
36) 1,2-Dichloropropane-d6	6.076	67	72849	4.890	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.800%
41) Toluene-d8	7.320	98	158416	3.723	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.400%
43) trans-1,3-Dichloroprop...	7.629	79	18471	4.211	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.200%
46) 2-Hexanone-d5	8.092	63	93540	48.465	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.920%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	49742	4.952	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	63751	5.192	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.800%
Target Compounds						Qvalue
47) Tetrachloroethene	7.985	164	587	0.046	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026061.D
Acq On : 09 Jun 2022 17:45
Operator : SY/MD
Sample : N3272-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B44


Quant Time: Jun 10 02:53:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 10 02:49:22 2022
Response via : Initial Calibration

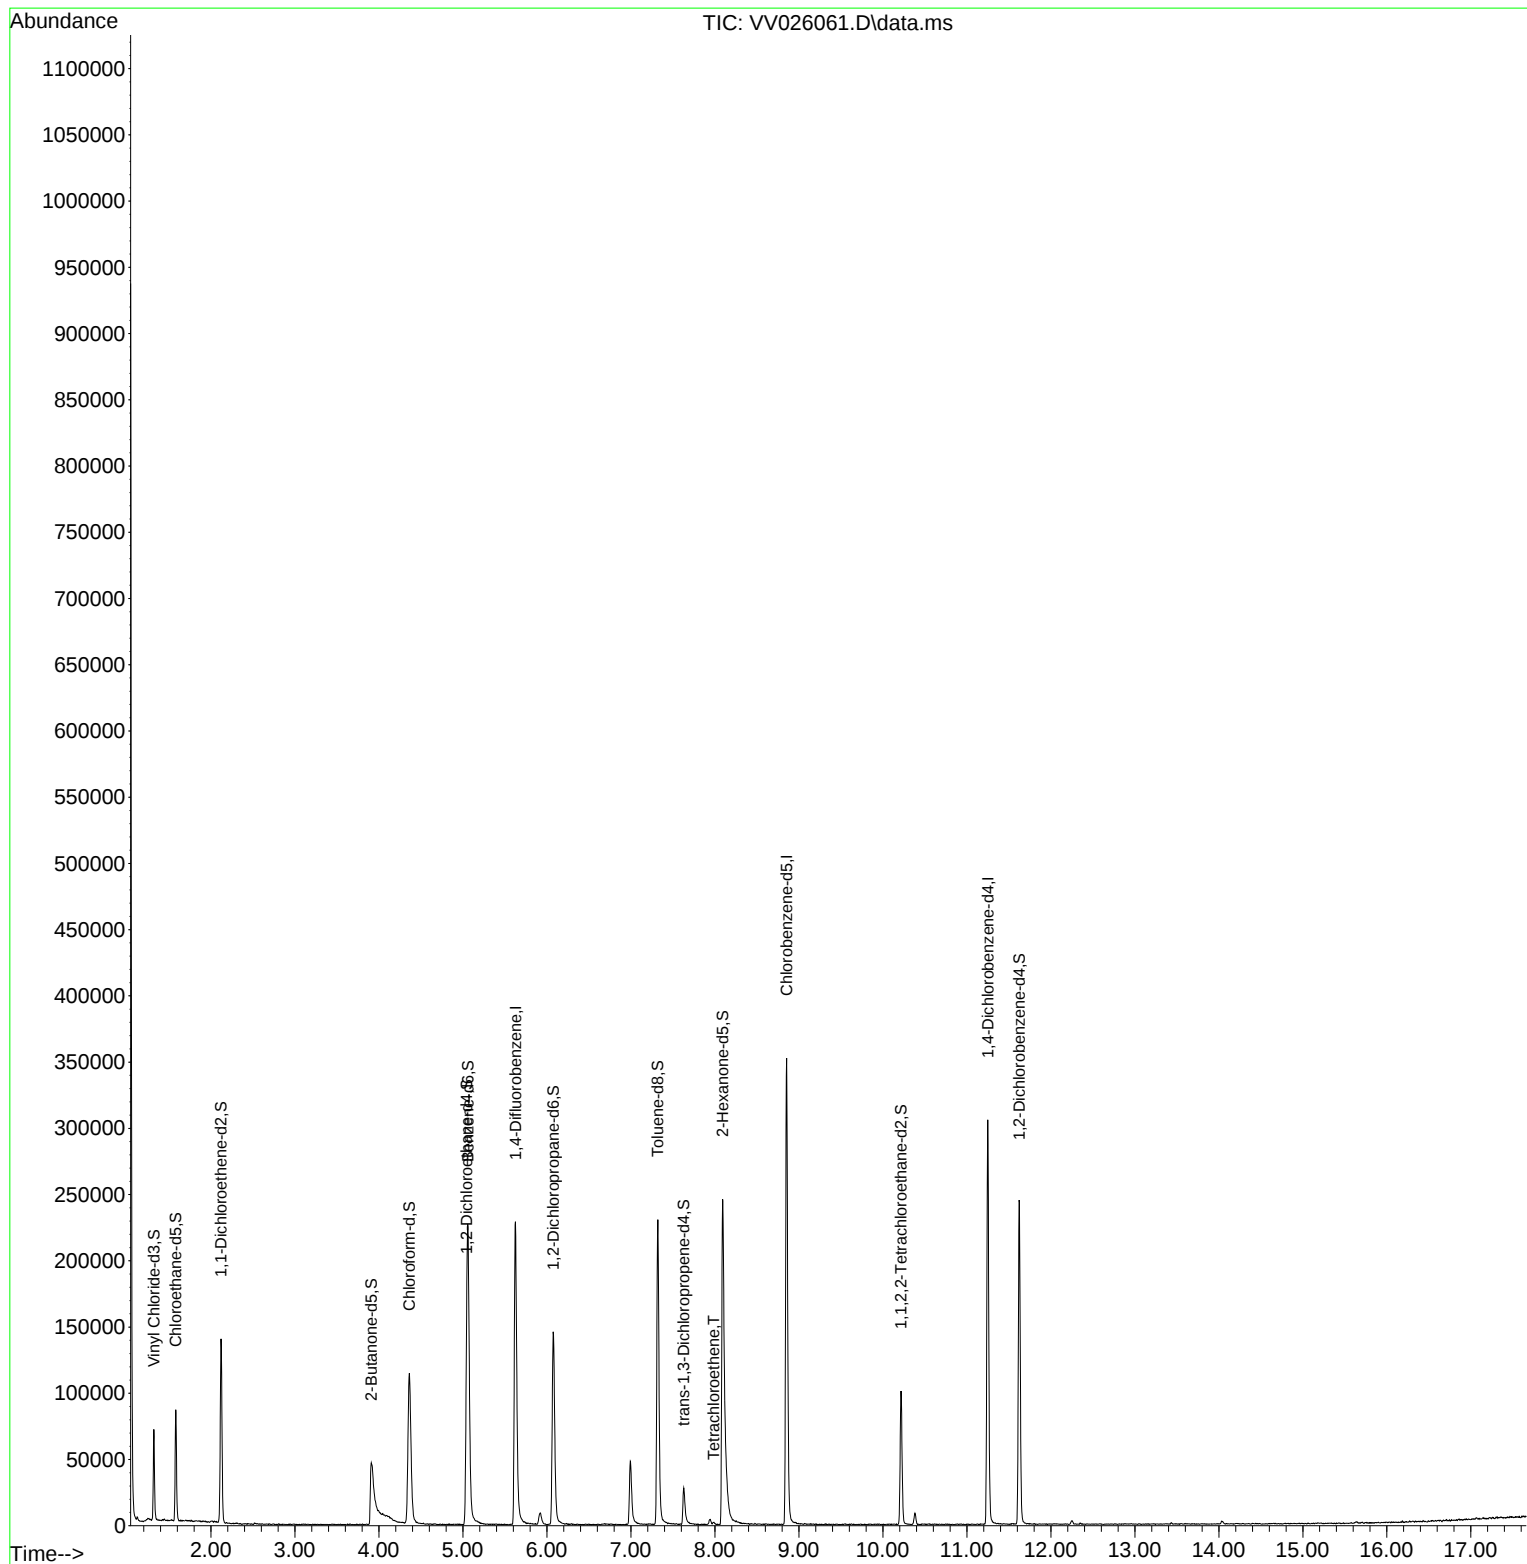

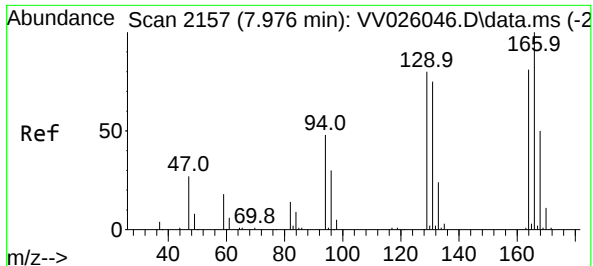

#47
 Tetrachloroethene
 Concen: 0.046 ug/L
 RT: 7.985 min Scan# 21
 Delta R.T. 0.010 min
 Lab File: VV026061.D
 Acq: 09 Jun 2022 17:45

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B44

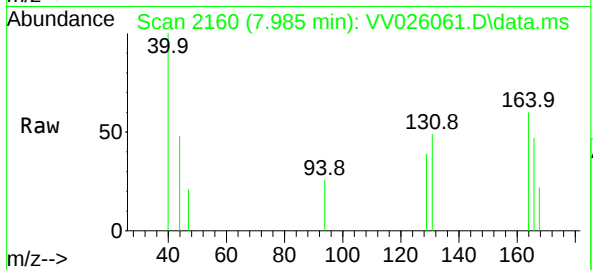

Tgt Ion:	164	Resp:	587
Ion	Ratio	Lower	Upper
164	100		
129	65.3	68.3	126.9#
131	80.7	66.5	123.5
166	77.9	88.1	163.7#

