

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060922\
 Data File : VW026071.D
 Acq On : 09 Jun 2022 22:32
 Operator : SY/MD
 Sample : N3272-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B52

Quant Time: Jun 10 05:44:47 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 10 05:25:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.625	114	176146	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	170560	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	69676	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.320	65	38173	3.692	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.800%	
7) Chloroethane-d5	1.584	69	46478	4.299	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	86.000%	
11) 1,1-Dichloroethene-d2	2.124	63	62687	2.625	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	52.400%#	
20) 2-Butanone-d5	3.915	46	67166	43.919	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	87.840%	
24) Chloroform-d	4.365	84	104286	4.759	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.200%	
26) 1,2-Dichloroethane-d4	5.043	65	45588	5.100	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.000%	
32) Benzene-d6	5.059	84	179595	4.358	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.200%	
36) 1,2-Dichloropropane-d6	6.075	67	63266	4.962	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	99.200%	
41) Toluene-d8	7.320	98	135582	3.723	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.400%	
43) trans-1,3-Dichloroprop...	7.628	79	14617	3.894	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	77.800%	
46) 2-Hexanone-d5	8.091	63	63684	38.550	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	77.100%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	42234	4.913	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152	53292	4.999	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	100.000%	
Target Compounds						Qvalue
34) Trichloroethene	5.921	95	45522	3.251	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026071.D
Acq On : 09 Jun 2022 22:32
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Time: Jun 10 05:44:47 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 10 05:25:55 2022
Response via : Initial Calibration

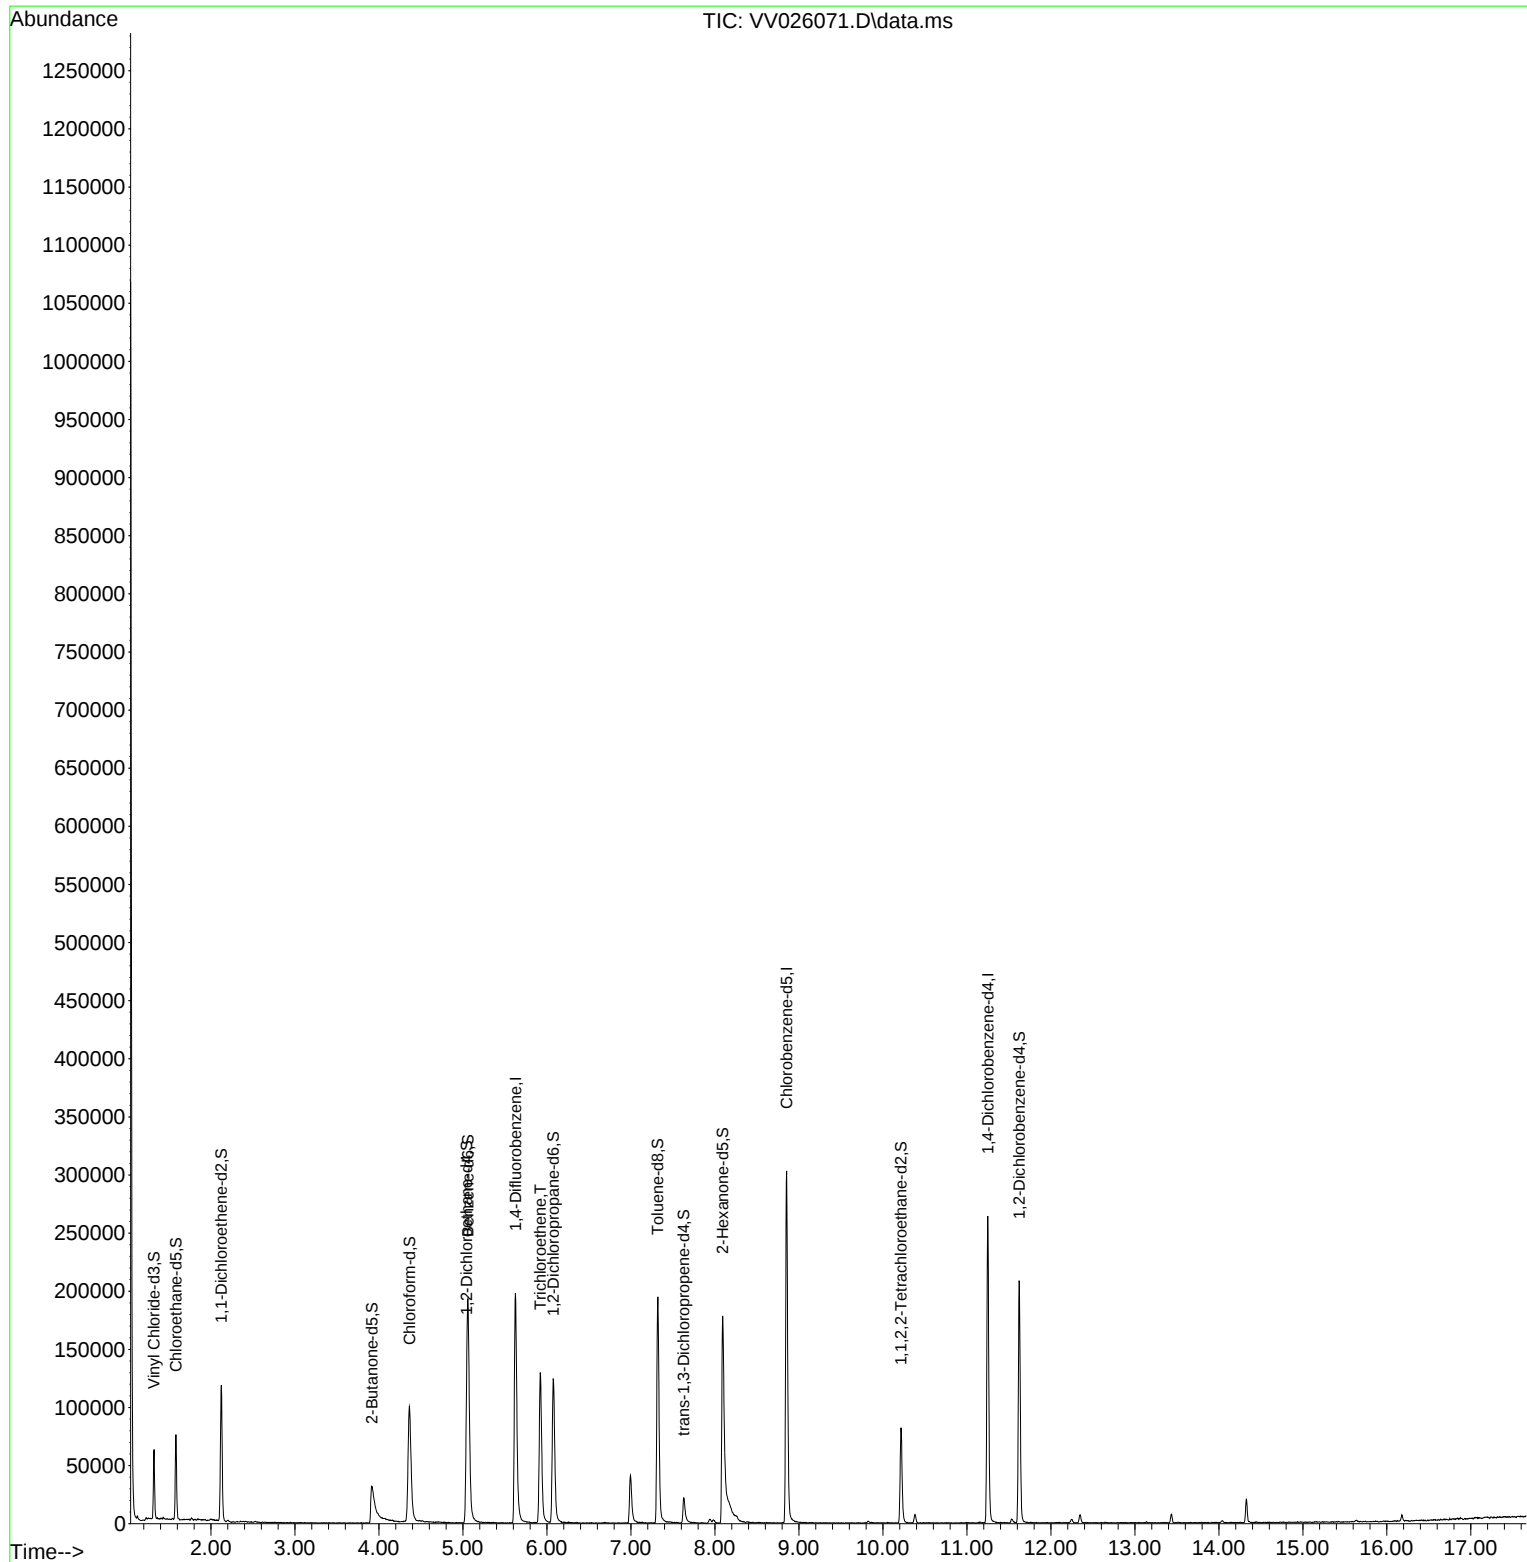

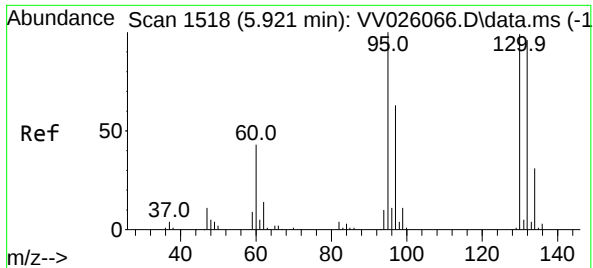

#34
 Trichloroethene
 Concen: 3.251 ug/L
 RT: 5.921 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VV026071.D
 Acq: 09 Jun 2022 22:32

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B52

Tgt Ion: 95 Resp: 45522

Ion	Ratio	Lower	Upper
95	100		
97	59.7	44.0	81.6
132	94.2	67.5	125.4
130	101.6	69.7	129.5

