

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026047.D
 Acq On : 09 Jun 2022 11:36
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK364

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	78	86	104	rVB	98153	105068	13.91%	1.633%
2	1.577	159	167	182	rVB	114092	133012	17.62%	2.067%
3	2.118	324	335	350	rVB	199563	287169	38.03%	4.463%
4	2.516	449	459	478	rVB2	15564	26928	3.57%	0.418%
5	3.902	876	890	917	rBV2	60279	214340	28.39%	3.331%
6	4.352	1015	1030	1068	rVB	149729	375851	49.78%	5.841%
7	5.050	1231	1247	1278	rBV2	299463	755097	100.00%	11.735%
8	5.619	1409	1424	1450	rBV	283334	582389	77.13%	9.051%
9	5.912	1504	1515	1538	rVB3	13059	28689	3.80%	0.446%
10	6.069	1549	1564	1591	rBV	186741	392056	51.92%	6.093%
11	6.986	1837	1849	1872	rBV2	64604	125059	16.56%	1.944%
12	7.317	1940	1952	1973	rBV	312411	558799	74.00%	8.684%
13	7.625	2039	2048	2067	rBV2	37053	69183	9.16%	1.075%
14	8.088	2181	2192	2238	rBV2	279746	717720	95.05%	11.154%
15	8.420	2285	2295	2307	rBV2	20838	37138	4.92%	0.577%
16	8.850	2417	2429	2458	rBV	440078	726190	96.17%	11.286%
17	10.214	2842	2853	2871	rBV	118040	191545	25.37%	2.977%
18	11.246	3164	3174	3199	rBV	381355	597886	79.18%	9.292%
19	11.622	3276	3291	3316	rBV	326316	510562	67.62%	7.935%




Sum of corrected areas: 6434681

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026047.D
Acq On : 09 Jun 2022 11:36
Operator : SY/MD
Sample : VV0609WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

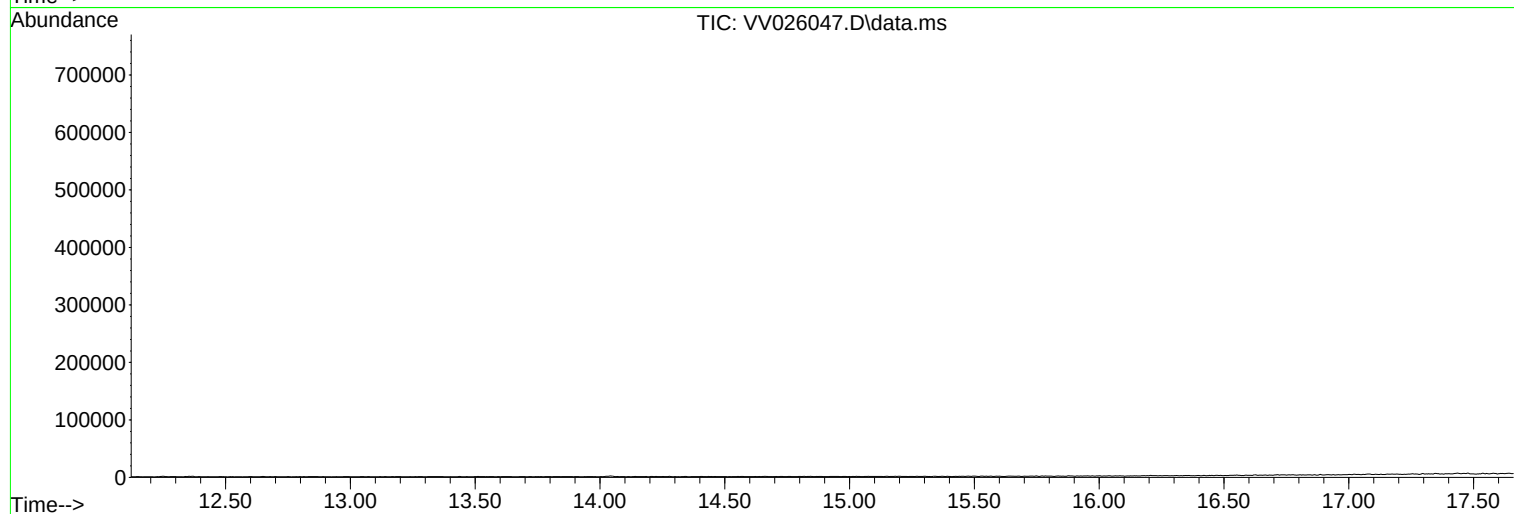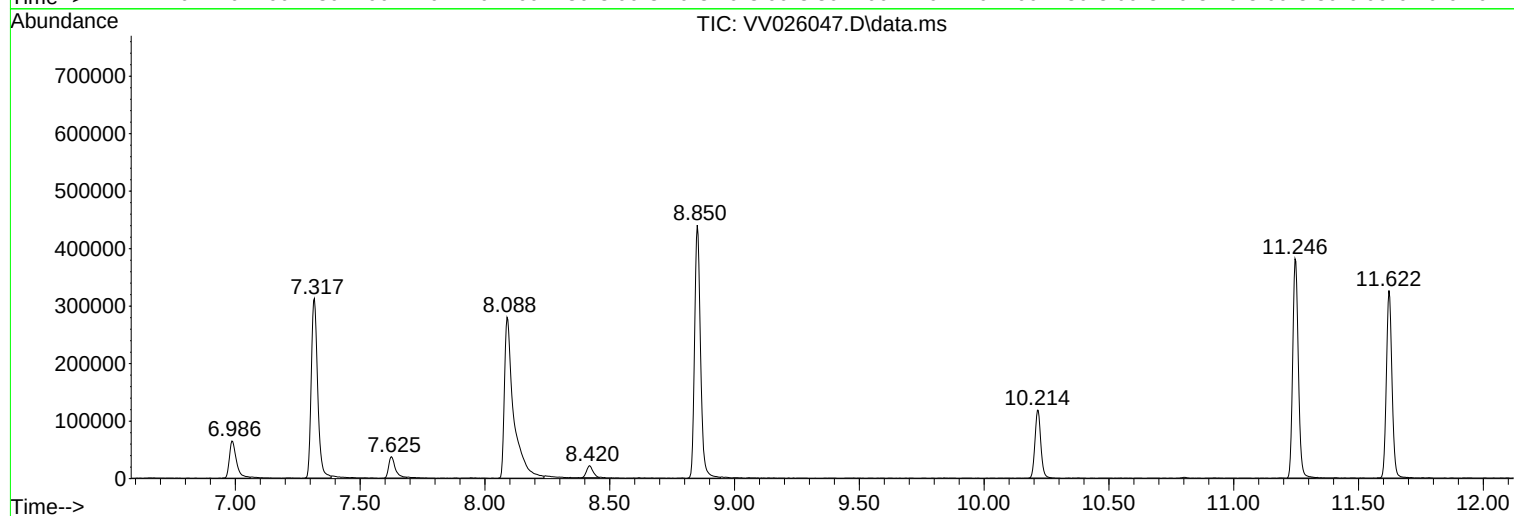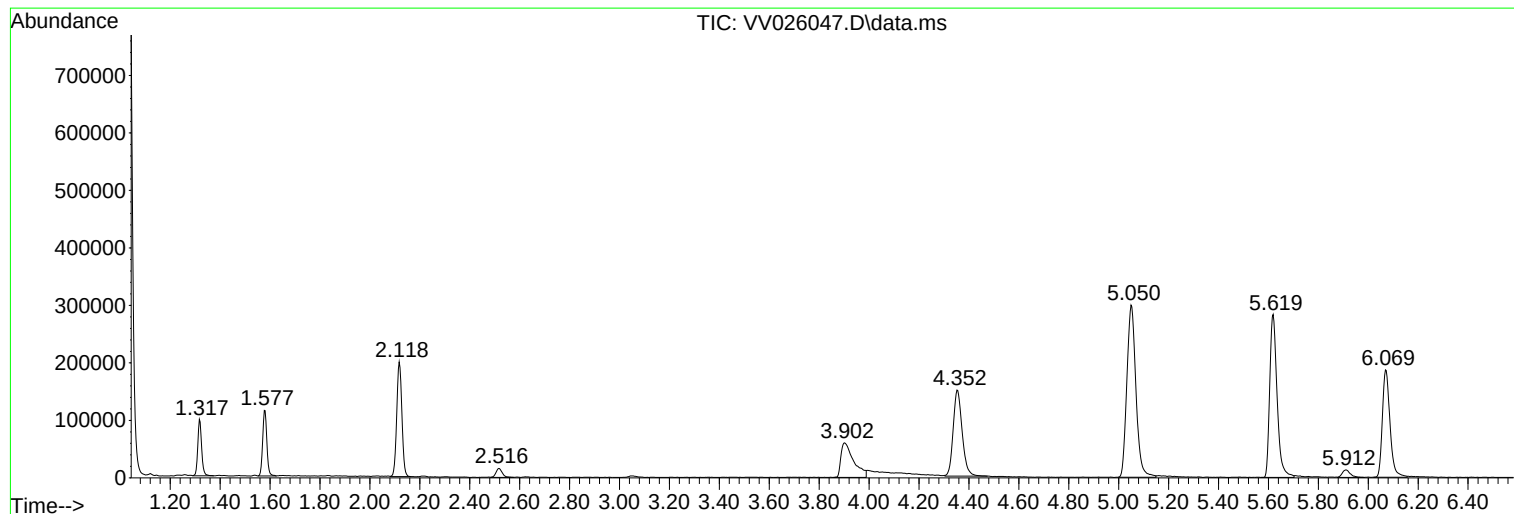

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026047.D
Acq On : 09 Jun 2022 11:36
Operator : SY/MD
Sample : VV0609WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026047.D
Acq On : 09 Jun 2022 11:36
Operator : SY/MD
Sample : VV0609WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK364

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc