

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026053.D
 Acq On : 09 Jun 2022 14:33
 Operator : SY/MD
 Sample : N3247-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.224	51	57	64	rBV	38555	35190	6.36%	0.737%
2	1.314	78	85	102	rVB	74438	79978	14.45%	1.675%
3	1.577	157	167	180	rBV	90019	102444	18.51%	2.145%
4	2.114	323	334	350	rVB	147786	211041	38.13%	4.419%
5	2.198	350	360	371	rBV	6515	15948	2.88%	0.334%
6	2.516	449	459	468	rVB	9073	14682	2.65%	0.307%
7	3.047	615	624	636	rVB6	5670	11386	2.06%	0.238%
8	3.905	874	891	916	rBV	39090	138879	25.09%	2.908%
9	4.352	1014	1030	1057	rBV	112298	284691	51.44%	5.961%
10	5.050	1228	1247	1271	rBV2	223941	553462	100.00%	11.588%
11	5.616	1411	1423	1444	rBV	201136	411503	74.35%	8.616%
12	5.912	1502	1515	1531	rBV4	9138	21552	3.89%	0.451%
13	6.069	1552	1564	1593	rBV	139206	295234	53.34%	6.181%
14	6.989	1839	1850	1876	rBV	47192	94080	17.00%	1.970%
15	7.313	1937	1951	1973	rBV	223317	400514	72.37%	8.386%
16	7.625	2037	2048	2067	rBV	26254	49977	9.03%	1.046%
17	7.937	2136	2145	2154	rBV4	4948	9184	1.66%	0.192%
18	8.088	2182	2192	2232	rBV2	220494	540011	97.57%	11.306%
19	8.249	2237	2242	2257	rVB9	3267	7414	1.34%	0.155%
20	8.850	2418	2429	2452	rBV	312575	521594	94.24%	10.921%
21	10.214	2841	2853	2870	rBV	91277	147921	26.73%	3.097%
22	10.381	2894	2905	2916	rBV	16028	26114	4.72%	0.547%
23	11.246	3163	3174	3197	rBV	261468	410957	74.25%	8.604%
24	11.622	3279	3291	3312	rBV	234301	369958	66.84%	7.746%
25	12.249	3475	3486	3496	rVB	3901	5547	1.00%	0.116%
26	12.342	3505	3515	3530	rBV5	10817	16955	3.06%	0.355%




Sum of corrected areas: 4776216

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026053.D
Acq On : 09 Jun 2022 14:33
Operator : SY/MD
Sample : N3247-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

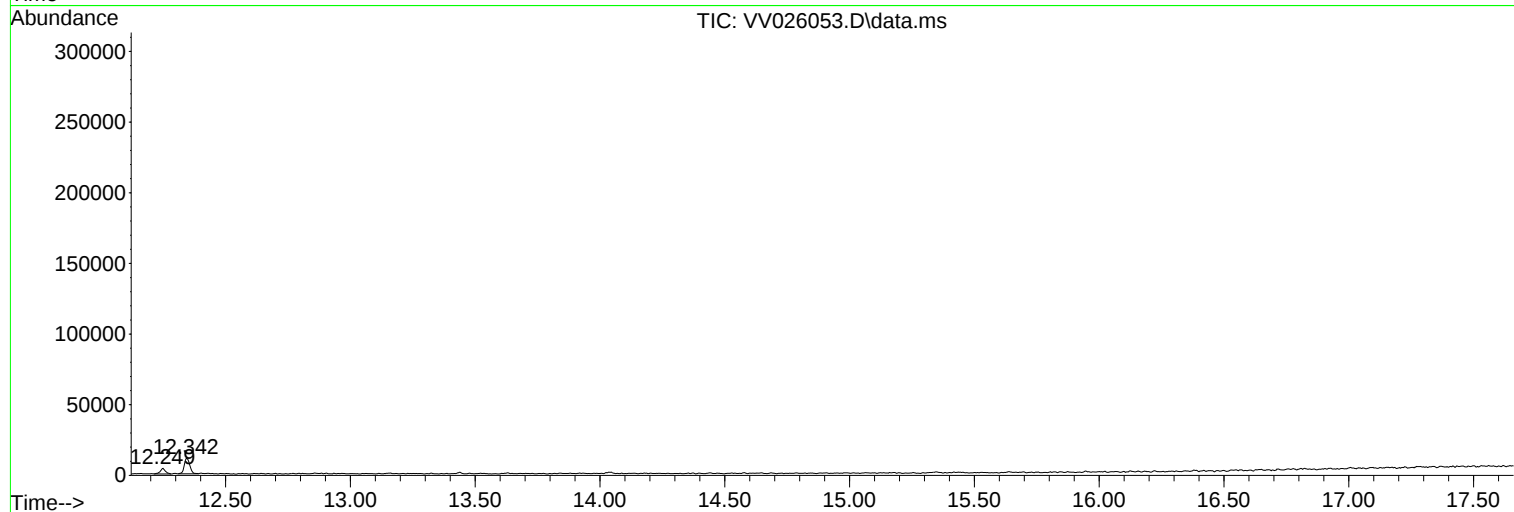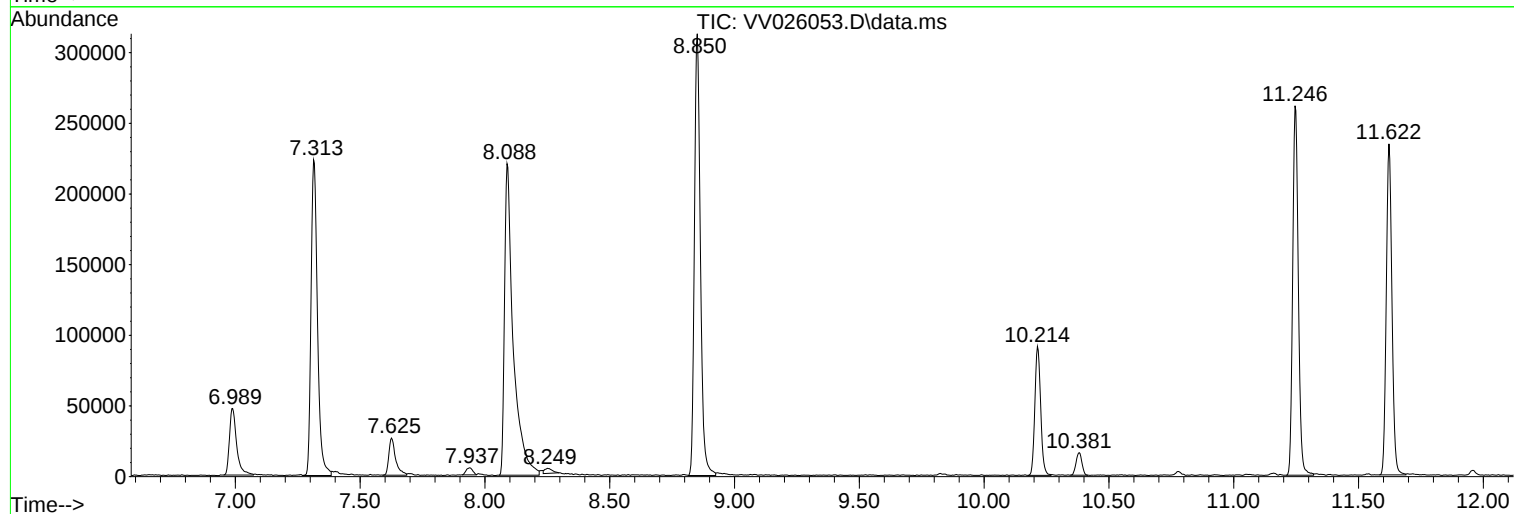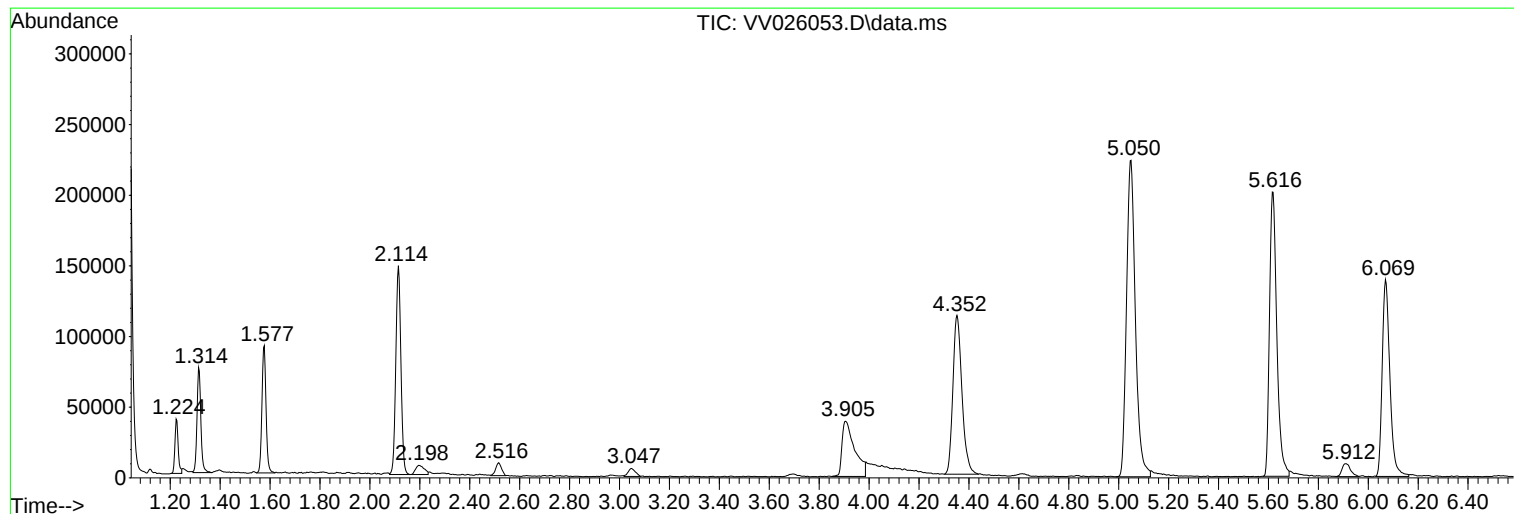

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026053.D
Acq On : 09 Jun 2022 14:33
Operator : SY/MD
Sample : N3247-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026053.D
Acq On : 09 Jun 2022 14:33
Operator : SY/MD
Sample : N3247-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc