

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026054.D
 Acq On : 09 Jun 2022 14:57
 Operator : SY/MD
 Sample : N3247-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYS9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.317	79	86	101	rVB	72391	78579	9.01%	1.342%
2	1.581	160	168	180	rBV	86008	98399	11.28%	1.680%
3	2.121	325	336	352	rVB2	153380	229857	26.35%	3.925%
4	3.204	659	673	698	rVB	56073	119683	13.72%	2.044%
5	3.921	881	896	919	rBV3	55569	185098	21.22%	3.161%
6	4.362	1016	1033	1058	rVB	113256	283593	32.51%	4.843%
7	4.616	1094	1112	1135	rBV	352484	872353	100.00%	14.896%
8	5.056	1233	1249	1274	rBV2	227886	569366	65.27%	9.723%
9	5.622	1413	1425	1451	rBV	214263	438924	50.31%	7.495%
10	5.924	1506	1519	1546	rVB5	22935	55819	6.40%	0.953%
11	6.076	1553	1566	1588	rBV	143677	299698	34.36%	5.118%
12	6.992	1840	1851	1874	rBV2	48651	92981	10.66%	1.588%
13	7.320	1941	1953	1977	rBV	225150	408076	46.78%	6.968%
14	7.629	2040	2049	2071	rBV	26814	51732	5.93%	0.883%
15	8.092	2183	2193	2240	rBV2	224512	550522	63.11%	9.401%
16	8.854	2418	2430	2462	rBV	327956	541847	62.11%	9.253%
17	10.217	2843	2854	2874	rBV	97620	158522	18.17%	2.707%
18	11.249	3164	3175	3199	rBV	284476	445480	51.07%	7.607%
19	11.622	3279	3291	3313	rBV	233073	375612	43.06%	6.414%




Sum of corrected areas: 5856141

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026054.D
Acq On : 09 Jun 2022 14:57
Operator : SY/MD
Sample : N3247-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

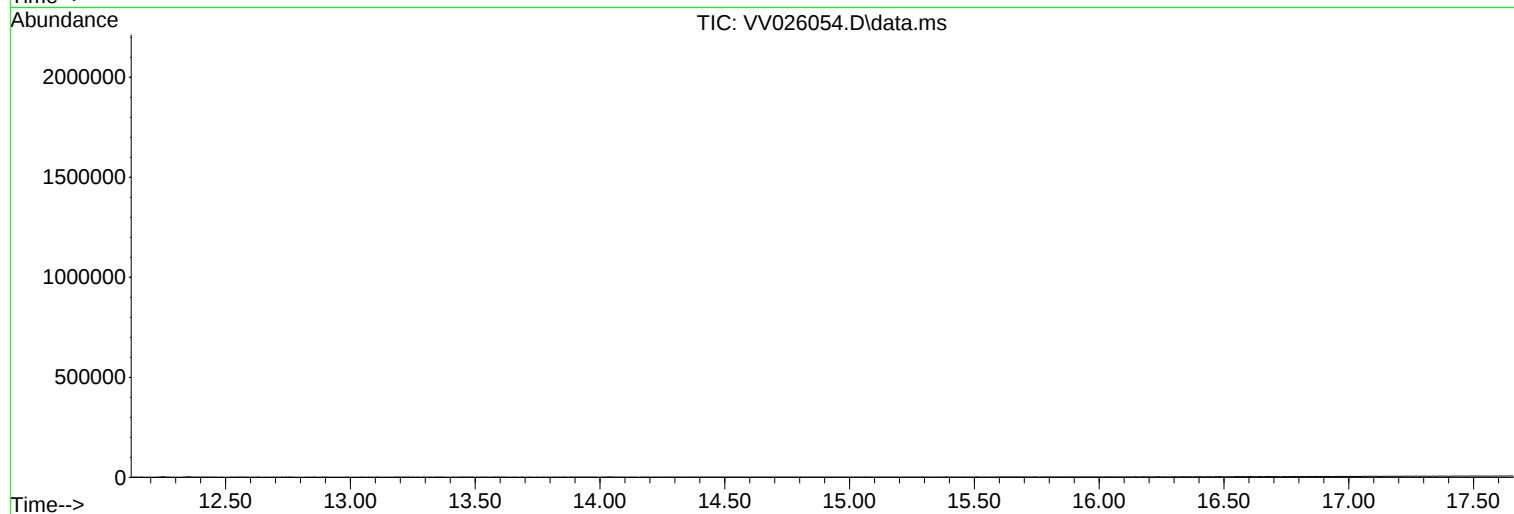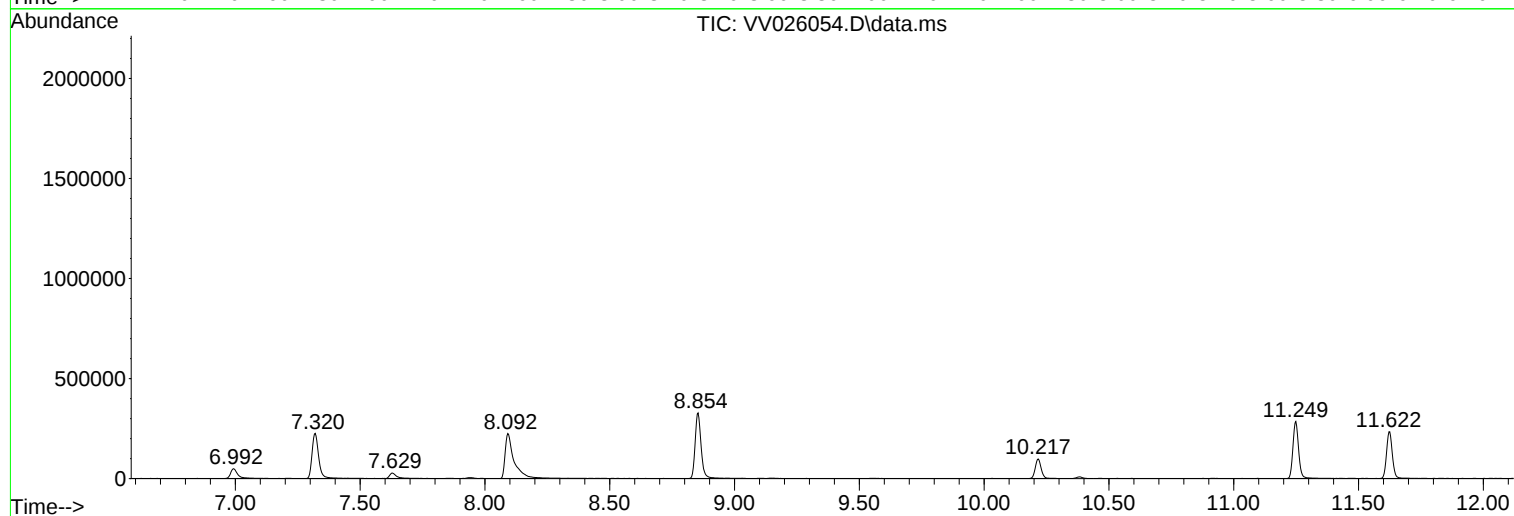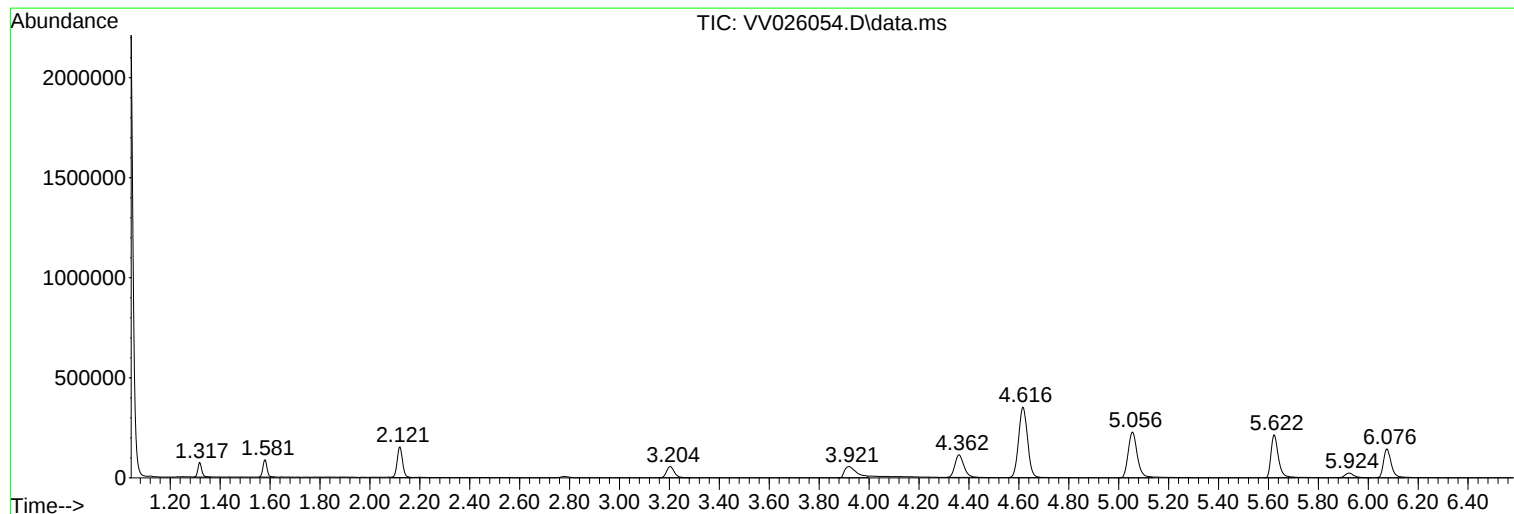

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026054.D
Acq On : 09 Jun 2022 14:57
Operator : SY/MD
Sample : N3247-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026054.D
Acq On : 09 Jun 2022 14:57
Operator : SY/MD
Sample : N3247-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc