

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026058.D
 Acq On : 09 Jun 2022 16:33
 Operator : SY/MD
 Sample : N3247-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	98	rBV	79516	83650	16.41%	1.777%
2	1.581	161	168	181	rBV	77311	87828	17.23%	1.866%
3	2.121	322	336	350	rVB2	135076	198581	38.96%	4.219%
4	3.925	885	897	931	rBV3	56703	207799	40.77%	4.415%
5	4.365	1017	1034	1060	rBV2	104353	290475	56.99%	6.171%
6	4.622	1098	1114	1130	rBV2	37033	94266	18.50%	2.003%
7	5.056	1233	1249	1280	rBV3	200968	509667	100.00%	10.828%
8	5.625	1414	1426	1453	rBV	191513	397053	77.90%	8.436%
9	5.924	1506	1519	1547	rVB4	41292	91685	17.99%	1.948%
10	6.076	1551	1566	1598	rBV	128946	279921	54.92%	5.947%
11	6.992	1841	1851	1869	rBV2	42143	80720	15.84%	1.715%
12	7.320	1942	1953	1974	rBV	201808	362325	71.09%	7.698%
13	7.629	2040	2049	2069	rBV3	23190	46138	9.05%	0.980%
14	7.979	2147	2158	2174	rVB3	67795	116794	22.92%	2.481%
15	8.092	2184	2193	2228	rBV2	214273	493886	96.90%	10.493%
16	8.854	2419	2430	2455	rBV	300648	491284	96.39%	10.438%
17	10.217	2841	2854	2873	rBV	91361	143547	28.16%	3.050%
18	11.249	3163	3175	3196	rBV	248840	391000	76.72%	8.307%
19	11.622	3280	3291	3314	rBV	215411	340267	66.76%	7.229%




Sum of corrected areas: 4706886

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026058.D
Acq On : 09 Jun 2022 16:33
Operator : SY/MD
Sample : N3247-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

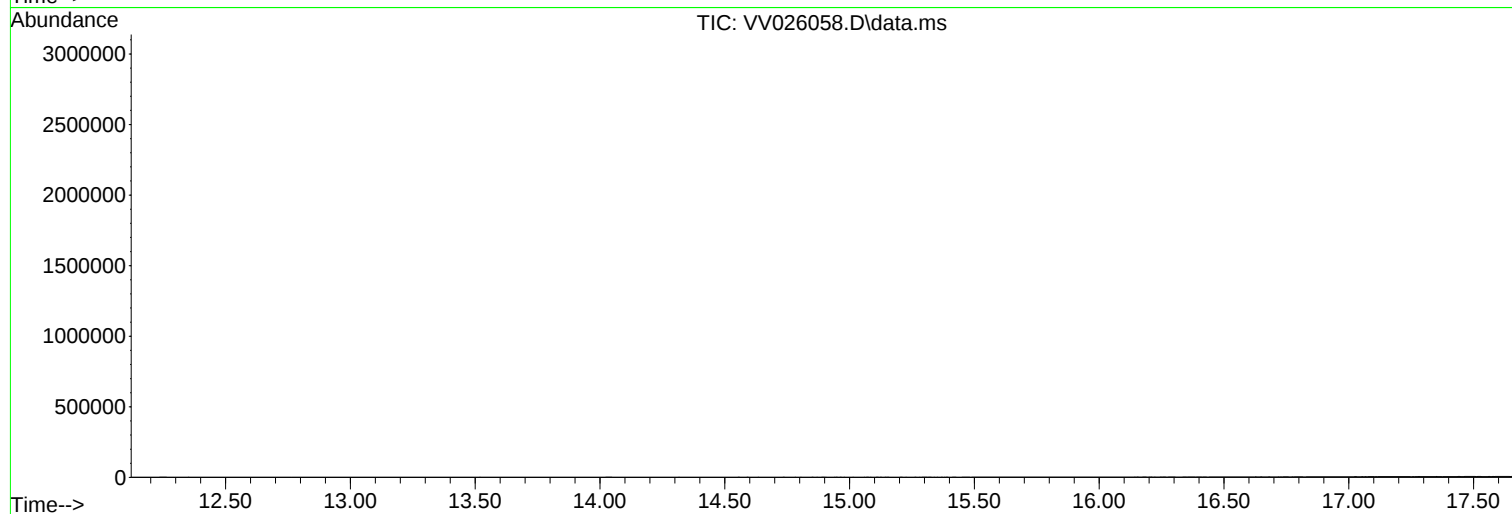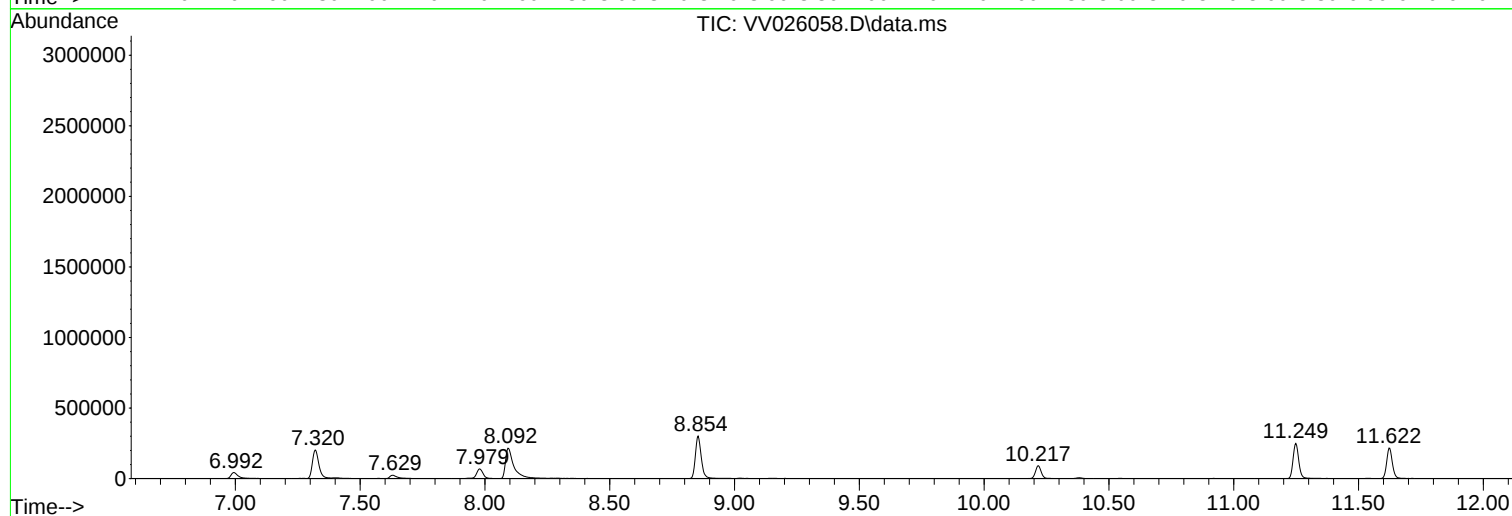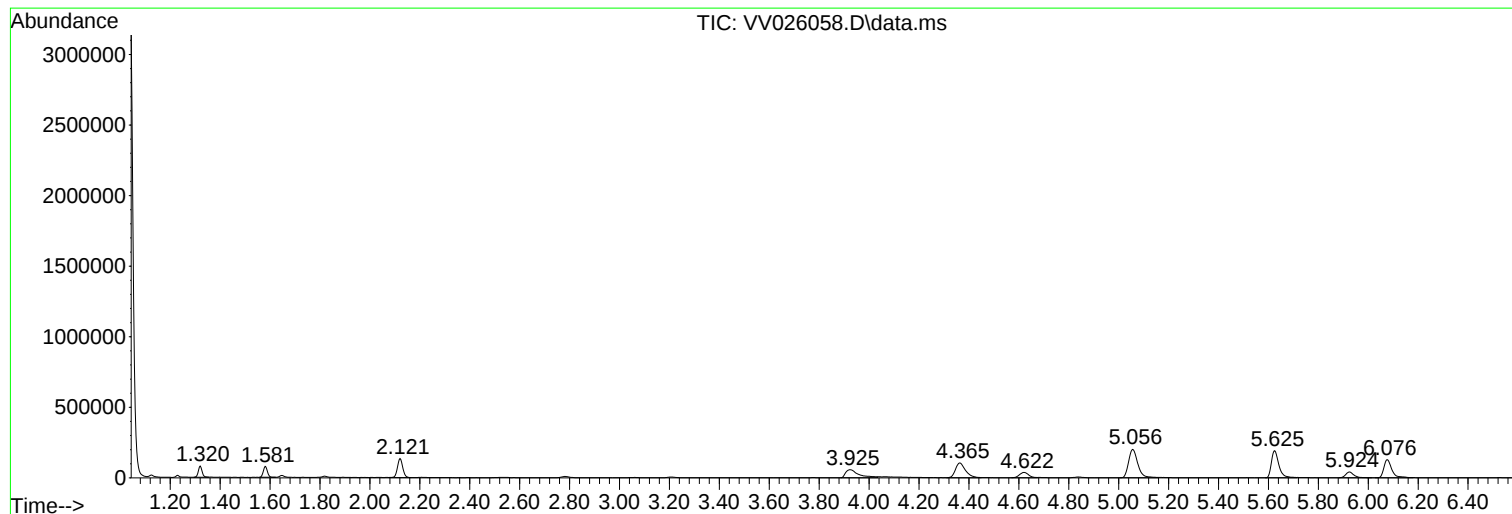

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026058.D
Acq On : 09 Jun 2022 16:33
Operator : SY/MD
Sample : N3247-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026058.D
Acq On : 09 Jun 2022 16:33
Operator : SY/MD
Sample : N3247-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
