

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026059.D
 Acq On : 09 Jun 2022 16:57
 Operator : SY/MD
 Sample : N3247-10
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYW5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	99	rVB	65520	69109	13.55%	1.383%
2	1.581	160	168	183	rBV	76829	89349	17.51%	1.787%
3	2.124	325	337	353	rVB3	156378	251465	49.29%	5.031%
4	2.523	452	461	473	rVB	12005	19291	3.78%	0.386%
5	3.207	659	674	697	rBV	38339	82308	16.13%	1.647%
6	3.921	885	896	924	rBV5	54614	190138	37.27%	3.804%
7	4.362	1018	1033	1060	rVB2	100674	251915	49.38%	5.040%
8	4.619	1096	1113	1136	rBV3	115299	290983	57.03%	5.821%
9	5.056	1235	1249	1281	rBV2	203721	510193	100.00%	10.207%
10	5.625	1413	1426	1454	rBV	196334	407365	79.85%	8.150%
11	5.924	1506	1519	1538	rBV6	30921	70280	13.78%	1.406%
12	6.075	1552	1566	1593	rBV	128742	269500	52.82%	5.392%
13	6.992	1842	1851	1876	rBV	41744	81771	16.03%	1.636%
14	7.320	1941	1953	1980	rBV	202523	362835	71.12%	7.259%
15	7.632	2040	2050	2075	rBV2	23142	46654	9.14%	0.933%
16	7.979	2148	2158	2180	rVB2	73592	129253	25.33%	2.586%
17	8.095	2180	2194	2230	rBV2	204276	479937	94.07%	9.601%
18	8.854	2419	2430	2449	rBV	306194	501046	98.21%	10.024%
19	10.217	2841	2854	2869	rBV	85361	139942	27.43%	2.800%
20	11.249	3162	3175	3198	rBV	267047	416752	81.69%	8.337%
21	11.625	3280	3292	3311	rBV	212758	338513	66.35%	6.772%




Sum of corrected areas: 4998599

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026059.D
Acq On : 09 Jun 2022 16:57
Operator : SY/MD
Sample : N3247-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

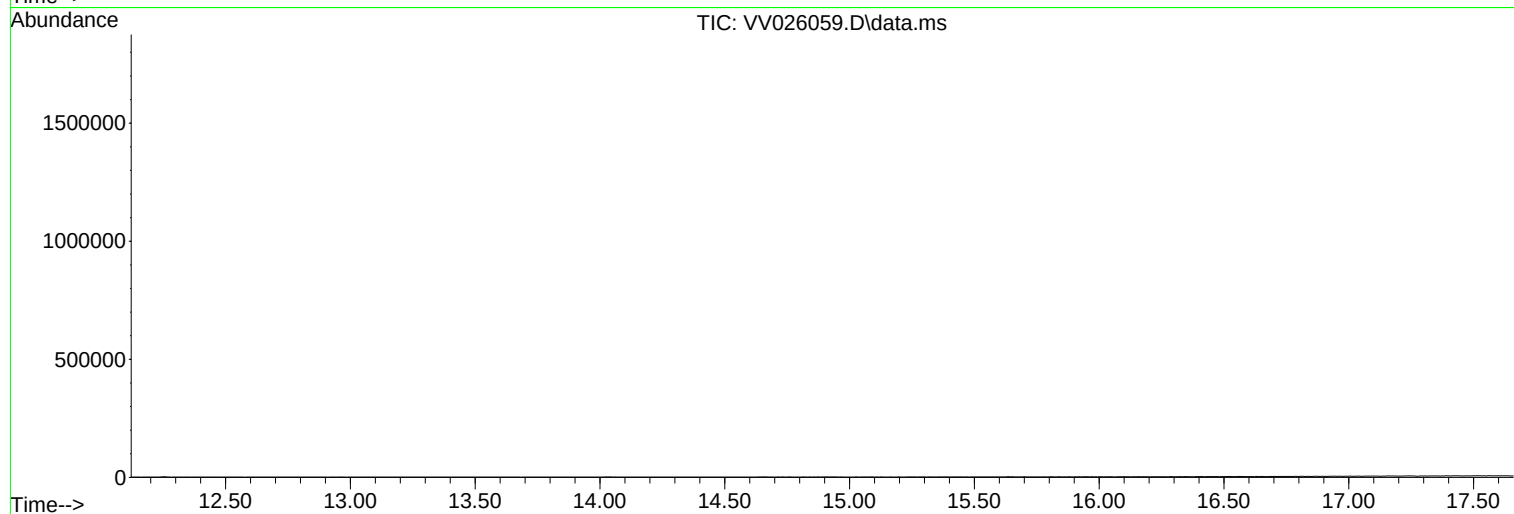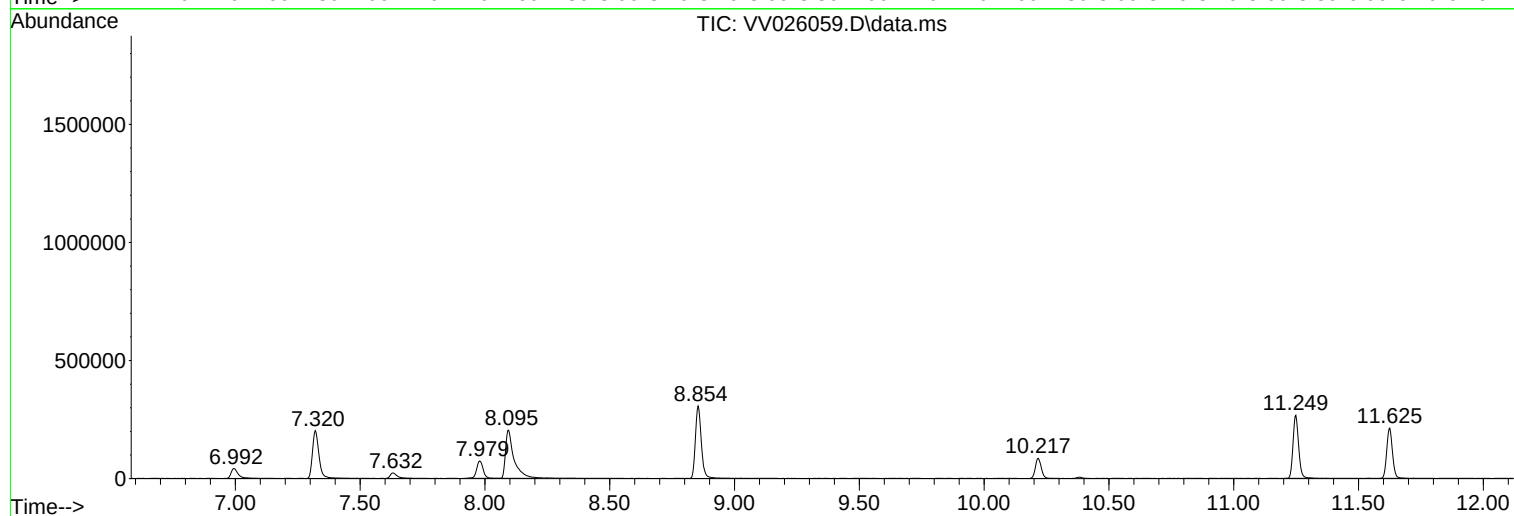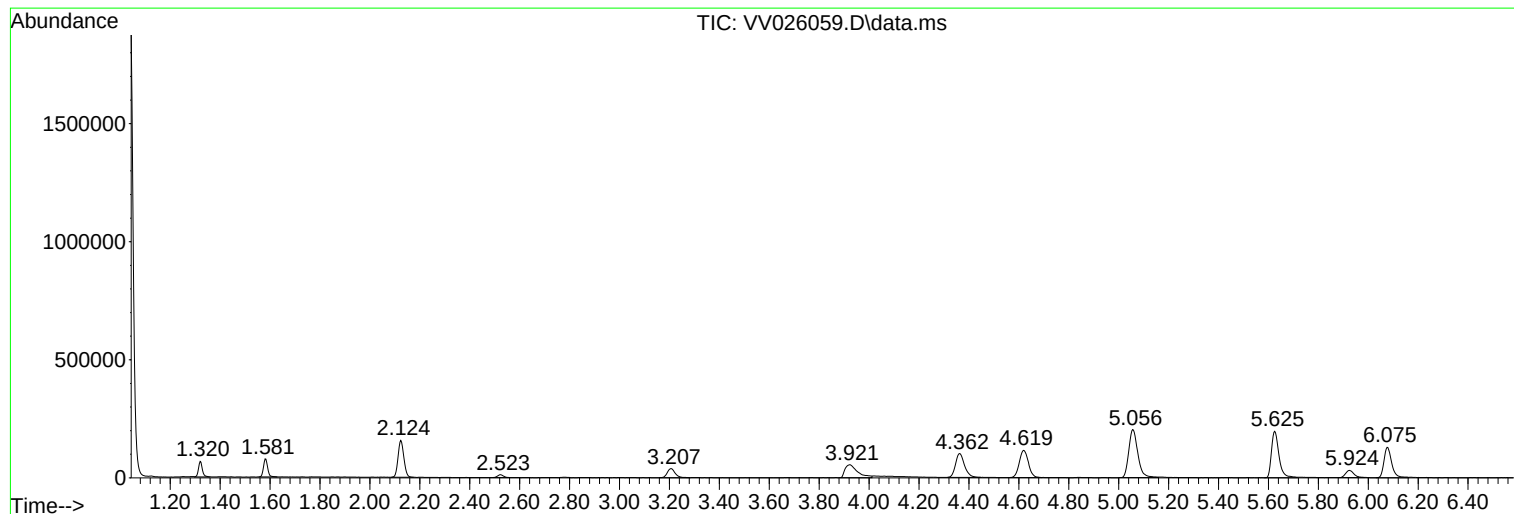

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026059.D
Acq On : 09 Jun 2022 16:57
Operator : SY/MD
Sample : N3247-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026059.D
Acq On : 09 Jun 2022 16:57
Operator : SY/MD
Sample : N3247-10
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
