

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026060.D
 Acq On : 09 Jun 2022 17:21
 Operator : SY/MD
 Sample : N3272-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B43

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	99	rBV	70548	75435	12.22%	1.435%
2	1.584	161	169	179	rBV	89205	102563	16.61%	1.951%
3	2.121	326	336	352	rVB	147973	215513	34.91%	4.100%
4	3.905	882	891	925	rBV	50922	179133	29.02%	3.408%
5	4.362	1017	1033	1065	rVB2	123135	307573	49.82%	5.851%
6	5.056	1233	1249	1276	rBV2	245699	615032	99.63%	11.700%
7	5.626	1414	1426	1461	rBV	231005	480208	77.79%	9.135%
8	5.918	1506	1517	1536	rVB6	11532	25600	4.15%	0.487%
9	6.076	1553	1566	1591	rBV	157106	325980	52.80%	6.201%
10	6.992	1842	1851	1875	rBV	52464	103212	16.72%	1.963%
11	7.320	1941	1953	1974	rBV	250363	445771	72.21%	8.480%
12	7.629	2040	2049	2067	rBV3	28482	54849	8.88%	1.043%
13	7.979	2150	2158	2173	rVB3	20055	34804	5.64%	0.662%
14	8.092	2182	2193	2230	rBV2	261885	617340	100.00%	11.744%
15	8.854	2413	2430	2466	rBV	357843	591856	95.87%	11.259%
16	10.217	2843	2854	2870	rBV	105665	166482	26.97%	3.167%
17	10.381	2896	2905	2916	rBV2	6138	9275	1.50%	0.176%
18	11.249	3155	3175	3194	rBV	307534	476064	77.12%	9.057%
19	11.625	3279	3292	3307	rBV	270545	423615	68.62%	8.059%
20	13.435	3848	3855	3870	rBV8	4158	6247	1.01%	0.119%




Sum of corrected areas: 5256552

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026060.D
Acq On : 09 Jun 2022 17:21
Operator : SY/MD
Sample : N3272-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

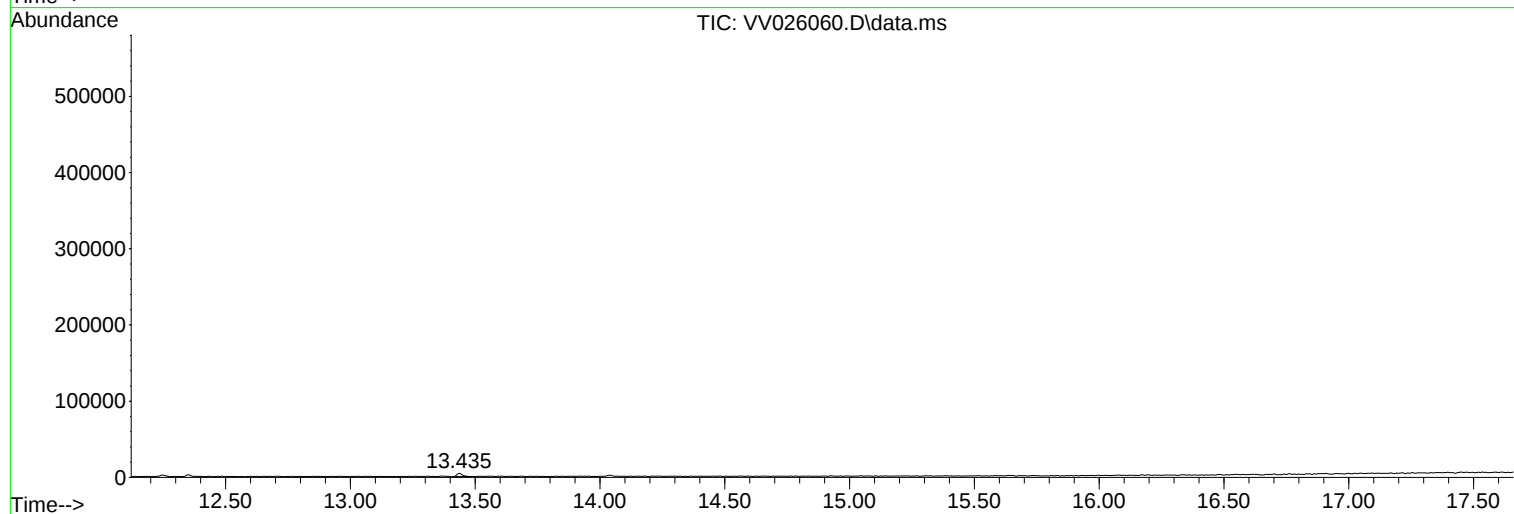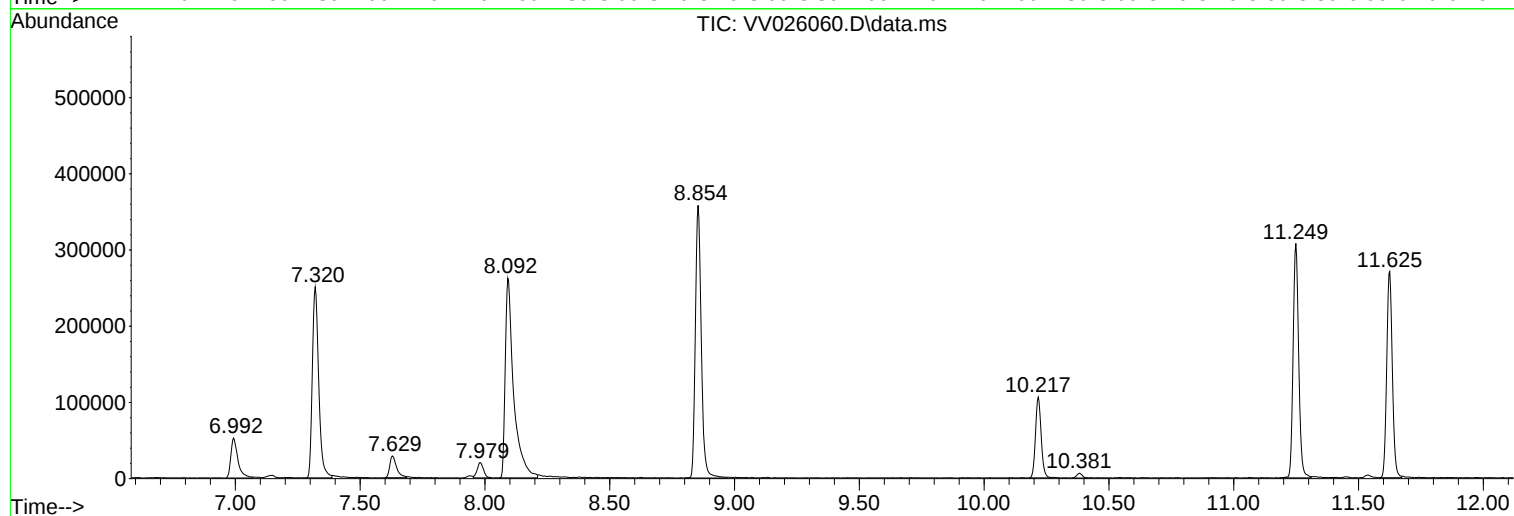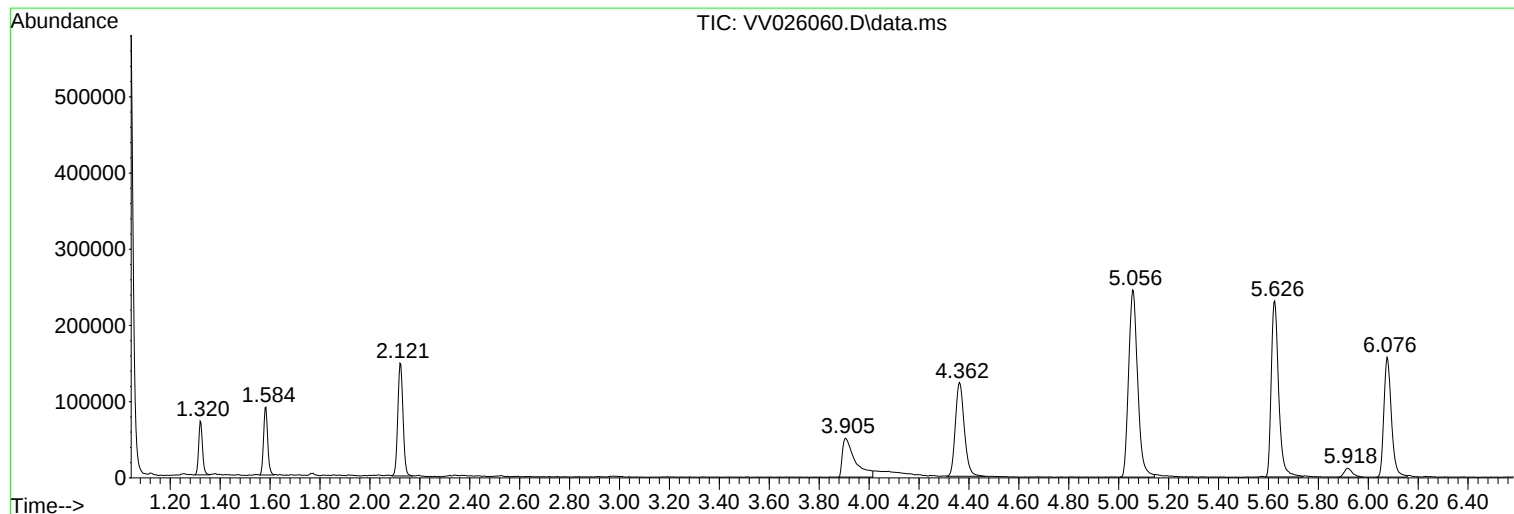

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026060.D
Acq On : 09 Jun 2022 17:21
Operator : SY/MD
Sample : N3272-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026060.D
Acq On : 09 Jun 2022 17:21
Operator : SY/MD
Sample : N3272-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc