

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026062.D
 Acq On : 09 Jun 2022 18:09
 Operator : SY/MD
 Sample : N3272-03
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B47

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026062.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	103	rVB	62334	67824	12.01%	1.452%
2	1.581	161	168	179	rVB	79762	90738	16.07%	1.942%
3	1.767	217	226	234	rBV2	7970	10485	1.86%	0.224%
4	2.121	326	336	353	rVB	128852	187949	33.28%	4.023%
5	3.912	883	893	918	rBV	44295	148975	26.38%	3.189%
6	4.362	1017	1033	1058	rBV2	106623	263493	46.66%	5.640%
7	5.056	1234	1249	1278	rBV2	210102	526750	93.28%	11.275%
8	5.625	1415	1426	1451	rBV	223740	453597	80.33%	9.709%
9	5.921	1507	1518	1534	rBV8	9802	22886	4.05%	0.490%
10	6.076	1553	1566	1590	rBV2	135801	282256	49.99%	6.041%
11	6.992	1841	1851	1870	rBV3	45451	87290	15.46%	1.868%
12	7.320	1941	1953	1976	rBV	211451	373695	66.18%	7.999%
13	7.629	2039	2049	2063	rBV	24378	46438	8.22%	0.994%
14	7.982	2149	2159	2177	rVB3	20309	37500	6.64%	0.803%
15	8.092	2184	2193	2225	rBV2	222694	521614	92.37%	11.165%
16	8.854	2419	2430	2456	rBV	343774	564678	100.00%	12.087%
17	10.217	2843	2854	2871	rBV	90899	147109	26.05%	3.149%
18	10.378	2896	2904	2915	rBV2	6842	11404	2.02%	0.244%
19	11.249	3163	3175	3196	rBV	294707	462543	81.91%	9.900%
20	11.622	3276	3291	3317	rBV	232413	364736	64.59%	7.807%




Sum of corrected areas: 4671960

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026062.D
Acq On : 09 Jun 2022 18:09
Operator : SY/MD
Sample : N3272-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

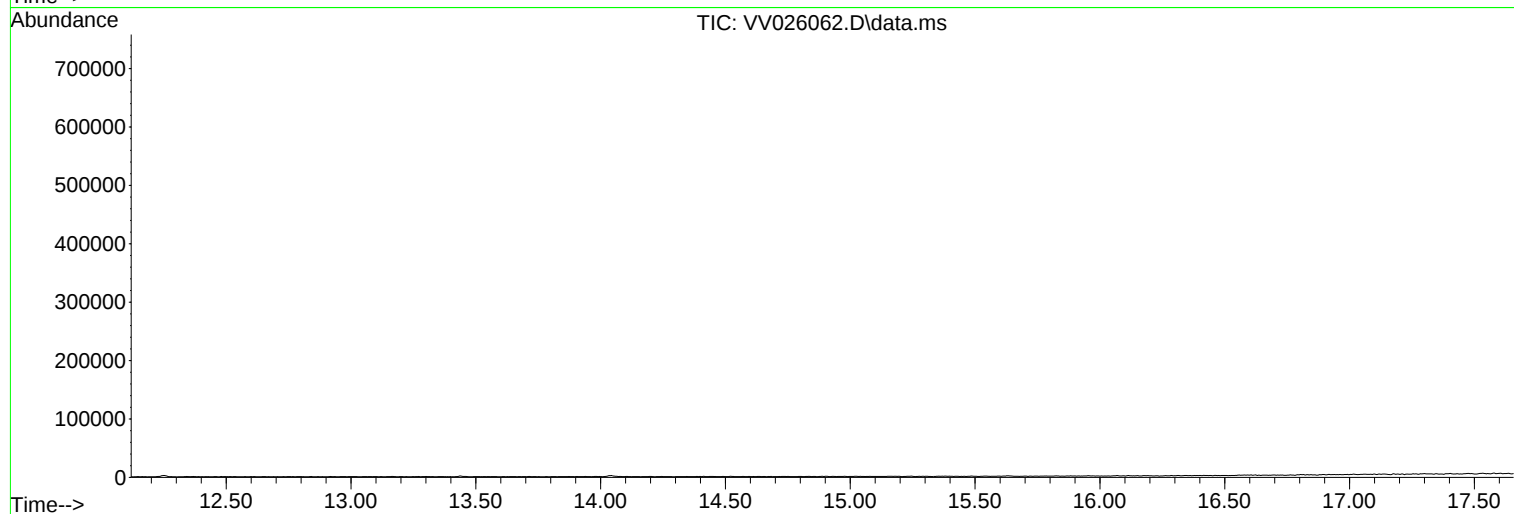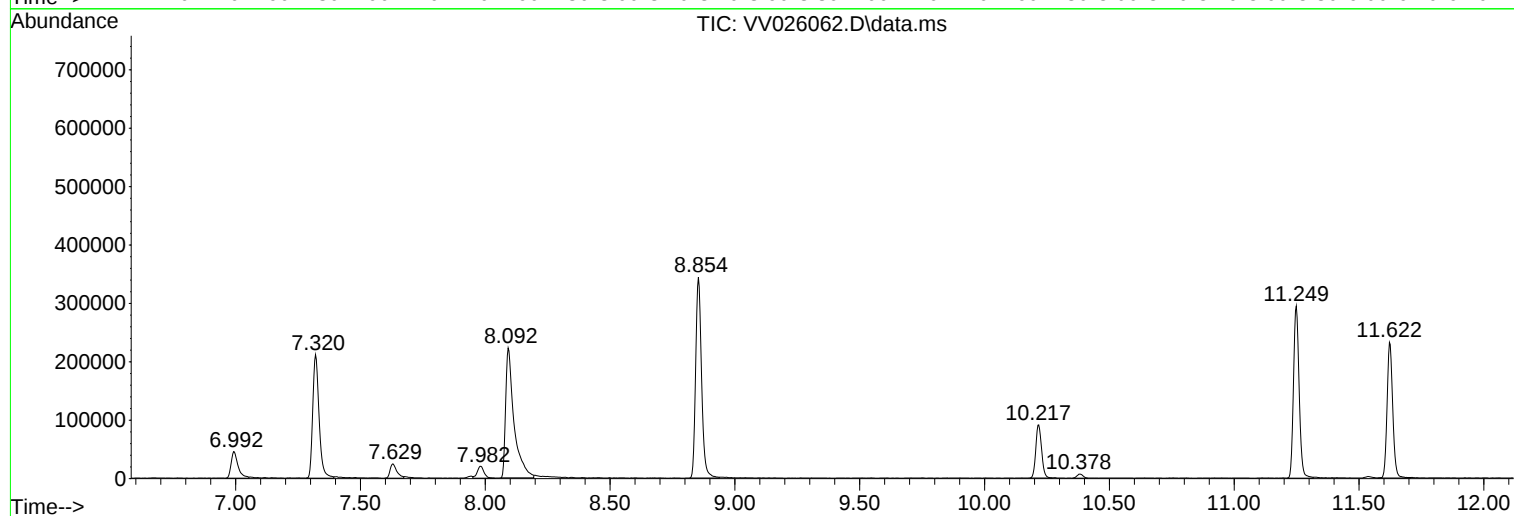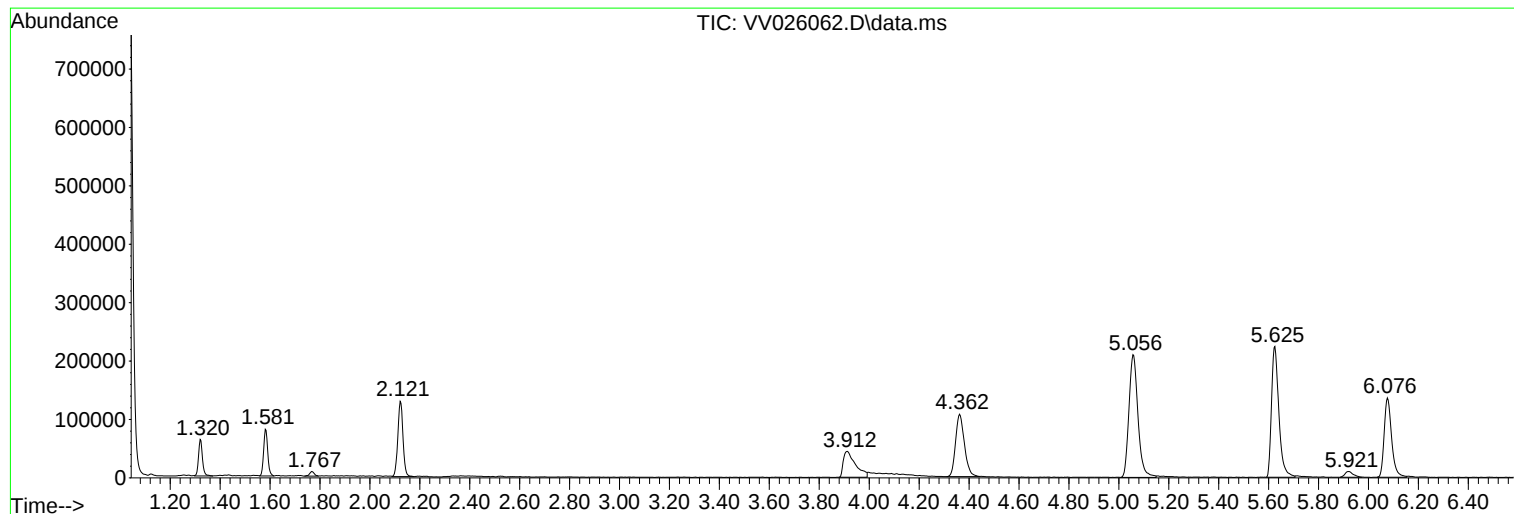

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026062.D
Acq On : 09 Jun 2022 18:09
Operator : SY/MD
Sample : N3272-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026062.D
Acq On : 09 Jun 2022 18:09
Operator : SY/MD
Sample : N3272-03
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc