

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026063.D
 Acq On : 09 Jun 2022 18:33
 Operator : SY/MD
 Sample : N3256-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026063.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	97	rBV	67915	70996	14.84%	1.778%
2	1.581	161	168	184	rVB	78059	88953	18.59%	2.228%
3	2.121	326	336	351	rVB	129663	185989	38.87%	4.659%
4	2.523	450	461	475	rBV	14232	23272	4.86%	0.583%
5	3.918	880	895	921	rBV3	54587	199449	41.68%	4.996%
6	4.362	1018	1033	1056	rBV	93298	230807	48.23%	5.782%
7	5.056	1234	1249	1290	rBV3	187535	478548	100.00%	11.988%
8	5.625	1412	1426	1461	rBV	174688	359922	75.21%	9.016%
9	5.915	1507	1516	1536	rVB5	6191	13350	2.79%	0.334%
10	6.076	1553	1566	1591	rBV2	117335	248064	51.84%	6.214%
11	6.995	1842	1852	1872	rBV2	33626	66090	13.81%	1.656%
12	7.320	1942	1953	1976	rBV	184573	334481	69.89%	8.379%
13	7.632	2039	2050	2067	rBV	18630	36469	7.62%	0.914%
14	8.095	2184	2194	2233	rBV2	187468	426138	89.05%	10.675%
15	8.419	2286	2295	2307	rBV3	11842	20812	4.35%	0.521%
16	8.854	2419	2430	2454	rBV	264300	440479	92.04%	11.034%
17	10.217	2841	2854	2871	rBV2	77556	123916	25.89%	3.104%
18	11.249	3164	3175	3193	rBV	226649	353399	73.85%	8.853%
19	11.625	3281	3292	3311	rBV	182403	290883	60.78%	7.287%




Sum of corrected areas: 3992017

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026063.D
Acq On : 09 Jun 2022 18:33
Operator : SY/MD
Sample : N3256-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

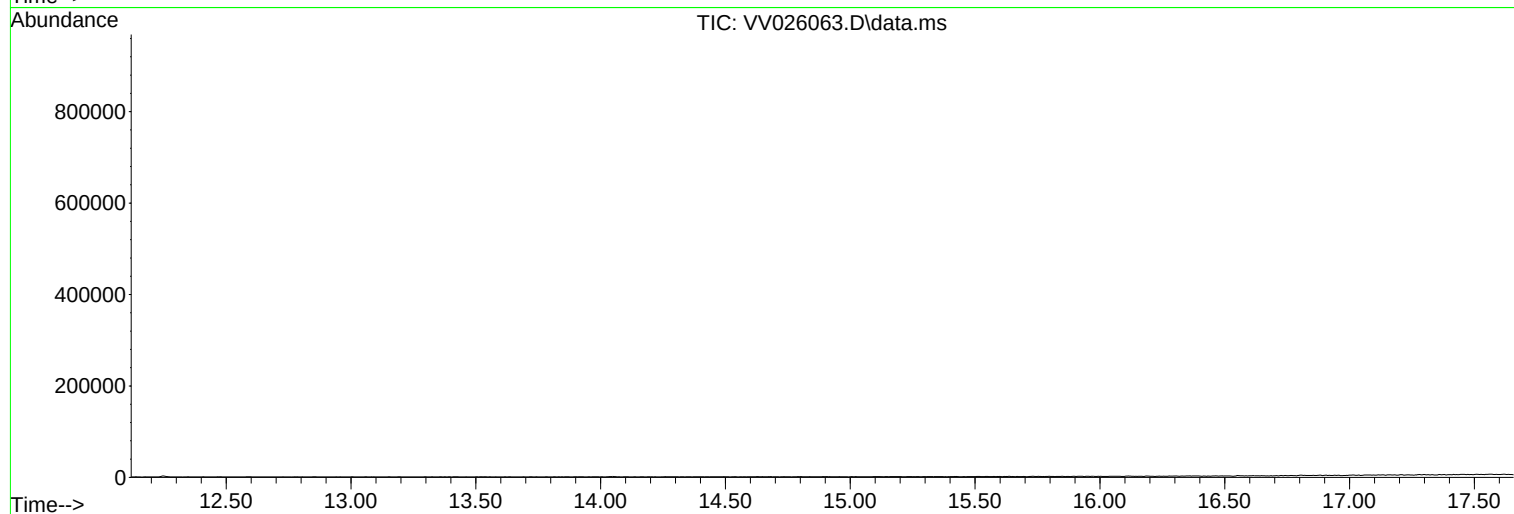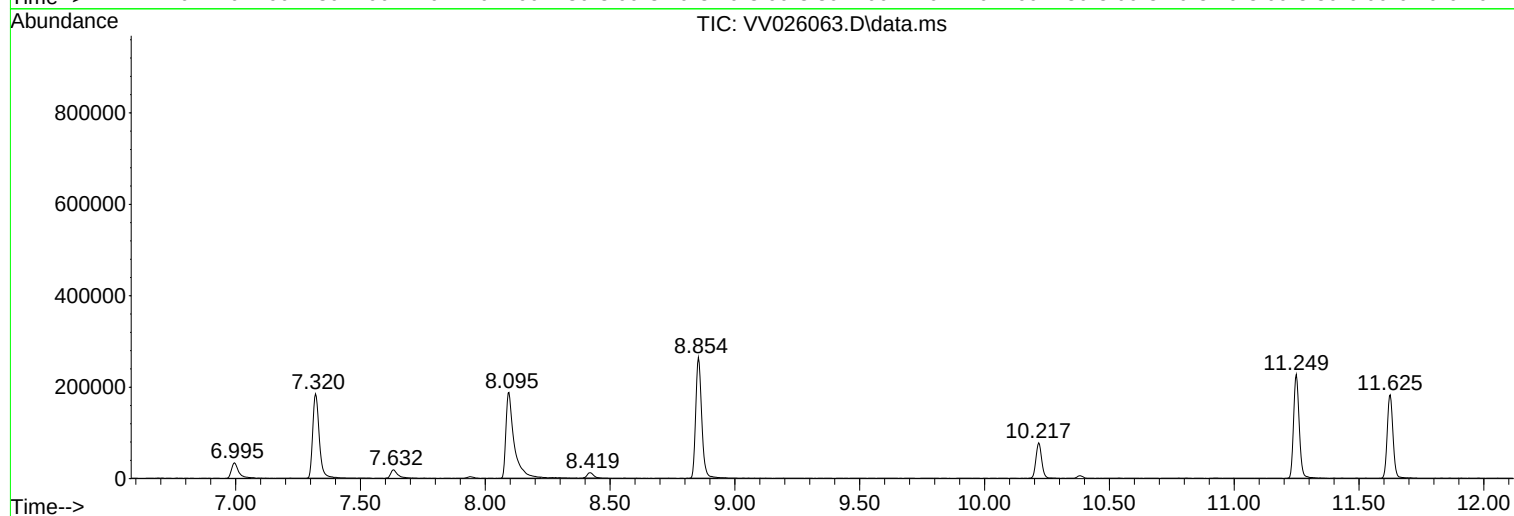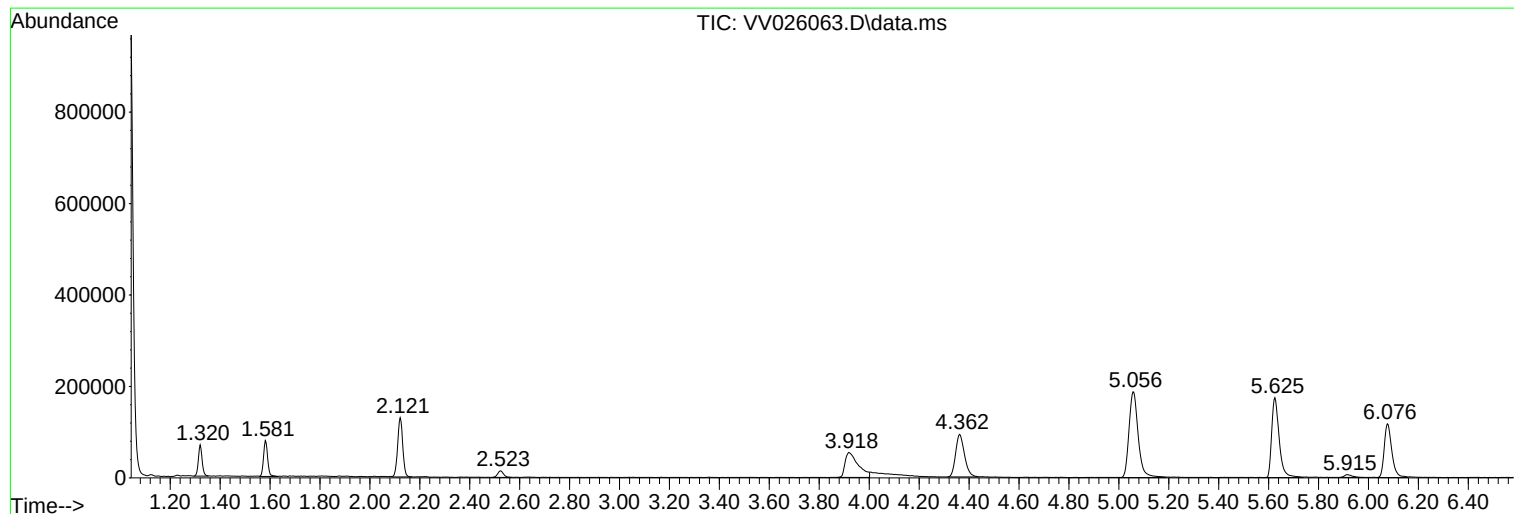

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026063.D
Acq On : 09 Jun 2022 18:33
Operator : SY/MD
Sample : N3256-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026063.D
Acq On : 09 Jun 2022 18:33
Operator : SY/MD
Sample : N3256-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc