

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026067.D
 Acq On : 09 Jun 2022 20:57
 Operator : SY/MD
 Sample : VV0609WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK365

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026067.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	101	rBV	66093	69940	13.74%	1.632%
2	1.581	160	168	180	rVB	77159	88627	17.42%	2.068%
3	2.121	326	336	357	rVB	125296	184279	36.21%	4.300%
4	2.523	452	461	475	rVB	10256	16736	3.29%	0.391%
5	3.921	879	896	929	rBV3	64525	266323	52.34%	6.215%
6	4.362	1019	1033	1059	rVB	97930	245662	48.28%	5.733%
7	5.056	1232	1249	1281	rBV2	201003	508848	100.00%	11.875%
8	5.625	1412	1426	1447	rBV	171775	352005	69.18%	8.214%
9	5.918	1506	1517	1538	rVB5	7111	16402	3.22%	0.383%
10	6.076	1553	1566	1594	rBV	127281	268700	52.81%	6.270%
11	6.995	1840	1852	1867	rBV2	40566	79367	15.60%	1.852%
12	7.320	1942	1953	1975	rBV	200282	357229	70.20%	8.336%
13	7.632	2037	2050	2073	rBV2	23304	45546	8.95%	1.063%
14	8.092	2182	2193	2231	rBV2	214908	495745	97.42%	11.569%
15	8.420	2285	2295	2308	rBV2	22544	39566	7.78%	0.923%
16	8.854	2416	2430	2453	rBV	259377	425134	83.55%	9.921%
17	10.217	2843	2854	2872	rBV	87426	139137	27.34%	3.247%
18	11.249	3164	3175	3194	rBV	225290	353437	69.46%	8.248%
19	11.622	3281	3291	3314	rBV	209998	332511	65.35%	7.760%




Sum of corrected areas: 4285194

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026067.D
Acq On : 09 Jun 2022 20:57
Operator : SY/MD
Sample : VV0609WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

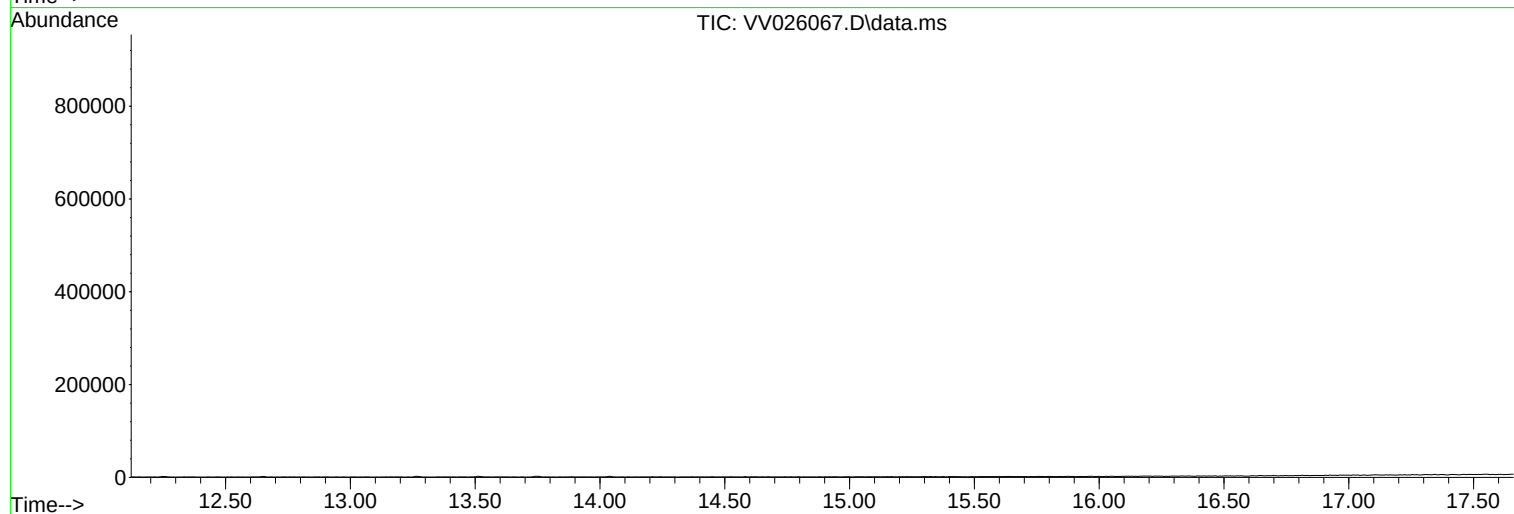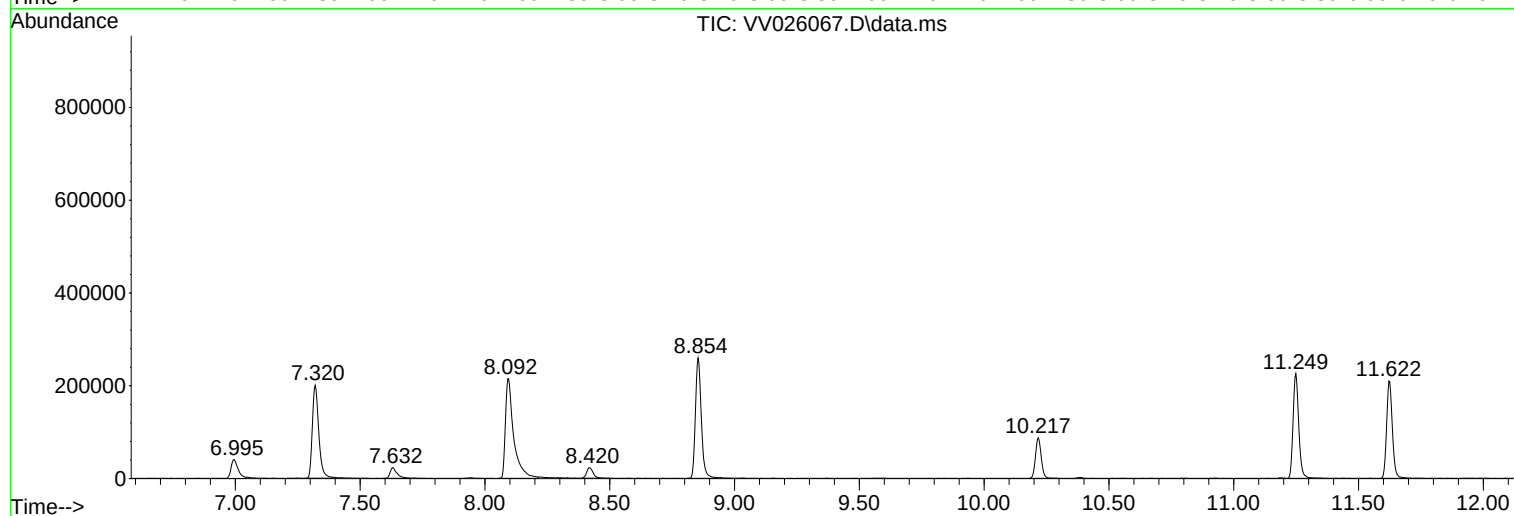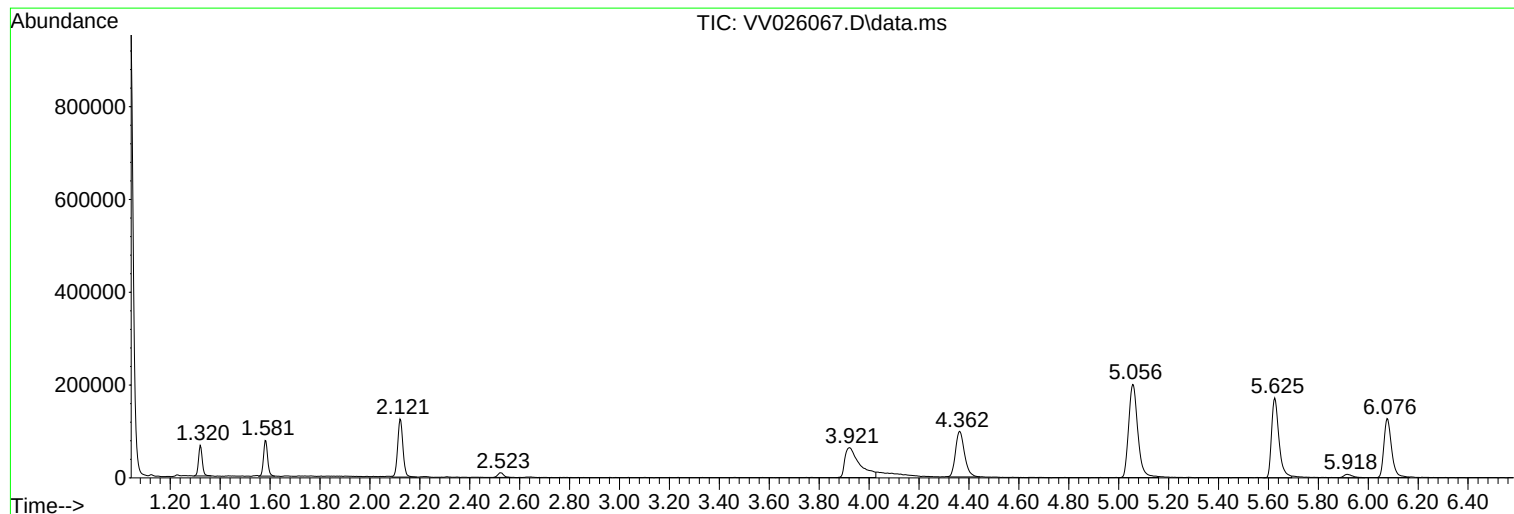

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026067.D
Acq On : 09 Jun 2022 20:57
Operator : SY/MD
Sample : VV0609WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026067.D
Acq On : 09 Jun 2022 20:57
Operator : SY/MD
Sample : VV0609WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK365

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc