

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026068.D
 Acq On : 09 Jun 2022 21:21
 Operator : SY/MD
 Sample : N3272-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B48

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026068.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	79	87	99	rVB	62571	65184	12.70%	1.478%
2	1.584	161	169	182	rVB	75780	87250	17.00%	1.978%
3	1.767	220	226	238	rVB	14473	19554	3.81%	0.443%
4	2.121	324	336	353	rVB	121184	179210	34.92%	4.064%
5	3.918	884	895	923	rBV	41241	153291	29.87%	3.476%
6	4.362	1016	1033	1062	rBV	99222	252165	49.14%	5.718%
7	5.060	1232	1250	1276	rBV3	201572	505342	98.48%	11.459%
8	5.625	1413	1426	1453	rBV	203374	420085	81.87%	9.526%
9	5.918	1508	1517	1519	rBV2	10184	12951	2.52%	0.294%
10	6.076	1554	1566	1594	rBV	127837	268826	52.39%	6.096%
11	6.995	1842	1852	1877	rBV2	42014	84470	16.46%	1.915%
12	7.320	1942	1953	1975	rBV	203306	358681	69.90%	8.133%
13	7.632	2038	2050	2072	rBV2	23740	47737	9.30%	1.082%
14	7.979	2147	2158	2173	rVB2	37116	64580	12.59%	1.464%
15	8.092	2184	2193	2220	rBV2	217059	492969	96.07%	11.179%
16	8.854	2418	2430	2454	rBV	308424	513134	100.00%	11.636%
17	10.217	2843	2854	2869	rBV2	89214	142232	27.72%	3.225%
18	11.249	3163	3175	3191	rBV	263899	404730	78.87%	9.178%
19	11.625	3279	3292	3308	rBV	214621	337549	65.78%	7.654%




Sum of corrected areas: 4409940

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026068.D
Acq On : 09 Jun 2022 21:21
Operator : SY/MD
Sample : N3272-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

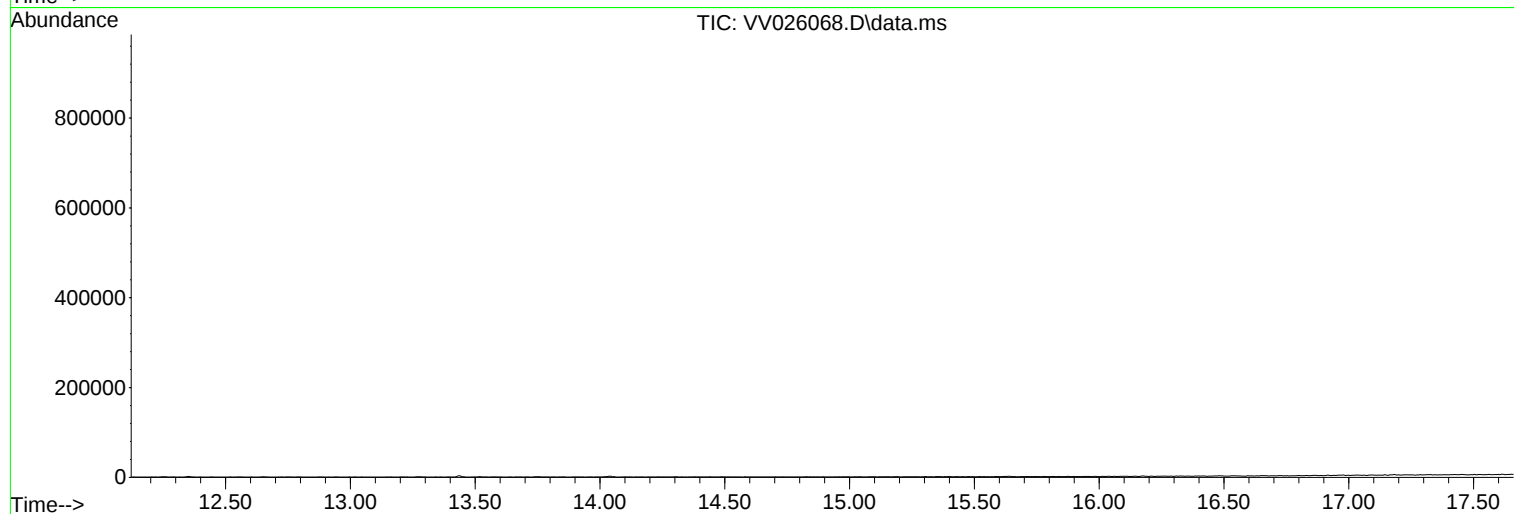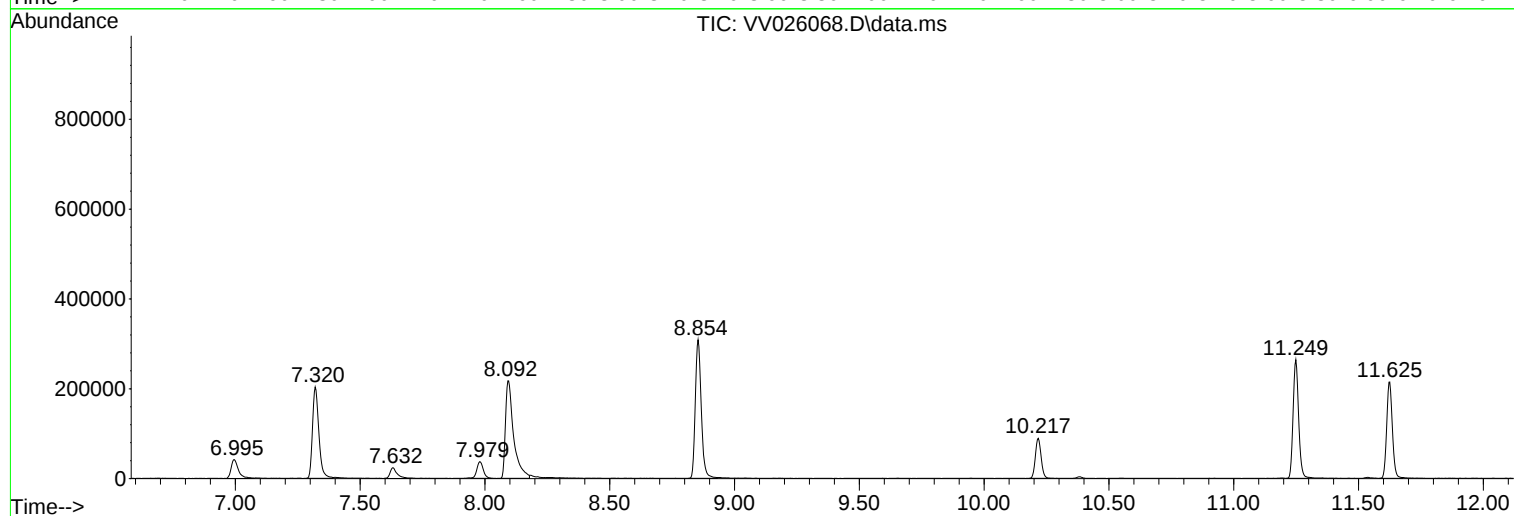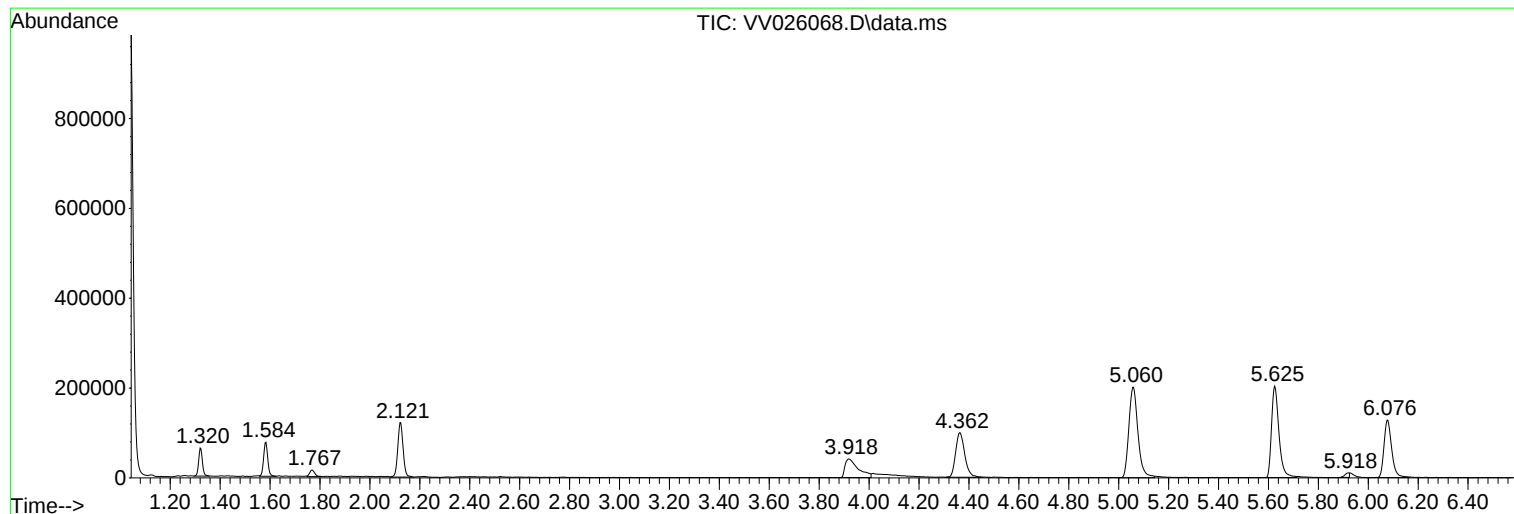

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026068.D
Acq On : 09 Jun 2022 21:21
Operator : SY/MD
Sample : N3272-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026068.D
Acq On : 09 Jun 2022 21:21
Operator : SY/MD
Sample : N3272-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc