

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026071.D
 Acq On : 09 Jun 2022 22:32
 Operator : SY/MD
 Sample : N3272-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B52

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026071.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	98	rVB	59417	61275	12.23%	1.377%
2	1.584	161	169	178	rBV	72695	81052	16.18%	1.822%
3	2.124	326	337	355	rVB	117647	174417	34.82%	3.920%
4	3.915	883	894	930	rBV2	31703	118100	23.58%	2.654%
5	4.362	1019	1033	1060	rBV	98638	248666	49.64%	5.589%
6	5.059	1234	1250	1279	rBV3	192640	483492	96.53%	10.867%
7	5.625	1413	1426	1456	rBV	197546	410244	81.90%	9.221%
8	5.921	1505	1518	1550	rBV3	128965	264058	52.72%	5.935%
9	6.075	1554	1566	1587	rBV	123696	256178	51.14%	5.758%
10	6.995	1843	1852	1877	rBV2	40912	81158	16.20%	1.824%
11	7.320	1941	1953	1976	rBV	194645	349638	69.80%	7.859%
12	7.628	2038	2049	2069	rBV	21639	42694	8.52%	0.960%
13	8.091	2183	2193	2235	rBV2	178231	438436	87.53%	9.854%
14	8.854	2418	2430	2449	rBV	302729	500897	100.00%	11.258%
15	10.217	2843	2854	2875	rBV	81991	135539	27.06%	3.046%
16	10.381	2897	2905	2920	rVB	7371	11879	2.37%	0.267%
17	11.249	3164	3175	3195	rBV	263993	411874	82.23%	9.257%
18	11.622	3280	3291	3309	rBV	208173	330041	65.89%	7.418%
19	12.349	3507	3517	3525	rBV7	6938	10560	2.11%	0.237%
20	13.435	3846	3855	3862	rBV5	7521	10313	2.06%	0.232%
21	14.326	4123	4132	4141	rBV2	20215	28591	5.71%	0.643%




Sum of corrected areas: 4449102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026071.D
Acq On : 09 Jun 2022 22:32
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

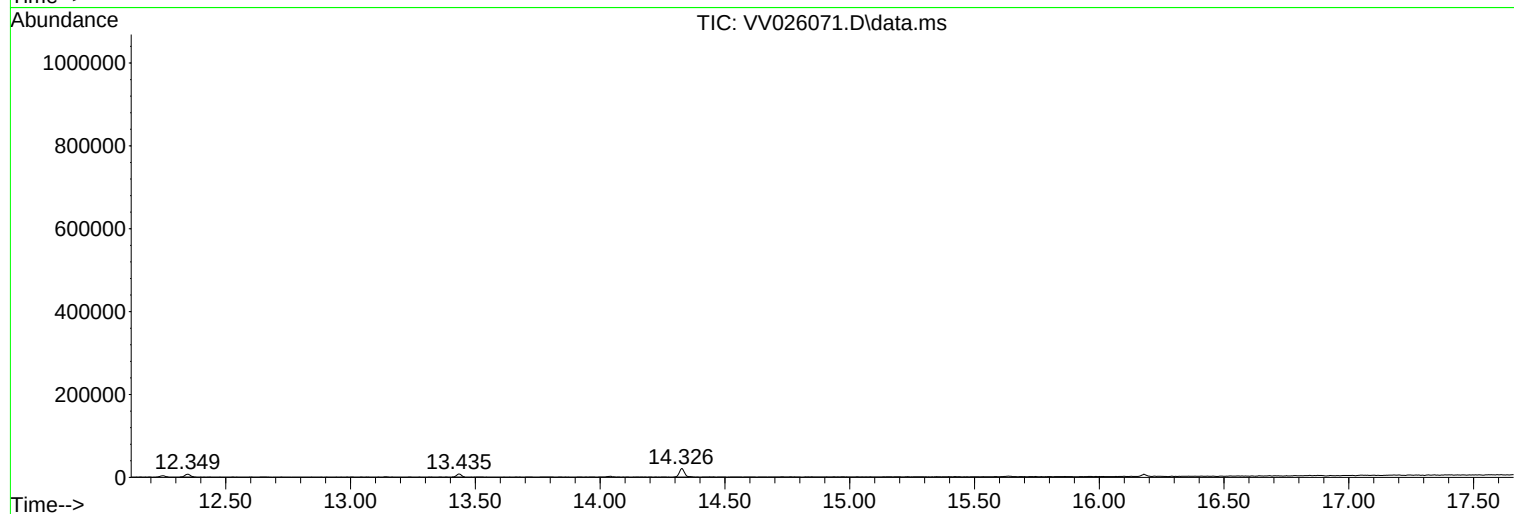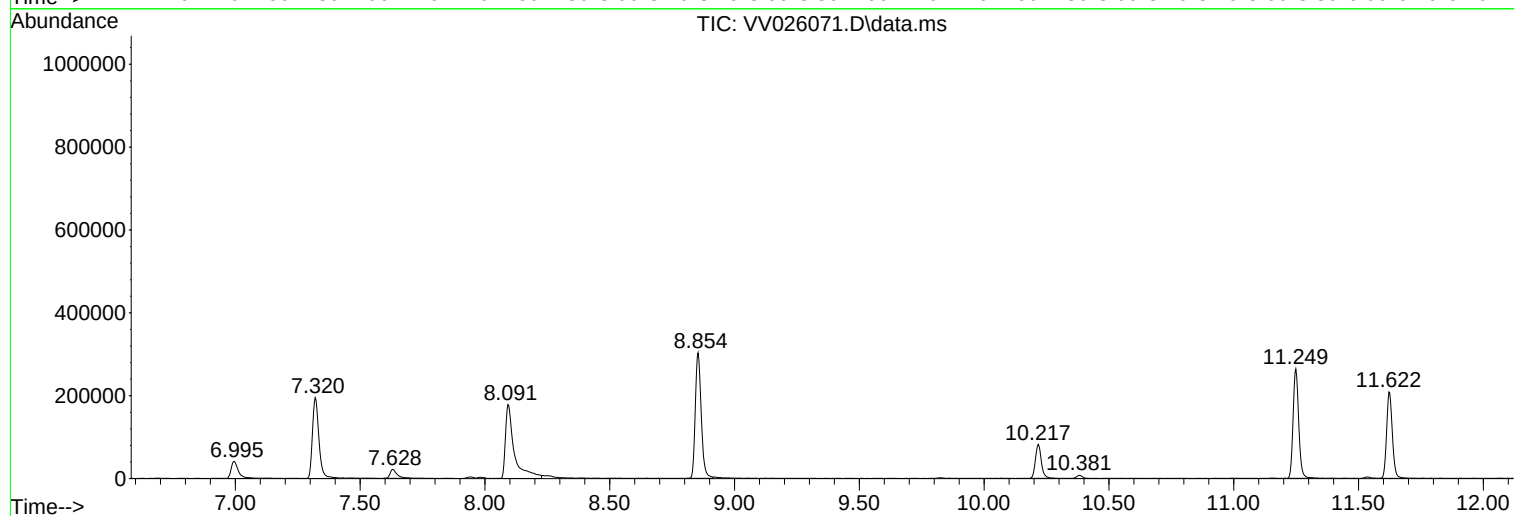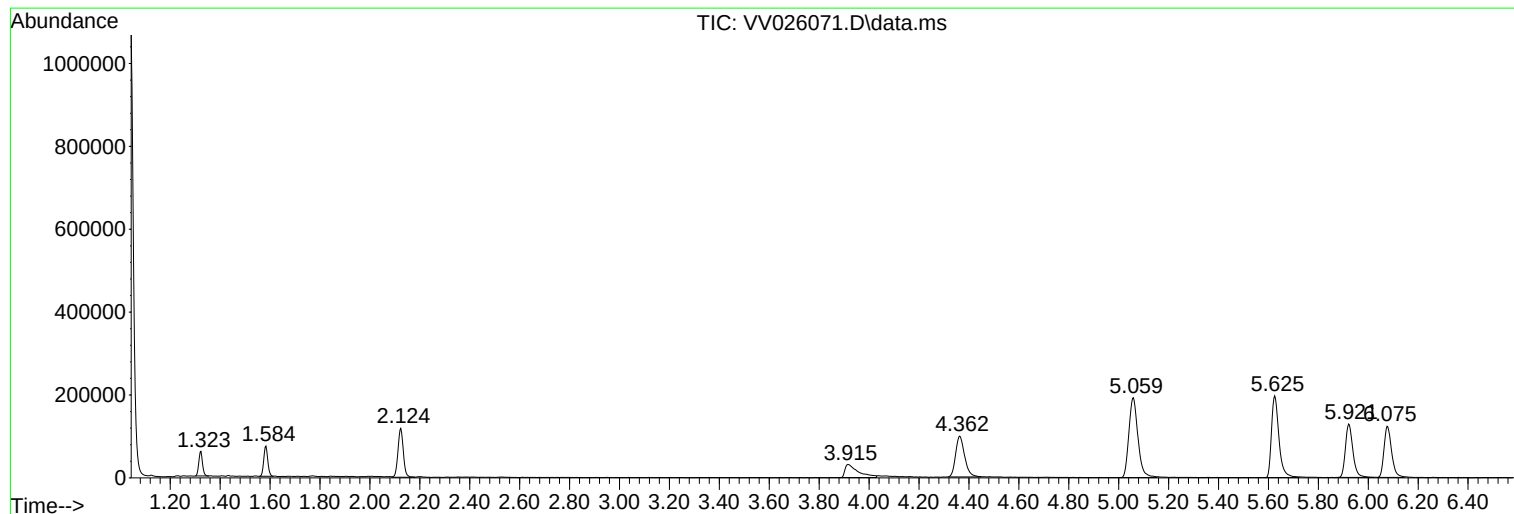

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026071.D
Acq On : 09 Jun 2022 22:32
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026071.D
Acq On : 09 Jun 2022 22:32
Operator : SY/MD
Sample : N3272-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
