

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026072.D
 Acq On : 09 Jun 2022 22:56
 Operator : SY/MD
 Sample : N3272-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	80	88	103	rVB	62515	66766	13.48%	1.503%
2	1.584	161	169	185	rVB	75244	86209	17.40%	1.941%
3	1.770	220	227	236	rVB	10919	14069	2.84%	0.317%
4	2.124	327	337	354	rVB	120542	173075	34.94%	3.897%
5	3.915	882	894	927	rBV	43273	156732	31.64%	3.529%
6	4.365	1017	1034	1059	rBV	97827	243815	49.22%	5.490%
7	5.060	1235	1250	1278	rBV3	196620	495340	100.00%	11.154%
8	5.625	1413	1426	1453	rBV	191792	396974	80.14%	8.939%
9	5.921	1506	1518	1545	rBV2	102050	215232	43.45%	4.847%
10	6.076	1553	1566	1593	rBV	127237	263698	53.24%	5.938%
11	6.995	1842	1852	1870	rBV2	42099	79911	16.13%	1.799%
12	7.320	1942	1953	1971	rBV	196460	348137	70.28%	7.839%
13	7.629	2040	2049	2075	rBV2	22987	44309	8.95%	0.998%
14	7.979	2152	2158	2174	rVB5	8857	15341	3.10%	0.345%
15	8.095	2184	2194	2230	rBV2	204223	484851	97.88%	10.918%
16	8.854	2418	2430	2459	rBV	291009	486273	98.17%	10.950%
17	10.217	2843	2854	2876	rBV	86410	140975	28.46%	3.174%
18	10.378	2895	2904	2916	rVB3	5494	8450	1.71%	0.190%
19	11.249	3163	3175	3194	rBV	248429	387490	78.23%	8.725%
20	11.625	3280	3292	3310	rBV	207983	333250	67.28%	7.504%




Sum of corrected areas: 4440897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026072.D
Acq On : 09 Jun 2022 22:56
Operator : SY/MD
Sample : N3272-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

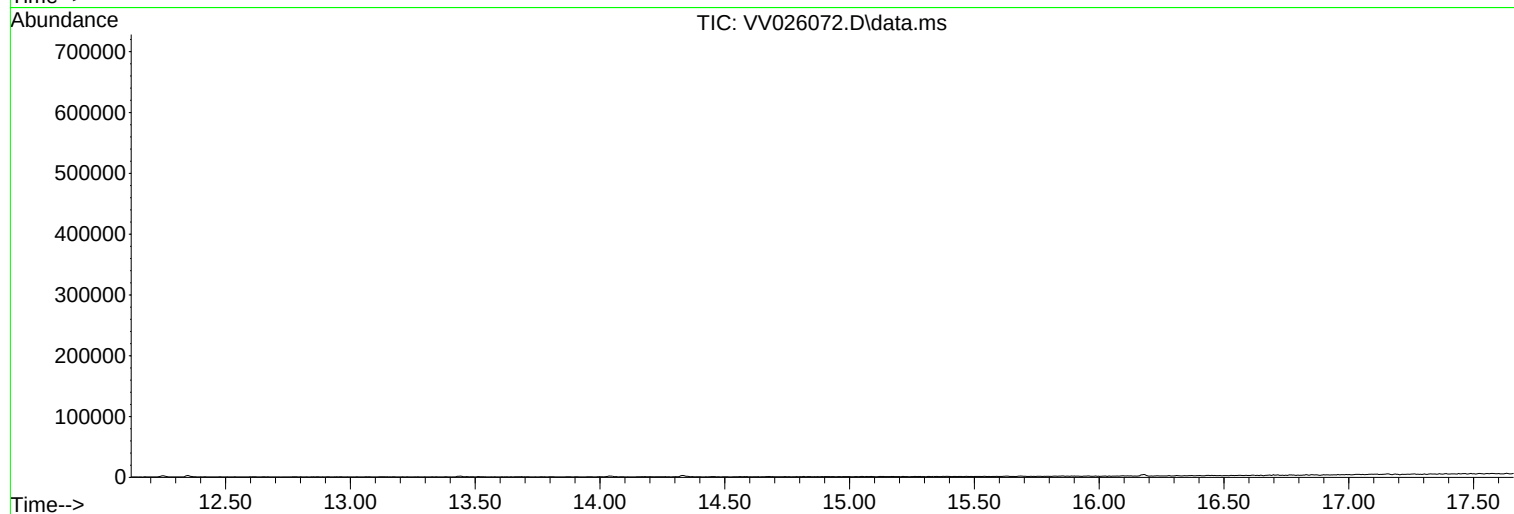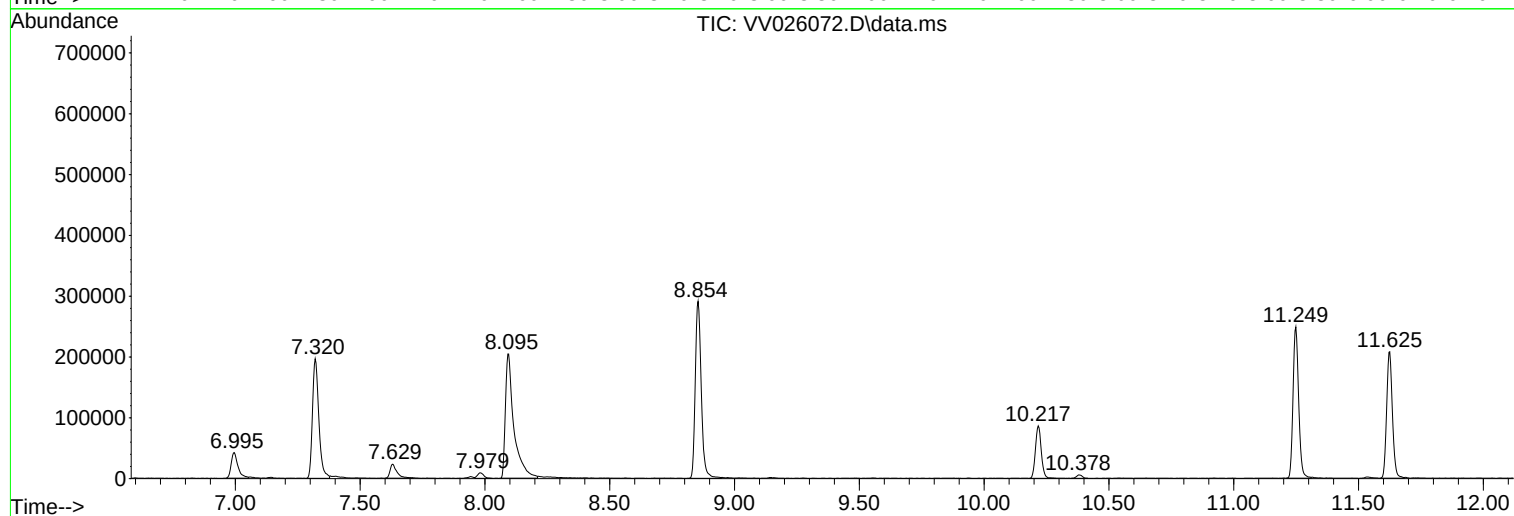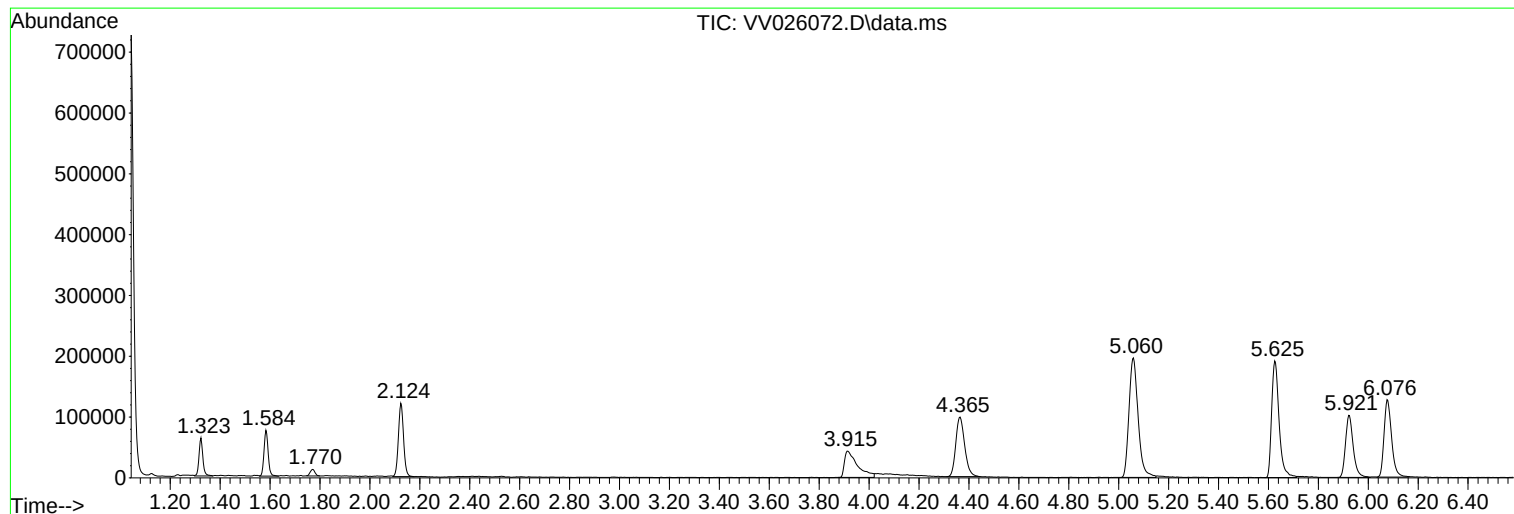

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026072.D
Acq On : 09 Jun 2022 22:56
Operator : SY/MD
Sample : N3272-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026072.D
Acq On : 09 Jun 2022 22:56
Operator : SY/MD
Sample : N3272-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc