

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026078.D
 Acq On : 10 Jun 2022 01:19
 Operator : SY/MD
 Sample : N3272-15
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B59

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	81	88	97	rVB	58916	61224	1.43%	0.623%
2	1.584	162	169	183	rVB	74124	85680	2.00%	0.872%
3	1.770	218	227	243	rVB	181688	238046	5.56%	2.424%
4	2.124	327	337	354	rVB	118437	176959	4.13%	1.802%
5	3.912	884	893	922	rBV2	42332	146774	3.43%	1.494%
6	4.365	1019	1034	1059	rVB2	101729	252561	5.90%	2.571%
7	5.059	1235	1250	1279	rBV2	196039	497106	11.61%	5.061%
8	5.625	1411	1426	1454	rBV	190031	401070	9.37%	4.083%
9	5.918	1503	1517	1554	rBV	2236491	4281265	100.00%	43.588%
10	6.075	1555	1566	1586	rVB	129527	267200	6.24%	2.720%
11	6.995	1842	1852	1876	rBV	42674	83492	1.95%	0.850%
12	7.320	1941	1953	1973	rBV	204733	364529	8.51%	3.711%
13	7.628	2039	2049	2071	rBV2	23816	47104	1.10%	0.480%
14	7.976	2136	2157	2180	rBV	601806	1022206	23.88%	10.407%
15	8.091	2184	2193	2230	rBV	213593	504578	11.79%	5.137%
16	8.853	2419	2430	2465	rBV	297698	497082	11.61%	5.061%
17	10.217	2843	2854	2871	rBV	92543	149556	3.49%	1.523%
18	11.249	3164	3175	3198	rBV	257553	402852	9.41%	4.101%
19	11.622	3280	3291	3317	rBV	214042	342907	8.01%	3.491%




Sum of corrected areas: 9822191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026078.D
Acq On : 10 Jun 2022 01:19
Operator : SY/MD
Sample : N3272-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

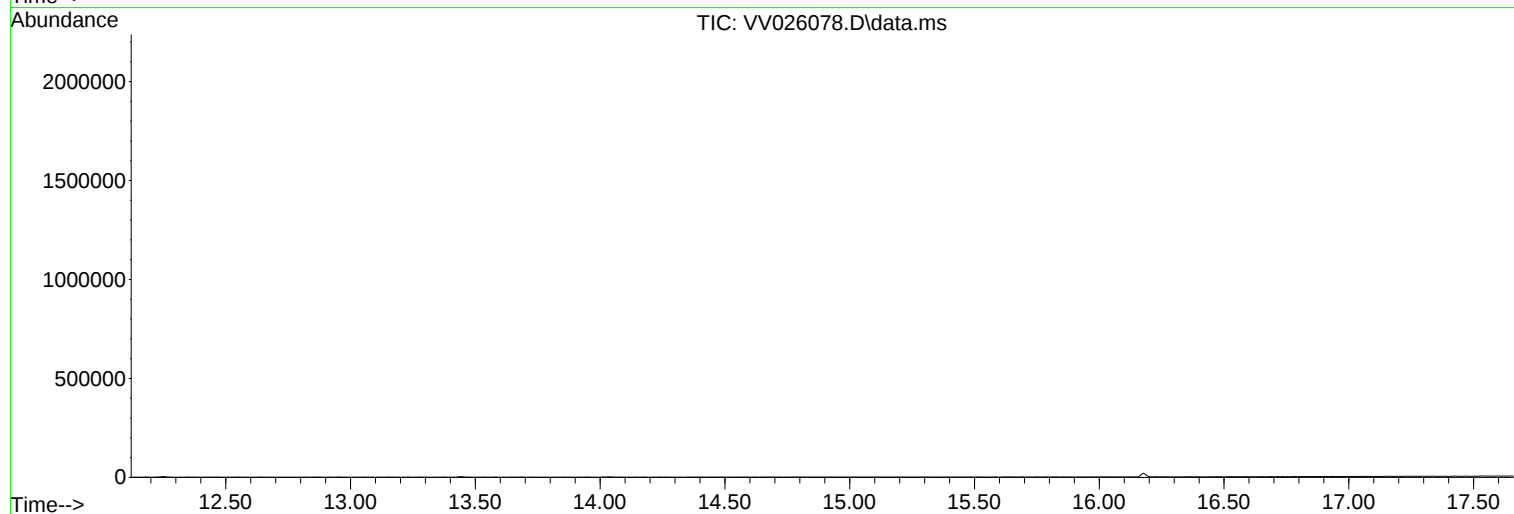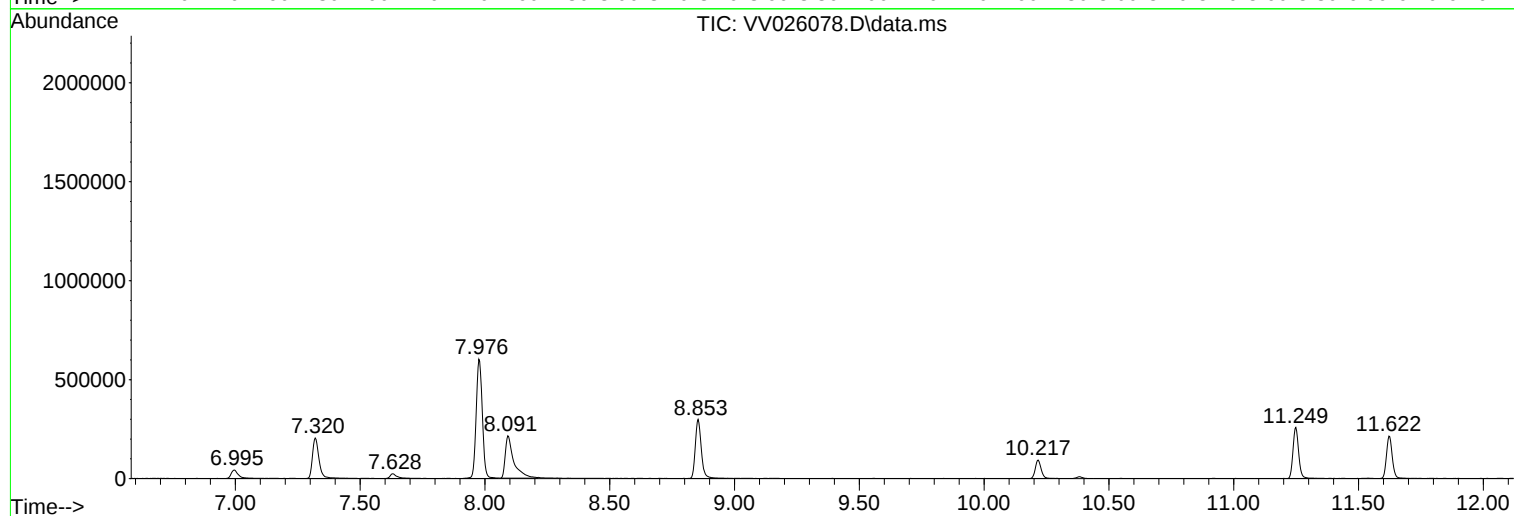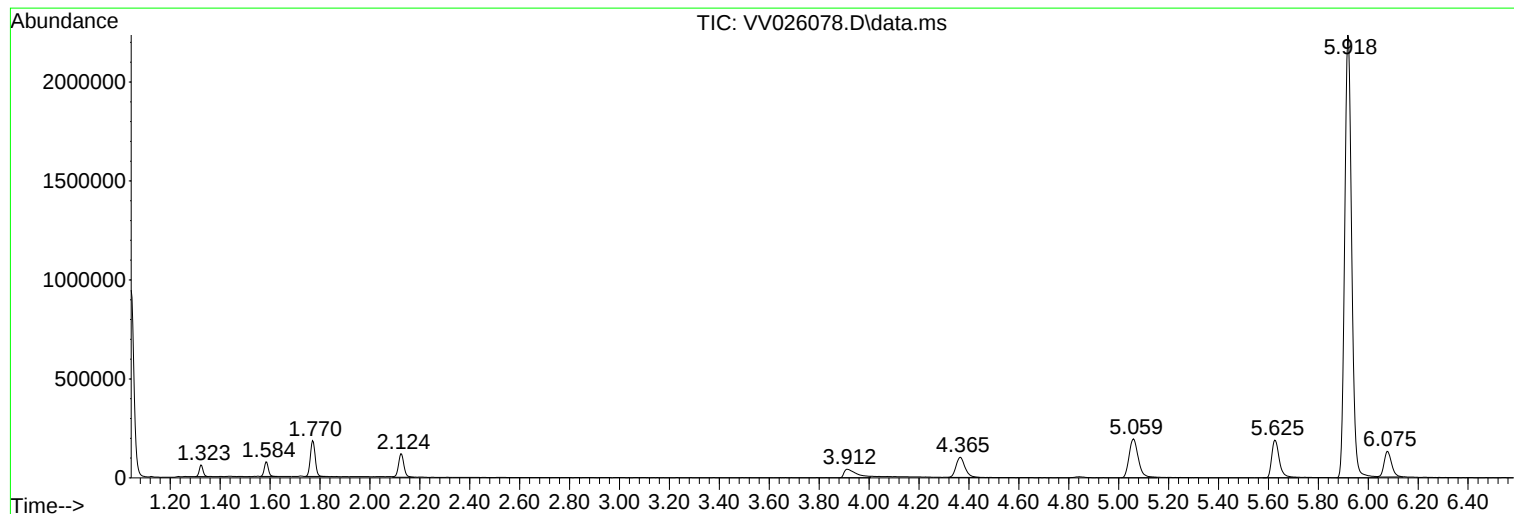

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026078.D
Acq On : 10 Jun 2022 01:19
Operator : SY/MD
Sample : N3272-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026078.D
Acq On : 10 Jun 2022 01:19
Operator : SY/MD
Sample : N3272-15
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc