

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026079.D
 Acq On : 10 Jun 2022 01:43
 Operator : SY/MD
 Sample : N3272-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B61

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026079.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.323	80	88	101	rVB	61454	65996	6.43%	1.255%
2	1.584	162	169	183	rVB	72567	84166	8.20%	1.600%
3	2.127	327	338	353	rVB	119748	179012	17.43%	3.404%
4	3.918	886	895	931	rBV	39361	154867	15.08%	2.945%
5	4.365	1019	1034	1059	rVB	99776	248932	24.24%	4.733%
6	5.059	1230	1250	1280	rBV2	194906	494966	48.21%	9.411%
7	5.625	1414	1426	1454	rBV	174765	370371	36.07%	7.042%
8	5.921	1503	1518	1554	rBV	513023	1026744	100.00%	19.523%
9	6.079	1554	1567	1585	rBV2	127462	261079	25.43%	4.964%
10	6.995	1840	1852	1874	rBV	40327	81136	7.90%	1.543%
11	7.320	1942	1953	1972	rBV	199369	355469	34.62%	6.759%
12	7.632	2040	2050	2066	rBV2	21894	41473	4.04%	0.789%
13	7.982	2150	2159	2171	rVB4	19254	33564	3.27%	0.638%
14	8.095	2183	2194	2237	rBV2	208905	500088	48.71%	9.509%
15	8.854	2418	2430	2453	rBV	282965	463375	45.13%	8.811%
16	10.217	2839	2854	2875	rBV	93091	149032	14.52%	2.834%
17	10.381	2896	2905	2918	rVB2	6634	10588	1.03%	0.201%
18	11.249	3162	3175	3198	rBV	244788	379636	36.97%	7.219%
19	11.622	3278	3291	3319	rBV	216635	339080	33.02%	6.447%
20	16.181	4700	4709	4720	rBV5	13154	19621	1.91%	0.373%




Sum of corrected areas: 5259195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026079.D
Acq On : 10 Jun 2022 01:43
Operator : SY/MD
Sample : N3272-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

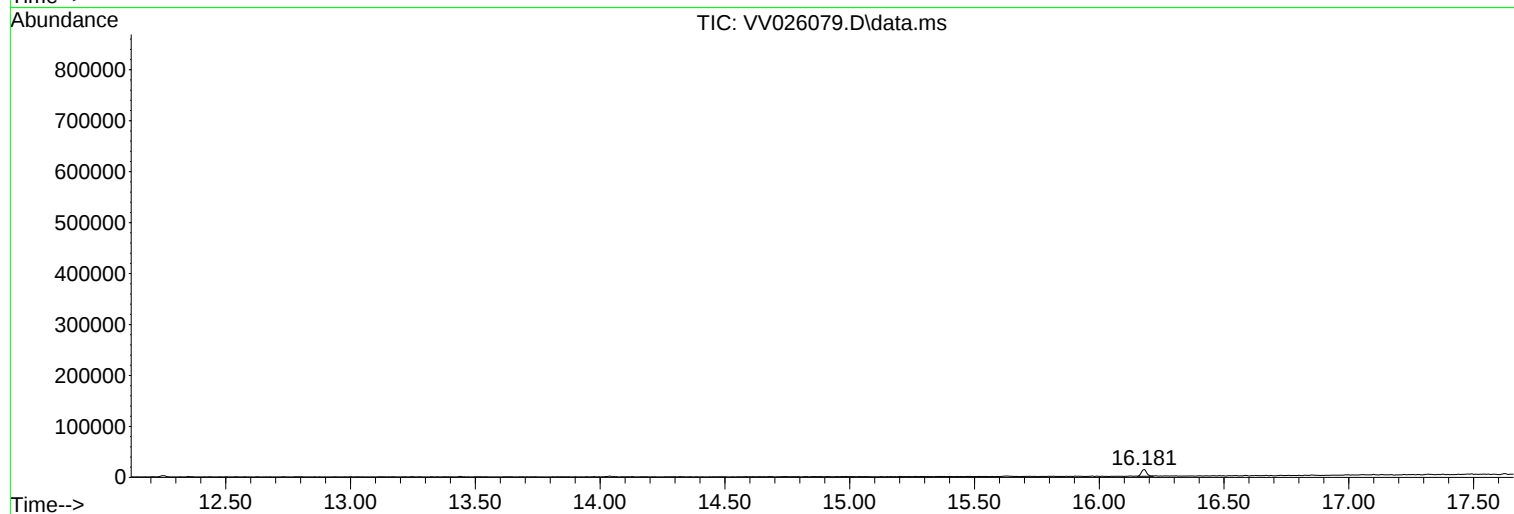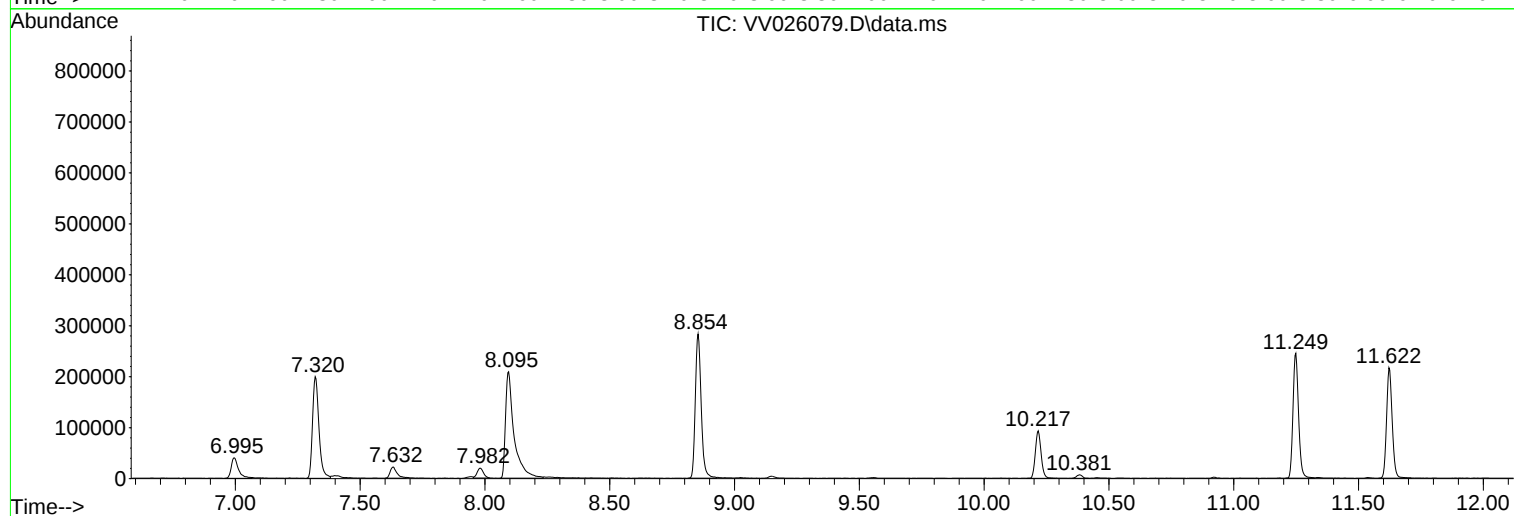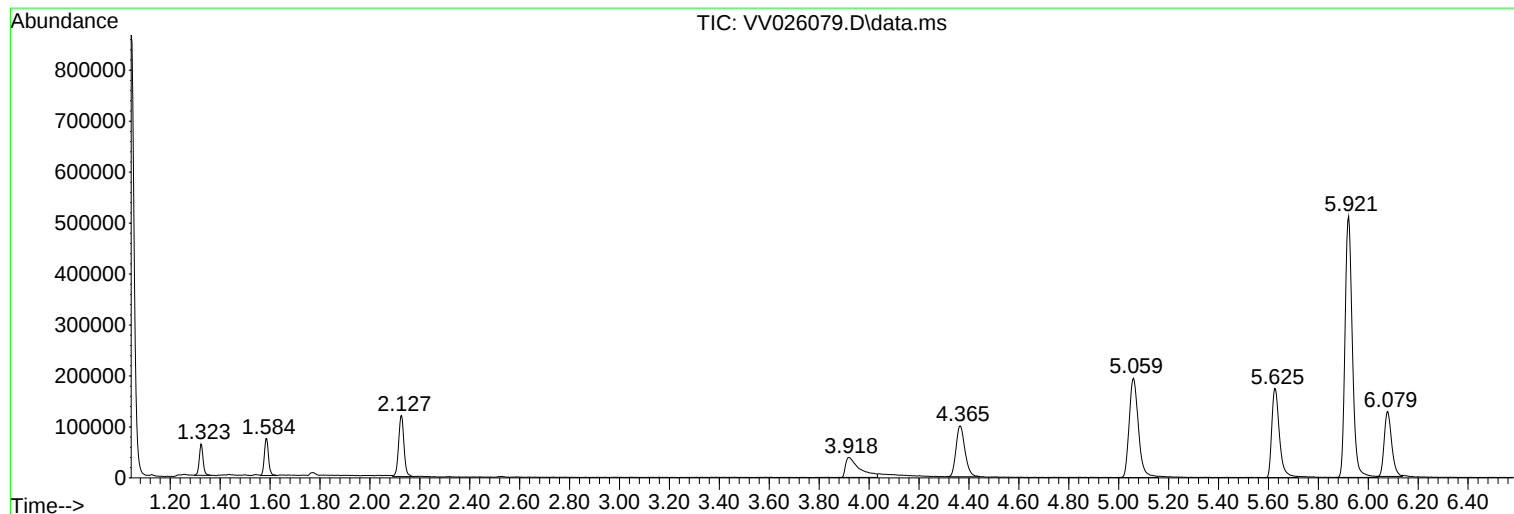

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026079.D
Acq On : 10 Jun 2022 01:43
Operator : SY/MD
Sample : N3272-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026079.D
Acq On : 10 Jun 2022 01:43
Operator : SY/MD
Sample : N3272-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc