

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026087.D
 Acq On : 10 Jun 2022 04:54
 Operator : SY/MD
 Sample : N3273-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B74

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	80	87	102	rVB	69018	74712	2.57%	0.991%
2	1.584	160	169	182	rBB	72973	83332	2.86%	1.105%
3	1.722	205	212	222	rVB	27262	32619	1.12%	0.433%
4	2.124	324	337	355	rVB	118193	178813	6.15%	2.372%
5	3.928	885	898	927	rBV3	80261	246646	8.48%	3.272%
6	4.362	1017	1033	1065	rVB2	100342	255760	8.79%	3.392%
7	5.056	1231	1249	1292	rBV3	196360	499068	17.16%	6.620%
8	5.625	1414	1426	1450	rBV	198095	412933	14.19%	5.477%
9	5.918	1503	1517	1554	rBV	1507495	2909131	100.00%	38.587%
10	6.075	1554	1566	1598	rVB	126319	269995	9.28%	3.581%
11	6.995	1839	1852	1875	rBV2	38385	75509	2.60%	1.002%
12	7.320	1941	1953	1971	rBV	201527	360592	12.40%	4.783%
13	7.632	2041	2050	2066	rBV2	20353	37706	1.30%	0.500%
14	7.976	2138	2157	2180	rBV	159670	277936	9.55%	3.687%
15	8.095	2184	2194	2232	rBV2	184518	425859	14.64%	5.649%
16	8.853	2419	2430	2459	rBV	315575	510187	17.54%	6.767%
17	10.217	2841	2854	2874	rBV	82372	134484	4.62%	1.784%
18	11.249	3159	3175	3191	rBV	268708	423418	14.55%	5.616%
19	11.622	3280	3291	3323	rVB	206197	330389	11.36%	4.382%




Sum of corrected areas: 7539089

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026087.D
Acq On : 10 Jun 2022 04:54
Operator : SY/MD
Sample : N3273-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

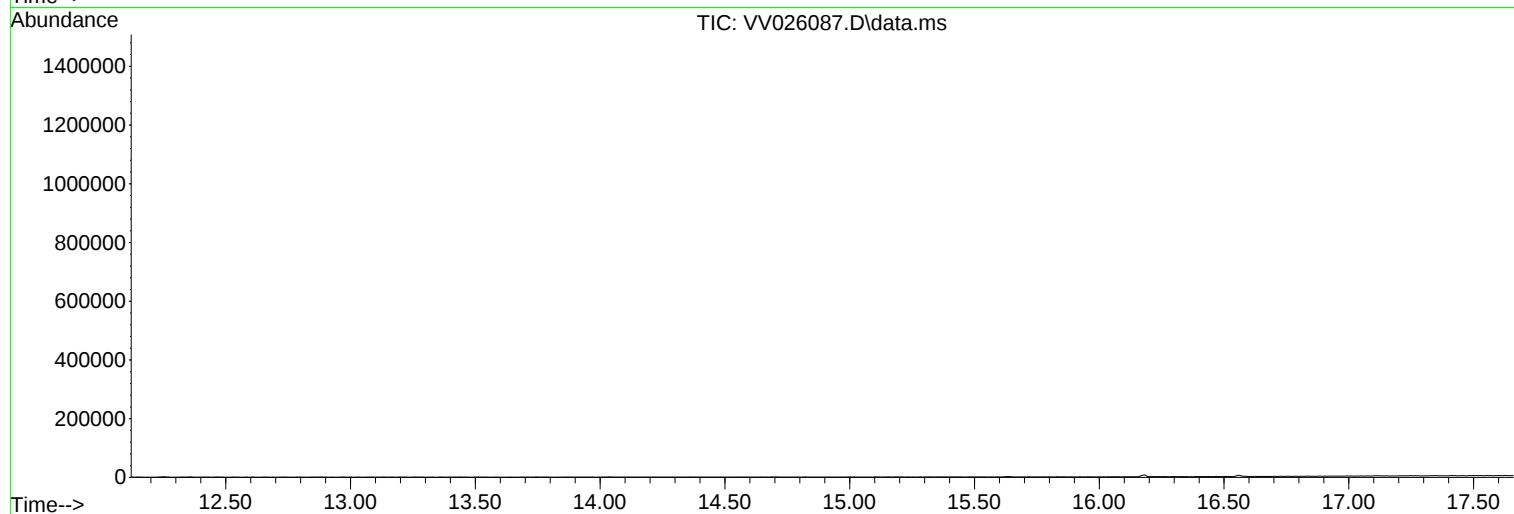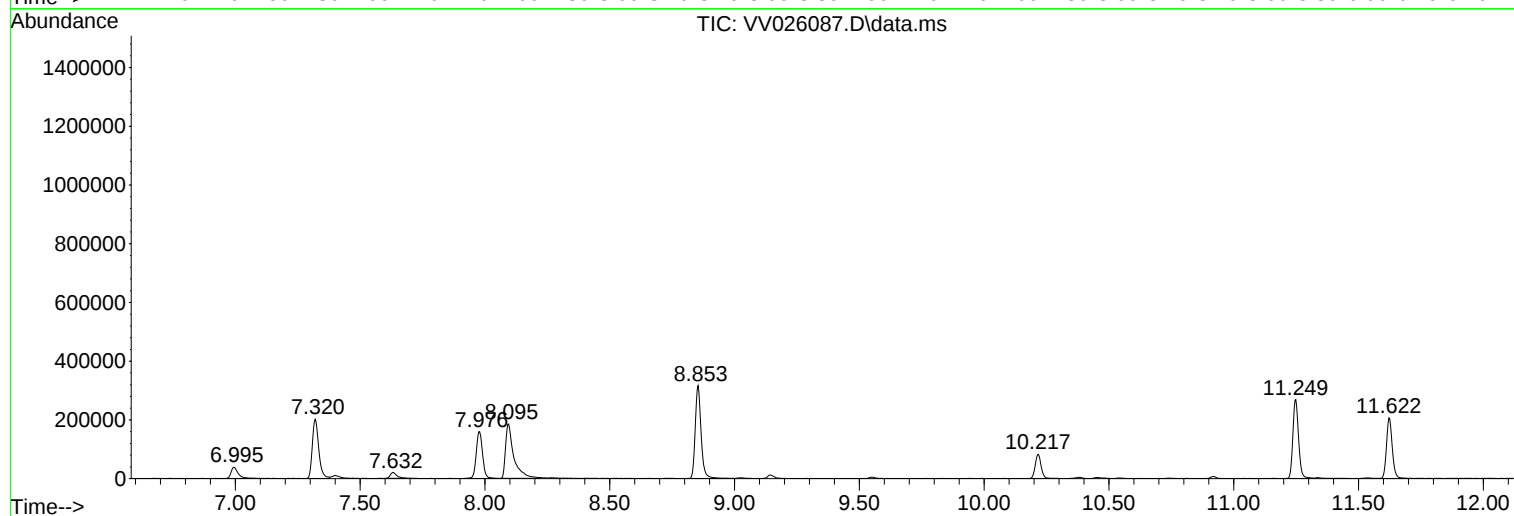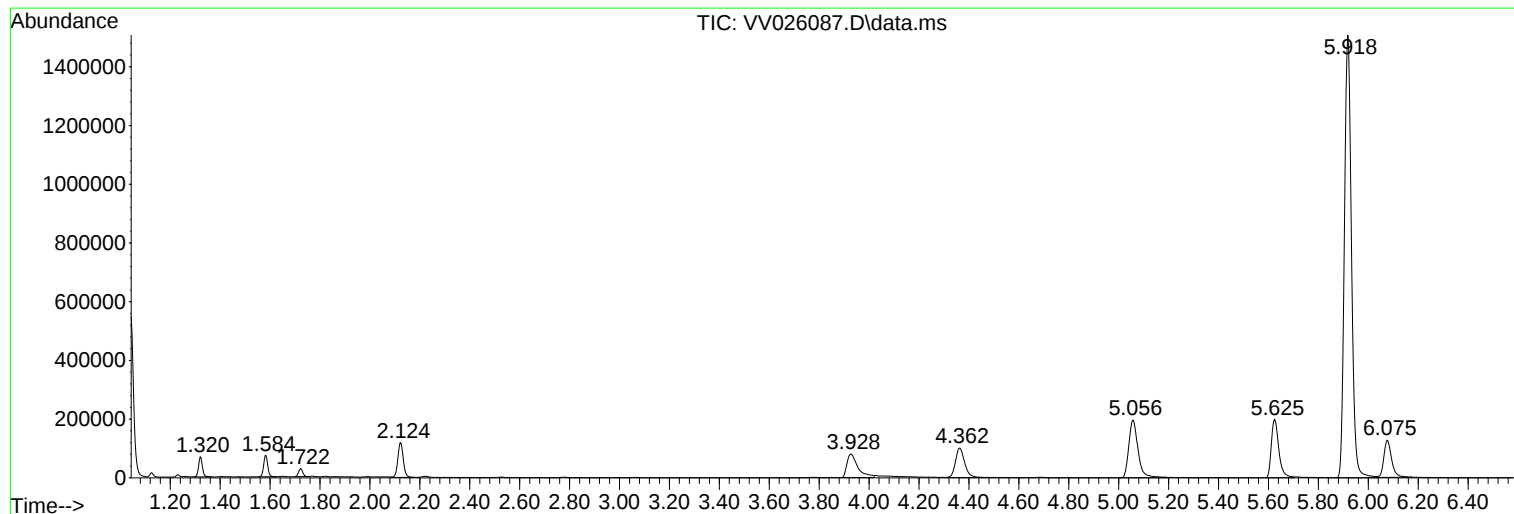

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026087.D
Acq On : 10 Jun 2022 04:54
Operator : SY/MD
Sample : N3273-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026087.D
Acq On : 10 Jun 2022 04:54
Operator : SY/MD
Sample : N3273-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc