

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026089.D
 Acq On : 10 Jun 2022 05:41
 Operator : SY/MD
 Sample : N3272-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B50

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	40	rVB	30976	36000	7.14%	0.791%
2	1.192	40	47	52	rBV	16825	18641	3.70%	0.409%
3	1.249	59	65	76	rVB	20013	20342	4.04%	0.447%
4	1.320	78	87	98	rVV	66651	79343	15.74%	1.743%
5	1.378	98	105	119	rVB2	28119	40123	7.96%	0.881%
6	1.581	152	168	182	rBV	73021	93928	18.63%	2.063%
7	2.121	326	336	351	rVB	117466	172497	34.22%	3.789%
8	3.921	886	896	938	rBV2	33569	165425	32.82%	3.633%
9	4.359	1017	1032	1067	rVB2	97373	251067	49.80%	5.514%
10	5.056	1233	1249	1279	rBV2	193453	488345	96.87%	10.725%
11	5.622	1412	1425	1456	rBV	197232	416775	82.68%	9.154%
12	5.921	1506	1518	1537	rBV2	80996	170865	33.89%	3.753%
13	6.076	1551	1566	1595	rBV	125694	263626	52.30%	5.790%
14	6.992	1838	1851	1876	rBV2	38238	74743	14.83%	1.642%
15	7.320	1942	1953	1977	rBV	195467	347593	68.95%	7.634%
16	7.629	2039	2049	2066	rBV2	19823	38434	7.62%	0.844%
17	8.095	2183	2194	2230	rBV2	198329	439360	87.16%	9.650%
18	8.854	2419	2430	2453	rBV	305089	504105	100.00%	11.072%
19	10.217	2842	2854	2868	rBV	84211	134047	26.59%	2.944%
20	10.381	2893	2905	2920	rBV	36456	59047	11.71%	1.297%
21	11.249	3163	3175	3194	rBV	266536	416899	82.70%	9.156%
22	11.622	3279	3291	3312	rBV	204410	321954	63.87%	7.071%




Sum of corrected areas: 4553159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026089.D
Acq On : 10 Jun 2022 05:41
Operator : SY/MD
Sample : N3272-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

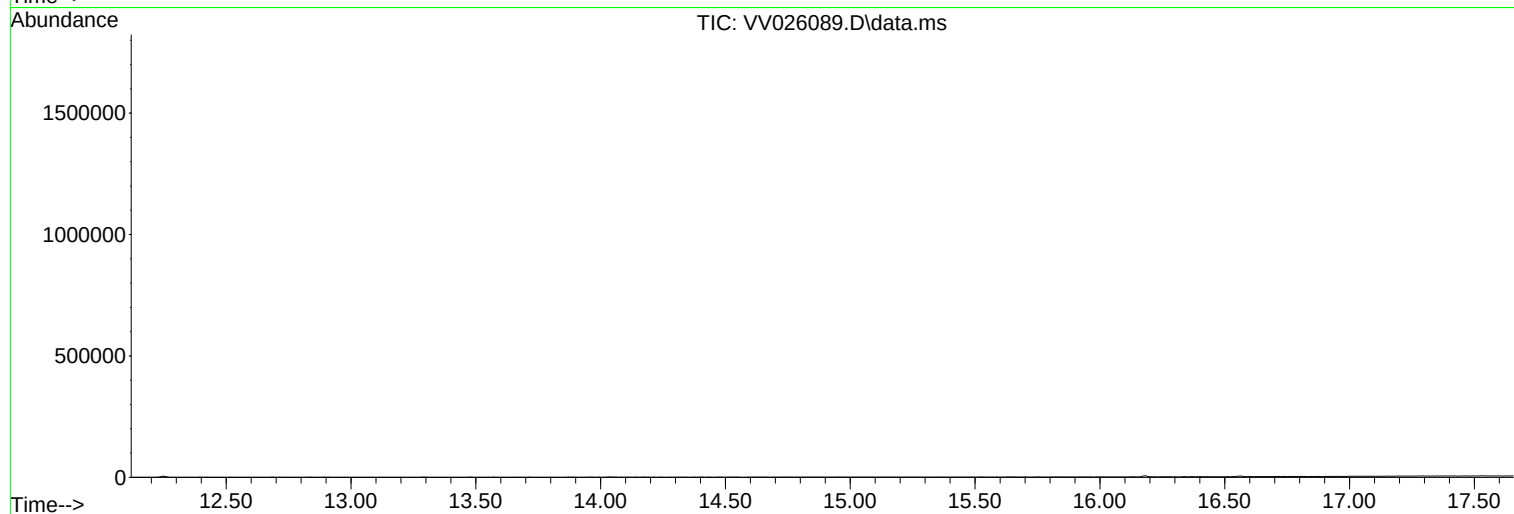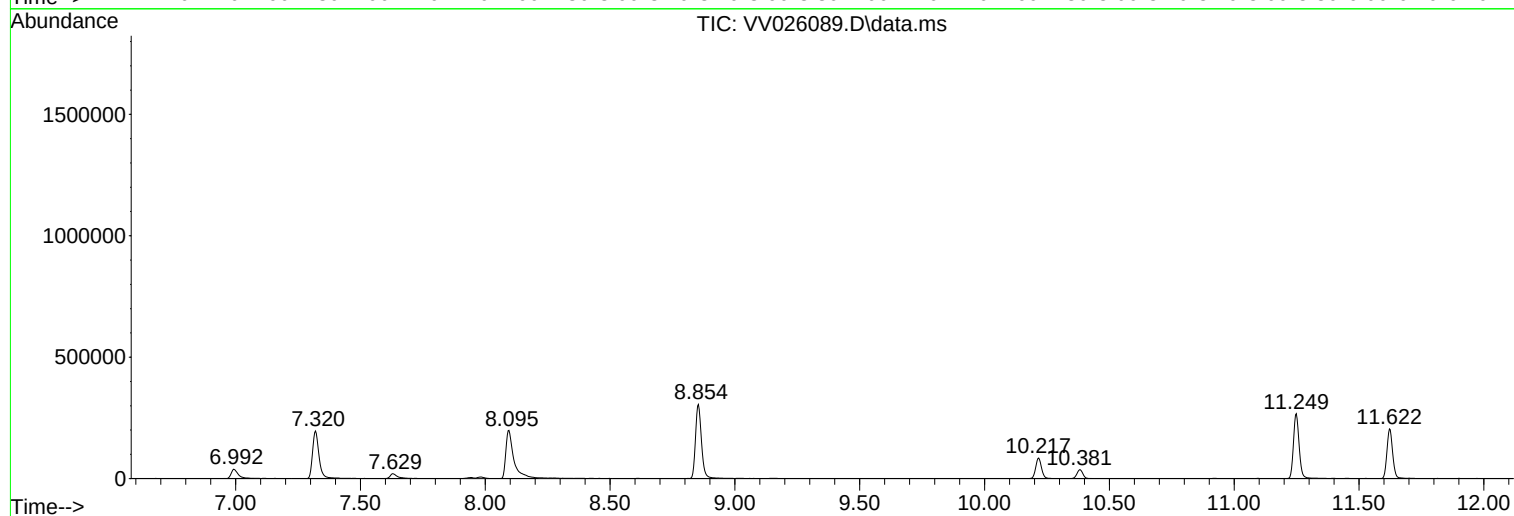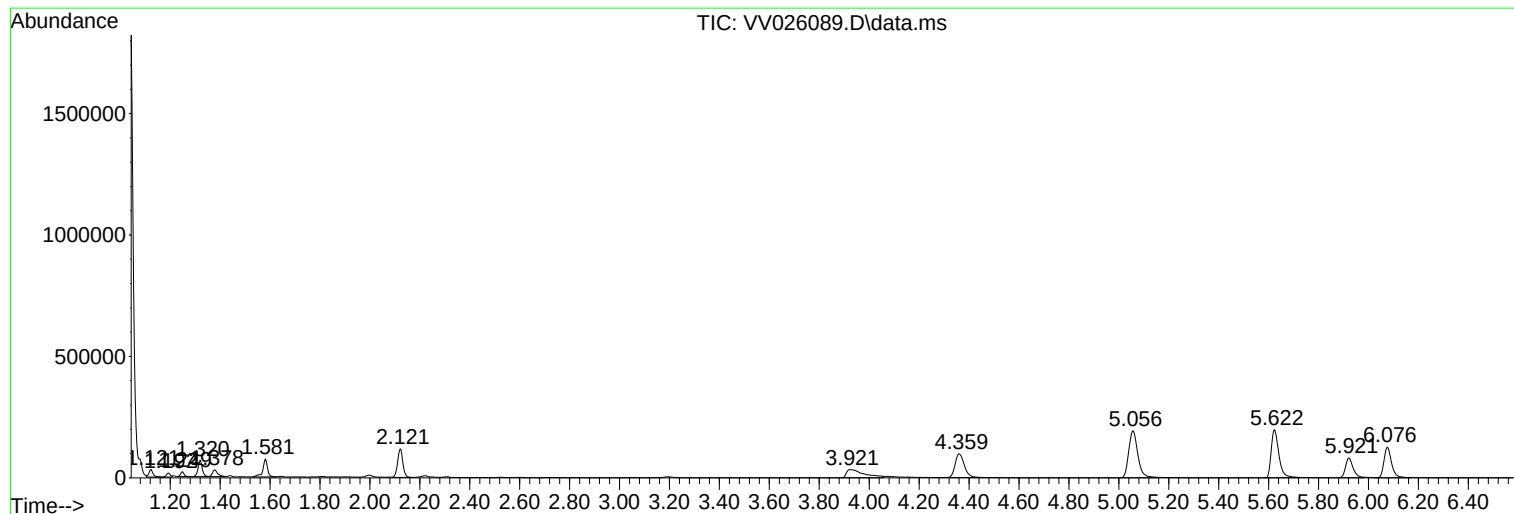

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026089.D
Acq On : 10 Jun 2022 05:41
Operator : SY/MD
Sample : N3272-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
Data File : VV026089.D
Acq On : 10 Jun 2022 05:41
Operator : SY/MD
Sample : N3272-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
