
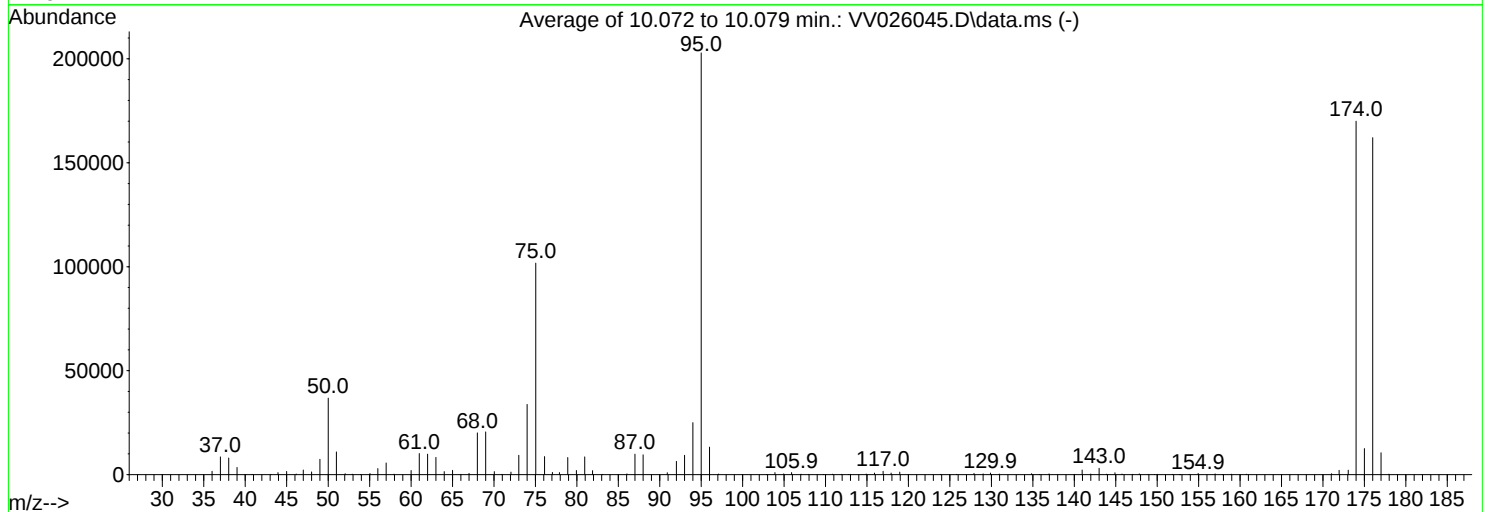


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060922\
 Data File : VV026045.D
 Acq On : 09 Jun 2022 08:51
 Operator : SY/MD
 Sample : BFB323
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB323

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Mon Jun 13 07:40:59 2022

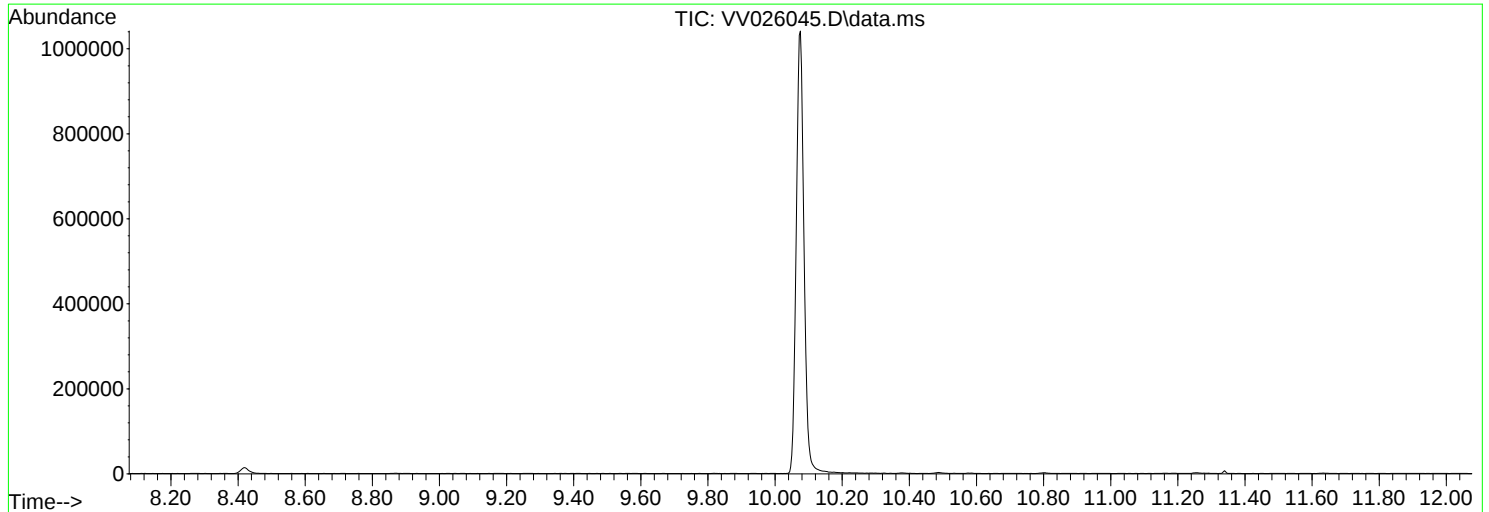

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	36819	PASS
75	95	30	80	50.1	101723	PASS
95	95	100	100	100.0	202859	PASS
96	95	5	9	6.5	13238	PASS
173	174	0.00	2	1.3	2162	PASS
174	95	50	120	83.8	170027	PASS
175	174	5	9	7.4	12556	PASS
176	174	95	105	95.3	162069	PASS
177	176	5	10	6.5	10550	PASS

m/z	Abundance
39.90	629.0
43.90	318.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323

m/z	Abundance
36.00	1681.0
37.00	8924.0
38.00	8271.0
39.00	3681.0
40.00	668.0
40.80	155.0
43.10	152.0
44.00	1436.0
45.00	1671.0
46.20	253.0
47.00	2284.0
48.00	1326.0
49.00	7634.0
50.00	38200.0
51.00	11425.0
52.10	504.0
52.90	338.0
53.90	109.0
55.10	634.0
56.00	3191.0
57.00	5880.0
57.90	246.0
60.00	1965.0
61.00	10460.0
62.00	10162.0
63.00	8583.0
64.00	1619.0
65.00	2154.0
66.00	179.0
67.00	664.0
68.00	20792.0
69.00	21184.0
70.00	1567.0
71.00	122.0
72.10	1247.0
73.00	9323.0
74.00	34488.0
75.00	105208.0
76.10	9013.0
77.10	1260.0
77.90	1063.0
78.90	8513.0
79.90	2022.0
80.90	8917.0
81.90	1967.0
83.10	191.0
86.10	356.0
87.00	10315.0
88.00	9820.0
90.90	919.0
92.00	6543.0
93.00	9712.0
94.00	25032.0
95.00	208320.0
96.00	13913.0
97.10	346.0
102.90	132.0
103.90	1034.0
104.90	414.0
105.90	1072.0
107.00	240.0
107.90	164.0
109.70	125.0
110.90	184.0
111.90	118.0
112.80	181.0
114.90	261.0
115.90	767.0
117.00	1668.0
117.90	784.0
118.90	1229.0
123.90	146.0
125.80	158.0
127.90	664.0
129.00	460.0
129.90	820.0
130.90	327.0
134.90	448.0
137.00	396.0
140.00	192.0
141.00	2263.0
142.00	313.0
143.00	3136.0
143.90	214.0
144.90	1021.0
145.80	333.0
147.10	157.0
147.80	436.0
148.90	170.0
150.00	256.0
151.90	118.0
152.70	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323

153.90	203.0
154.90	633.0
157.00	428.0
159.00	247.0
160.80	178.0
171.00	419.0
172.00	2202.0
173.10	2143.0
174.00	172032.0
175.00	12770.0
176.00	162496.0
177.00	10704.0
177.90	255.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323

m/z	Abundance
36.00	1686.0
37.00	8872.0
38.00	8259.0
39.00	3483.0
40.00	635.0
40.80	164.0
43.10	138.0
44.00	1389.0
45.00	1567.0
46.20	290.0
47.00	2257.0
48.00	1400.0
49.00	7609.0
50.00	37976.0
51.00	11291.0
52.00	490.0
52.90	265.0
53.90	108.0
55.10	603.0
56.00	3023.0
57.00	5869.0
57.90	262.0
60.00	2137.0
61.00	10438.0
62.00	10264.0
63.00	8576.0
64.00	1471.0
65.00	2131.0
66.00	168.0
67.00	650.0
68.00	20600.0
69.00	21136.0
70.10	1557.0
71.00	126.0
72.00	1247.0
73.00	9624.0
74.00	34704.0
75.00	104632.0
76.10	9022.0
77.00	1121.0
77.90	1011.0
78.90	8440.0
80.00	2086.0
80.90	8836.0
81.90	1991.0
83.10	199.0
86.00	351.0
87.00	10118.0
88.00	9913.0
90.90	956.0
92.00	6647.0
93.00	9557.0
94.00	25760.0
95.00	209984.0
96.00	13681.0
97.10	361.0
102.90	111.0
103.90	1001.0
105.00	357.0
105.90	1090.0
107.10	209.0
107.90	207.0
109.80	102.0
110.90	206.0
111.90	132.0
113.00	189.0
114.90	331.0
115.90	768.0
116.90	1675.0
117.90	842.0
118.90	1278.0
123.90	195.0
125.80	157.0
127.90	668.0
129.00	430.0
129.90	821.0
131.00	361.0
134.90	453.0
135.80	122.0
136.90	407.0
140.00	169.0
141.00	2342.0
142.00	331.0
143.00	3139.0
143.90	256.0
144.90	976.0
145.80	297.0
147.00	156.0
147.90	403.0
148.90	169.0
150.00	199.0
151.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323

153.90	176.0
154.90	621.0
157.00	423.0
158.90	256.0
160.70	215.0
171.10	481.0
172.00	2195.0
173.00	2247.0
174.00	175808.0
175.00	12997.0
176.00	167360.0
177.00	10936.0
177.90	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323

m/z	Abundance
36.00	1517.0
37.00	7865.0
38.00	7544.0
39.00	3168.0
40.00	627.0
40.80	166.0
43.10	125.0
44.00	1262.0
45.00	1395.0
46.10	321.0
47.00	2141.0
48.00	1269.0
49.00	7039.0
50.00	34280.0
51.00	10091.0
52.00	458.0
52.90	210.0
53.90	110.0
55.00	506.0
56.00	2528.0
57.00	5209.0
58.00	279.0
60.00	1929.0
61.00	9486.0
62.00	9240.0
63.00	7804.0
64.00	1224.0
65.00	1913.0
66.00	144.0
67.00	542.0
68.00	18792.0
69.00	19368.0
70.10	1373.0
70.90	132.0
72.00	1222.0
73.00	8972.0
74.00	32136.0
75.10	95328.0
76.10	8157.0
77.10	944.0
77.90	886.0
78.90	7687.0
80.00	1995.0
81.00	7848.0
81.90	1934.0
83.10	186.0
86.00	384.0
87.00	9190.0
88.00	8880.0
90.90	875.0
92.00	6080.0
93.00	8739.0
94.00	24184.0
95.00	190272.0
96.00	12121.0
97.10	345.0
103.90	886.0
104.90	321.0
105.90	901.0
107.10	166.0
108.00	205.0
110.80	238.0
111.90	177.0
113.00	234.0
114.90	324.0
115.90	725.0
116.90	1579.0
117.90	796.0
119.00	1252.0
123.90	183.0
125.80	139.0
127.90	620.0
129.00	370.0
129.90	729.0
131.00	334.0
134.80	419.0
135.80	102.0
136.90	392.0
140.00	156.0
140.90	2152.0
142.00	323.0
143.00	2880.0
143.90	236.0
144.90	822.0
145.70	258.0
147.00	149.0
147.90	383.0
148.90	158.0
149.70	216.0
151.80	137.0
153.80	143.0
155.00	557.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323

157.00	393.0
157.90	107.0
158.90	278.0
160.70	239.0
171.10	464.0
171.90	1959.0
173.00	2095.0
174.00	162240.0
175.00	11902.0
176.00	156352.0
177.00	10010.0
178.00	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB323