

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060923\
 Data File : VW031489.D
 Acq On : 09 Jun 2023 12:13
 Operator : SY/MD
 Sample : 03098-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP9

Quant Time: Jun 10 01:40:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 10 01:38:32 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	222804	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	230221	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	107670	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	69830	35.622	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	71.240%		
7) Chloroethane-d5	1.532	69	72811	45.877	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	91.760%		
11) 1,1-Dichloroethene-d2	2.063	65	39901	42.947	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	85.900%		
21) 2-Butanone-d5	3.793	46	128922	91.002	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	91.000%		
24) Chloroform-d	4.256	84	181704	48.729	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	97.460%		
26) 1,2-Dichloroethane-d4	4.947	65	126663	50.635	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	101.260%		
32) Benzene-d6	4.966	84	318400	46.844	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	93.680%		
36) 1,2-Dichloropropane-d6	5.995	67	117091	49.560	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	99.120%		
41) Toluene-d8	7.249	98	269167	43.109	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	86.220%		
43) trans-1,3-Dichloroprop...	7.558	79	49034	41.202	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	82.400%		
47) 2-Hexanone-d5	8.030	63	66681	74.936	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	74.940%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	130014	43.605	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	87.220%		
66) 1,2-Dichlorobenzene-d4	11.567	152	111622	55.886	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	111.780%		
Target Compounds						
48) 2-Hexanone	8.085	43	14919	6.417	ug/L #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031489.D
 Acq On : 09 Jun 2023 12:13
 Operator : SY/MD
 Sample : 03098-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP9

Quant Time: Jun 10 01:40:20 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Jun 10 01:38:32 2023
 Response via : Initial Calibration

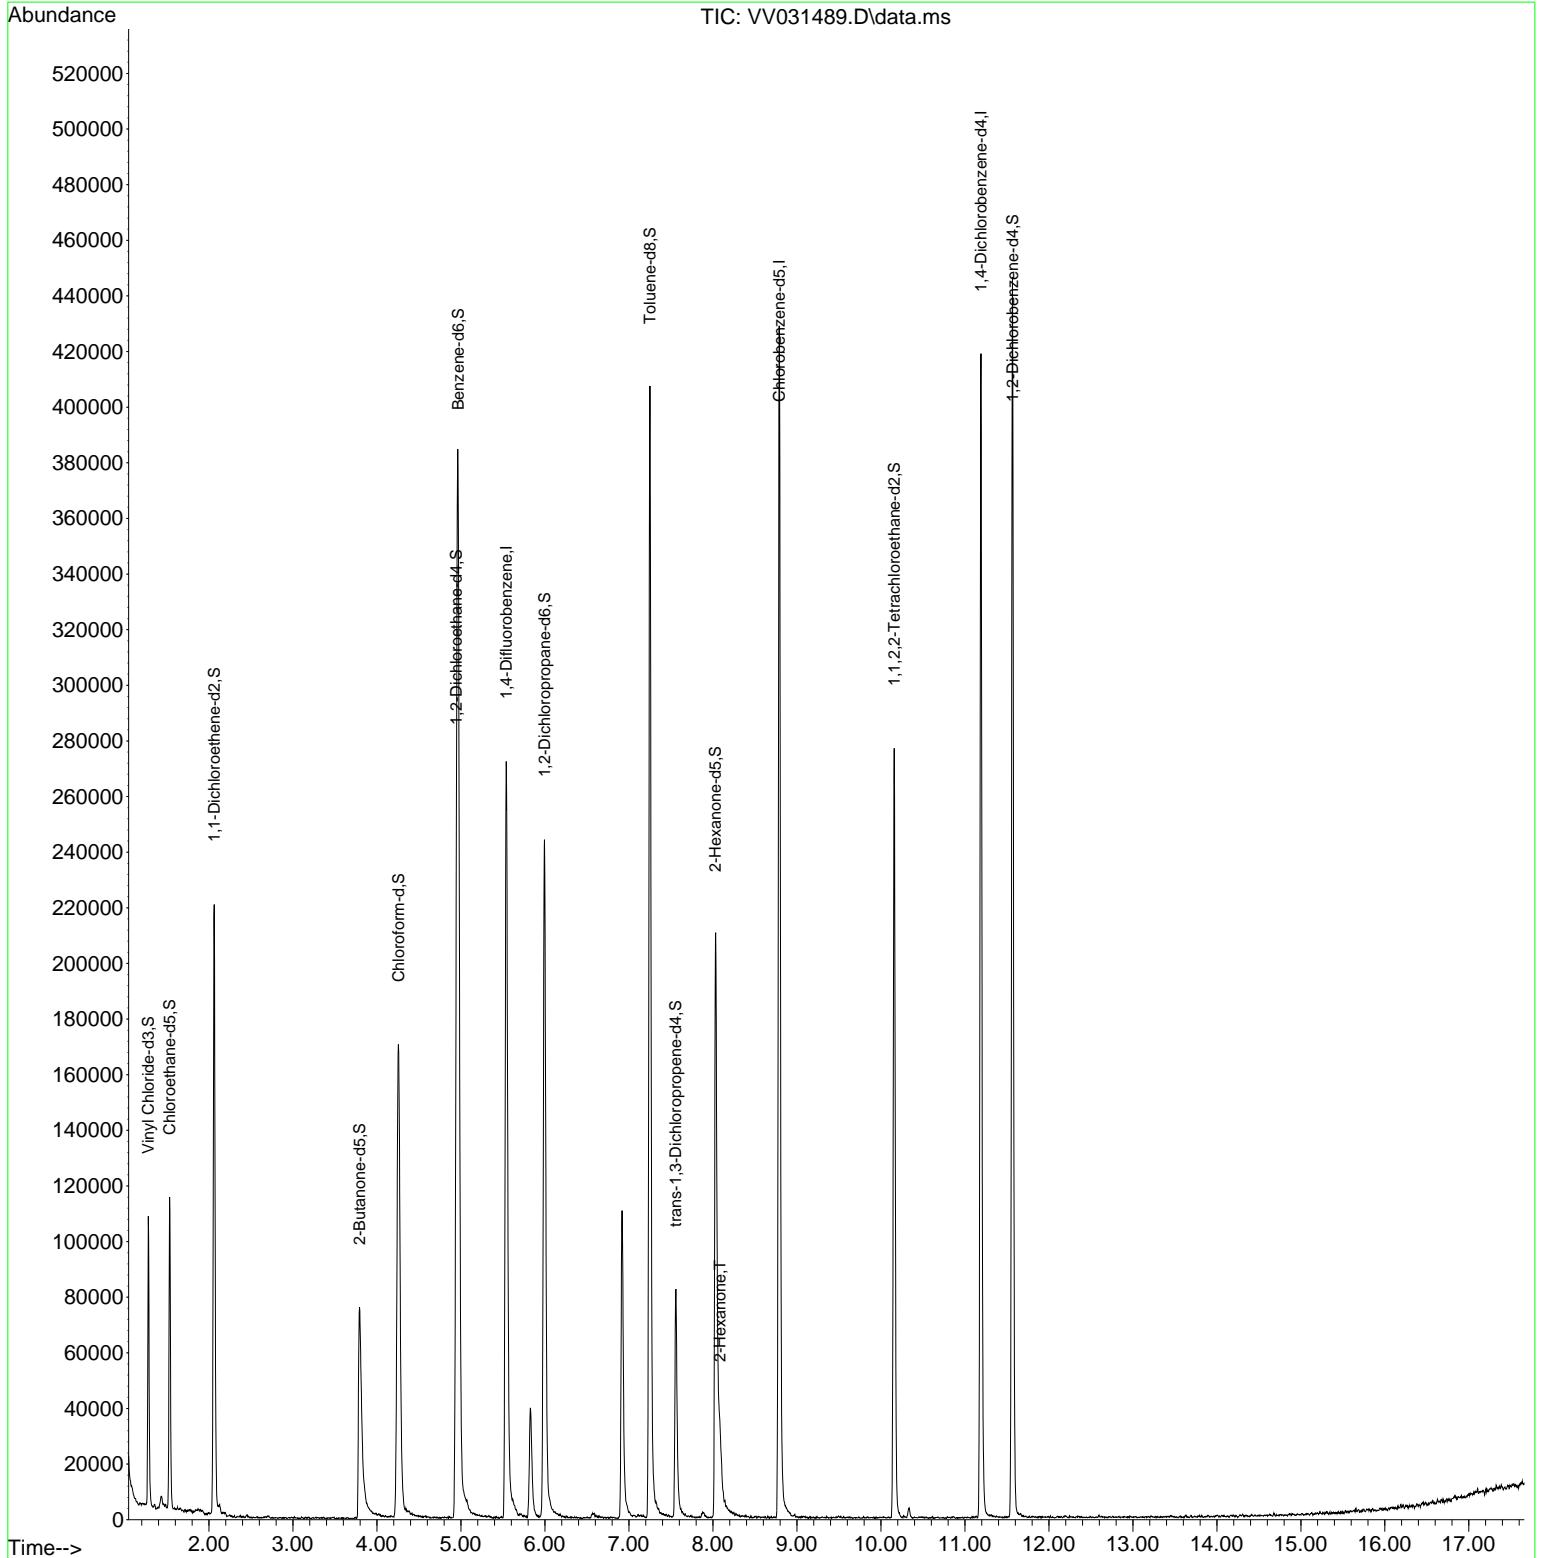

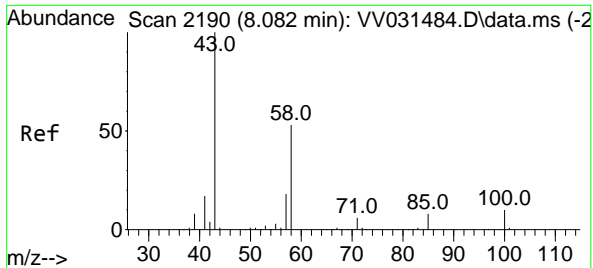

#48
 2-Hexanone
 Concen: 6.417 ug/L
 RT: 8.085 min Scan# 2191
 Delta R.T. 0.003 min
 Lab File: VV031489.D
 Acq: 09 Jun 2023 12:13

Instrument : MSVOA_V
 ClientSampleId : EZE9

Tgt Ion: 43 Resp: 14919

Ion	Ratio	Lower	Upper
43	100		
58	28.2	42.9	64.3#
57	15.3	14.6	22.0
100	9.0	8.2	12.2

