

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031485.D
 Acq On : 09 Jun 2023 10:40
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	119371	129795	12.49%	1.705%
2	1.532	146	153	166	rVB	120789	139591	13.43%	1.834%
3	2.063	308	318	334	rBV	236618	349553	33.63%	4.593%
4	2.416	427	428	431	rVB2	489	228	0.02%	0.003%
5	2.452	431	439	440	rBV5	2370	2569	0.25%	0.034%
6	2.587	479	481	484	rBV	290	176	0.02%	0.002%
7	2.654	499	502	507	rVB3	377	331	0.03%	0.004%
8	2.680	507	510	512	rBV2	782	290	0.03%	0.004%
9	2.693	512	514	517	rBV2	320	162	0.02%	0.002%
10	2.725	522	524	527	rVV	317	132	0.01%	0.002%
11	2.751	530	532	533	rBV	385	170	0.02%	0.002%
12	2.793	543	545	547	rVB	477	170	0.02%	0.002%
13	2.805	547	549	552	rVB2	415	237	0.02%	0.003%
14	2.821	552	554	556	rBV2	312	177	0.02%	0.002%
15	2.841	559	560	561	rBV	264	88	0.01%	0.001%
16	2.883	571	573	576	rBV	288	191	0.02%	0.003%
17	2.937	588	590	593	rVB2	176	86	0.01%	0.001%
18	2.960	593	597	598	rBV2	351	163	0.02%	0.002%
19	2.976	600	602	605	rBV	235	153	0.01%	0.002%
20	3.037	619	621	625	rVB	297	189	0.02%	0.002%
21	3.095	637	639	641	rVB2	466	220	0.02%	0.003%
22	3.230	679	681	682	rBV2	141	67	0.01%	0.001%
23	3.236	682	683	685	rVV2	288	108	0.01%	0.001%
24	3.265	689	692	693	rBV	205	112	0.01%	0.001%
25	3.278	693	696	697	rBV	268	118	0.01%	0.002%
26	3.330	708	712	718	rBV3	497	584	0.06%	0.008%
27	3.387	728	730	732	rBV	224	88	0.01%	0.001%
28	3.416	734	739	742	rVV2	209	207	0.02%	0.003%
29	3.465	751	754	756	rBV2	423	262	0.03%	0.003%
30	3.503	764	766	767	rBV	223	71	0.01%	0.001%
31	3.616	799	801	803	rBV	231	109	0.01%	0.001%
32	3.632	803	806	808	rBV2	234	171	0.02%	0.002%
33	3.693	822	825	826	rBV	317	143	0.01%	0.002%
34	3.725	833	835	836	rBV	204	93	0.01%	0.001%
35	3.754	842	844	845	rBV	175	39	0.00%	0.001%
36	3.799	848	858	893	rBV2	76344	234025	22.51%	3.075%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031485.D
 Acq On : 09 Jun 2023 10:40
 Operator : SY/MD
 Sample : VV0609WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	4.256	985	1000	1029	rBV	170848	447743	43.07%	5.883%
38	4.564	1094	1096	1099	rBV2	390	226	0.02%	0.003%
39	4.686	1132	1134	1135	rBV	361	151	0.01%	0.002%
40	4.812	1170	1173	1175	rBV	216	147	0.01%	0.002%
41	4.873	1187	1192	1197	rBV4	550	682	0.07%	0.009%
42	4.963	1203	1220	1242	rBV2	391041	1039523	100.00%	13.659%
43	5.329	1332	1334	1335	rBV	437	200	0.02%	0.003%
44	5.374	1346	1348	1353	rBV2	441	268	0.03%	0.004%
45	5.448	1369	1371	1374	rVB3	838	358	0.03%	0.005%
46	5.471	1374	1378	1380	rBV2	428	354	0.03%	0.005%
47	5.538	1387	1399	1429	rBV	260073	562755	54.14%	7.394%
48	5.828	1477	1489	1506	rBV2	40617	90128	8.67%	1.184%
49	5.995	1526	1541	1560	rBV	244956	513406	49.39%	6.746%
50	6.458	1682	1685	1686	rBV	348	158	0.02%	0.002%
51	6.468	1686	1688	1691	rVB2	716	362	0.03%	0.005%
52	6.519	1701	1704	1706	rBV2	535	341	0.03%	0.004%
53	6.857	1807	1809	1811	rBV2	198	97	0.01%	0.001%
54	6.918	1816	1828	1848	rBV	108082	209525	20.16%	2.753%
55	7.249	1919	1931	1960	rBV	406586	733357	70.55%	9.636%
56	7.558	2018	2027	2048	rBV	81129	149186	14.35%	1.960%
57	7.844	2109	2116	2120	rBV4	554	749	0.07%	0.010%
58	7.908	2133	2136	2138	rBV3	794	490	0.05%	0.006%
59	7.943	2144	2147	2148	rBV	331	124	0.01%	0.002%
60	8.001	2162	2165	2166	rBV	397	220	0.02%	0.003%
61	8.033	2166	2175	2210	rBV2	204688	485126	46.67%	6.374%
62	8.339	2267	2270	2275	rVB5	1010	969	0.09%	0.013%
63	8.468	2307	2310	2312	rBV2	556	309	0.03%	0.004%
64	8.525	2324	2328	2329	rBV3	430	266	0.03%	0.003%
65	8.789	2399	2410	2441	rBV	427801	727542	69.99%	9.559%
66	8.985	2468	2471	2475	rBV4	798	605	0.06%	0.008%
67	9.168	2525	2528	2529	rBV	317	179	0.02%	0.002%
68	9.213	2539	2542	2544	rBV	319	201	0.02%	0.003%
69	9.304	2565	2570	2571	rBV2	325	235	0.02%	0.003%
70	9.451	2613	2616	2623	rBV4	655	785	0.08%	0.010%
71	9.699	2691	2693	2696	rVB2	534	233	0.02%	0.003%
72	9.879	2745	2749	2754	rVB2	1059	898	0.09%	0.012%
73	9.940	2764	2768	2770	rBV2	382	274	0.03%	0.004%
74	9.979	2778	2780	2781	rBV	230	85	0.01%	0.001%
75	9.988	2781	2783	2786	rVB2	300	131	0.01%	0.002%
76	10.021	2790	2793	2796	rBV4	1268	1044	0.10%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031485.D
Acq On : 09 Jun 2023 10:40
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK353

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

77	10.159	2823	2836	2855	rBV	265668	431535	41.51%	5.670%
78	10.310	2882	2883	2886	rBV	295	181	0.02%	0.002%
79	10.487	2937	2938	2943	rVB3	418	278	0.03%	0.004%
80	10.644	2985	2987	2989	rBV2	502	234	0.02%	0.003%
81	10.953	3081	3083	3084	rBV	276	88	0.01%	0.001%
82	11.098	3125	3128	3131	rBV	410	260	0.03%	0.003%
83	11.111	3131	3132	3133	rVB	283	59	0.01%	0.001%
84	11.191	3146	3157	3177	rBV	409316	651196	62.64%	8.556%
85	11.567	3261	3274	3294	rBV	433998	696062	66.96%	9.146%
86	11.982	3400	3403	3404	rBV	533	294	0.03%	0.004%
87	12.647	3607	3610	3611	rBV2	413	206	0.02%	0.003%




Sum of corrected areas: 7610693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031485.D
Acq On : 09 Jun 2023 10:40
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK353

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

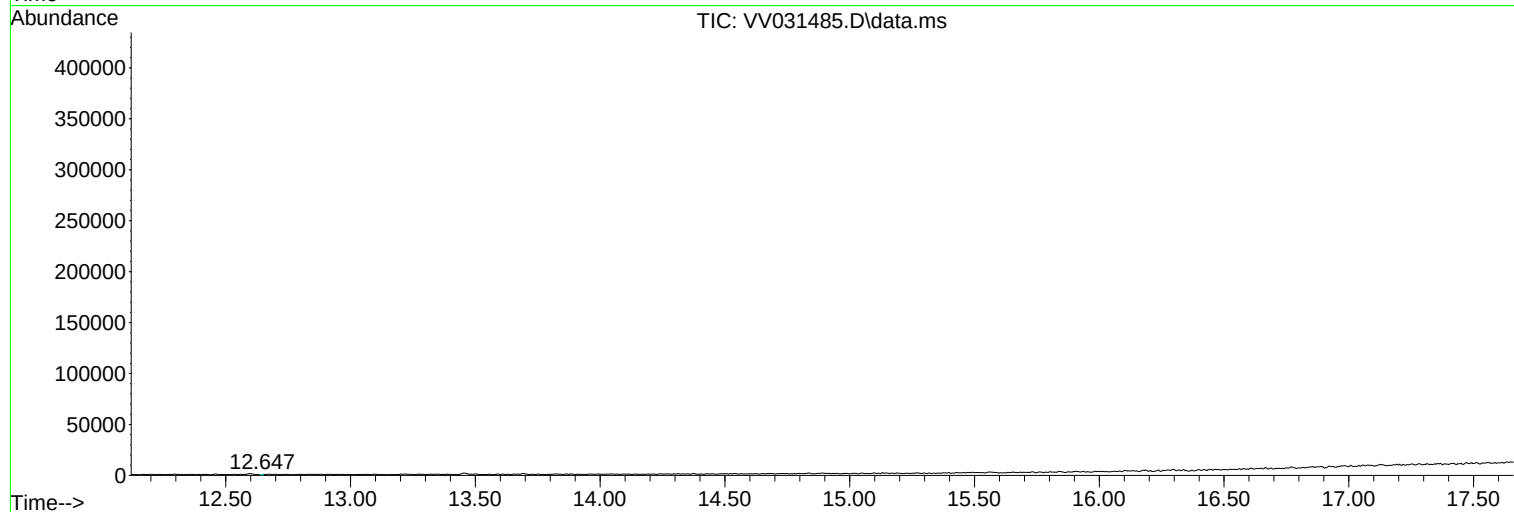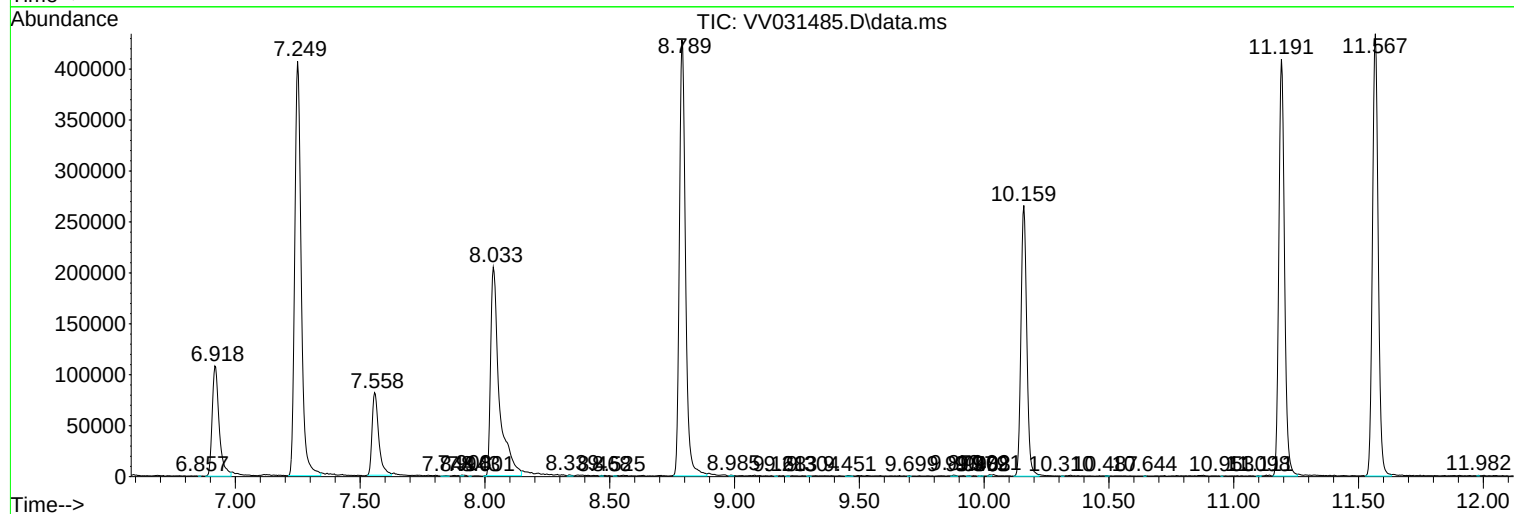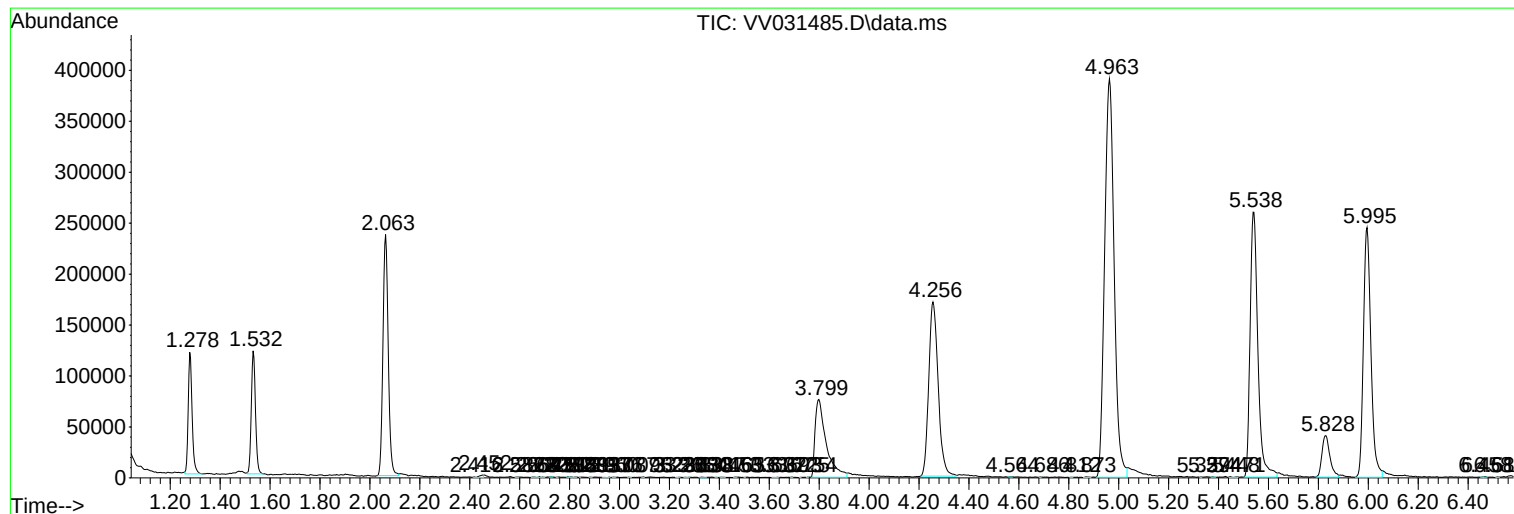

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031485.D
Acq On : 09 Jun 2023 10:40
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK353

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031485.D
Acq On : 09 Jun 2023 10:40
Operator : SY/MD
Sample : VV0609WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK353

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc