

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031486.D
 Acq On : 09 Jun 2023 11:03
 Operator : SY/MD
 Sample : 03098-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	116522	127070	12.26%	1.654%
2	1.532	146	153	167	rVB	115930	136691	13.19%	1.779%
3	2.063	308	318	332	rBV	228656	337050	32.53%	4.387%
4	2.387	416	419	420	rBV	468	216	0.02%	0.003%
5	2.455	435	440	444	rBV5	1042	977	0.09%	0.013%
6	2.513	456	458	460	rBV	482	236	0.02%	0.003%
7	2.596	482	484	486	rVV2	408	247	0.02%	0.003%
8	2.609	486	488	489	rVV2	630	222	0.02%	0.003%
9	2.619	489	491	495	rVB2	360	188	0.02%	0.002%
10	2.796	543	546	551	rVB3	586	356	0.03%	0.005%
11	2.895	571	577	579	rBV4	536	502	0.05%	0.007%
12	3.027	615	618	621	rVB2	465	296	0.03%	0.004%
13	3.047	621	624	627	rBV	228	146	0.01%	0.002%
14	3.304	702	704	708	rVB	393	218	0.02%	0.003%
15	3.326	708	711	716	rVB4	456	250	0.02%	0.003%
16	3.352	716	719	720	rBV	333	216	0.02%	0.003%
17	3.455	748	751	755	rVB2	667	420	0.04%	0.005%
18	3.516	768	770	775	rVB3	382	264	0.03%	0.003%
19	3.616	798	801	802	rBV	452	189	0.02%	0.002%
20	3.674	817	819	820	rBV	492	162	0.02%	0.002%
21	3.683	820	822	827	rVB	252	210	0.02%	0.003%
22	3.725	832	835	838	rBV2	368	200	0.02%	0.003%
23	3.760	845	846	848	rBV2	414	157	0.02%	0.002%
24	3.796	848	857	886	rBV2	71820	209961	20.26%	2.733%
25	4.256	984	1000	1027	rBV2	171027	445462	42.99%	5.799%
26	4.590	1102	1104	1107	rVB2	557	258	0.02%	0.003%
27	4.706	1138	1140	1142	rVB3	490	181	0.02%	0.002%
28	4.725	1142	1146	1150	rVB3	434	368	0.04%	0.005%
29	4.751	1150	1154	1155	rBV2	325	242	0.02%	0.003%
30	4.828	1176	1178	1186	rVB4	701	637	0.06%	0.008%
31	4.870	1186	1191	1194	rBV2	629	569	0.05%	0.007%
32	4.963	1200	1220	1246	rBV2	383328	1036190	100.00%	13.488%
33	5.423	1361	1363	1366	rBV2	274	160	0.02%	0.002%
34	5.452	1368	1372	1375	rVB2	406	299	0.03%	0.004%
35	5.474	1377	1379	1383	rBV2	603	404	0.04%	0.005%
36	5.538	1387	1399	1431	rBV	274190	587519	56.70%	7.648%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060923\
 Data File : VW031486.D
 Acq On : 09 Jun 2023 11:03
 Operator : SY/MD
 Sample : 03098-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.828	1478	1489	1505	rBV2	36764	77849	7.51%	1.013%
38	5.944	1522	1525	1527	rBV3	724	452	0.04%	0.006%
39	5.995	1527	1541	1575	rVV	244676	517661	49.96%	6.738%
40	6.236	1613	1616	1617	rBV2	534	376	0.04%	0.005%
41	6.307	1635	1638	1643	rVB4	696	609	0.06%	0.008%
42	6.416	1670	1672	1675	rBV	220	148	0.01%	0.002%
43	6.497	1694	1697	1701	rBV3	579	405	0.04%	0.005%
44	6.522	1703	1705	1707	rBV2	325	149	0.01%	0.002%
45	6.567	1711	1719	1723	rBV5	1704	2631	0.25%	0.034%
46	6.667	1748	1750	1754	rVB4	698	421	0.04%	0.005%
47	6.841	1801	1804	1806	rBV	552	281	0.03%	0.004%
48	6.873	1811	1814	1817	rBV2	309	176	0.02%	0.002%
49	6.918	1817	1828	1856	rBV	110294	214927	20.74%	2.798%
50	7.249	1918	1931	1952	rBV	403660	722137	69.69%	9.400%
51	7.558	2017	2027	2047	rBV2	80317	152205	14.69%	1.981%
52	7.825	2107	2110	2114	rBV3	426	424	0.04%	0.006%
53	7.847	2115	2117	2119	rVB	348	156	0.02%	0.002%
54	7.863	2119	2122	2123	rBV	489	222	0.02%	0.003%
55	8.034	2165	2175	2209	rBV2	202346	479864	46.31%	6.246%
56	8.503	2314	2321	2326	rVB4	637	734	0.07%	0.010%
57	8.525	2326	2328	2329	rBV2	408	162	0.02%	0.002%
58	8.580	2343	2345	2348	rBV2	331	245	0.02%	0.003%
59	8.635	2359	2362	2364	rBV2	412	253	0.02%	0.003%
60	8.648	2364	2366	2369	rVB2	535	305	0.03%	0.004%
61	8.664	2369	2371	2373	rBV2	337	149	0.01%	0.002%
62	8.789	2395	2410	2442	rBV	447233	757402	73.09%	9.859%
63	9.017	2479	2481	2485	rVB3	728	532	0.05%	0.007%
64	9.059	2492	2494	2498	rVB3	459	212	0.02%	0.003%
65	9.082	2499	2501	2506	rBV3	539	455	0.04%	0.006%
66	9.207	2538	2540	2542	rBV3	920	391	0.04%	0.005%
67	9.275	2559	2561	2566	rVB2	480	292	0.03%	0.004%
68	9.326	2576	2577	2579	rBV2	522	202	0.02%	0.003%
69	9.400	2597	2600	2603	rBV2	240	161	0.02%	0.002%
70	9.423	2603	2607	2611	rBV	495	359	0.03%	0.005%
71	9.641	2672	2675	2677	rVB	630	320	0.03%	0.004%
72	9.654	2677	2679	2682	rBV2	590	273	0.03%	0.004%
73	9.805	2722	2726	2731	rBV4	434	510	0.05%	0.007%
74	9.876	2746	2748	2751	rVV2	500	278	0.03%	0.004%
75	9.931	2762	2765	2768	rBV	497	346	0.03%	0.005%
76	10.033	2794	2797	2801	rBV3	634	557	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031486.D
 Acq On : 09 Jun 2023 11:03
 Operator : SY/MD
 Sample : 03098-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.159	2824	2836	2860	rVB	276507	448159	43.25%	5.834%
78	10.246	2860	2863	2867	rVB3	987	758	0.07%	0.010%
79	10.278	2867	2873	2877	rBV4	794	899	0.09%	0.012%
80	10.320	2882	2886	2887	rBV3	483	339	0.03%	0.004%
81	10.329	2887	2889	2900	rVB6	1128	1453	0.14%	0.019%
82	10.400	2907	2911	2913	rBV2	293	206	0.02%	0.003%
83	10.480	2933	2936	2937	rBV2	660	320	0.03%	0.004%
84	10.644	2984	2987	2989	rBV2	553	293	0.03%	0.004%
85	10.728	3011	3013	3014	rBV	428	204	0.02%	0.003%
86	11.072	3118	3120	3124	rVB2	427	214	0.02%	0.003%
87	11.107	3129	3131	3135	rBV3	397	248	0.02%	0.003%
88	11.127	3135	3137	3139	rBV	423	271	0.03%	0.004%
89	11.191	3146	3157	3176	rBV	433028	689429	66.53%	8.974%
90	11.567	3261	3274	3293	rBV	446962	712224	68.73%	9.271%
91	12.114	3440	3444	3447	rBV4	459	387	0.04%	0.005%
92	12.152	3454	3456	3458	rBV4	399	233	0.02%	0.003%
93	12.963	3706	3708	3710	rBV2	304	180	0.02%	0.002%
94	13.024	3725	3727	3730	rVB2	377	172	0.02%	0.002%
95	13.487	3869	3871	3874	rBV3	476	205	0.02%	0.003%
96	13.815	3971	3973	3975	rBV3	495	228	0.02%	0.003%
97	13.988	4024	4027	4029	rBV3	668	406	0.04%	0.005%
98	14.046	4039	4045	4046	rBV3	680	597	0.06%	0.008%
99	14.082	4053	4056	4060	rBV2	985	703	0.07%	0.009%
100	14.117	4065	4067	4069	rBV3	532	248	0.02%	0.003%




Sum of corrected areas: 7682340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031486.D
Acq On : 09 Jun 2023 11:03
Operator : SY/MD
Sample : 03098-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

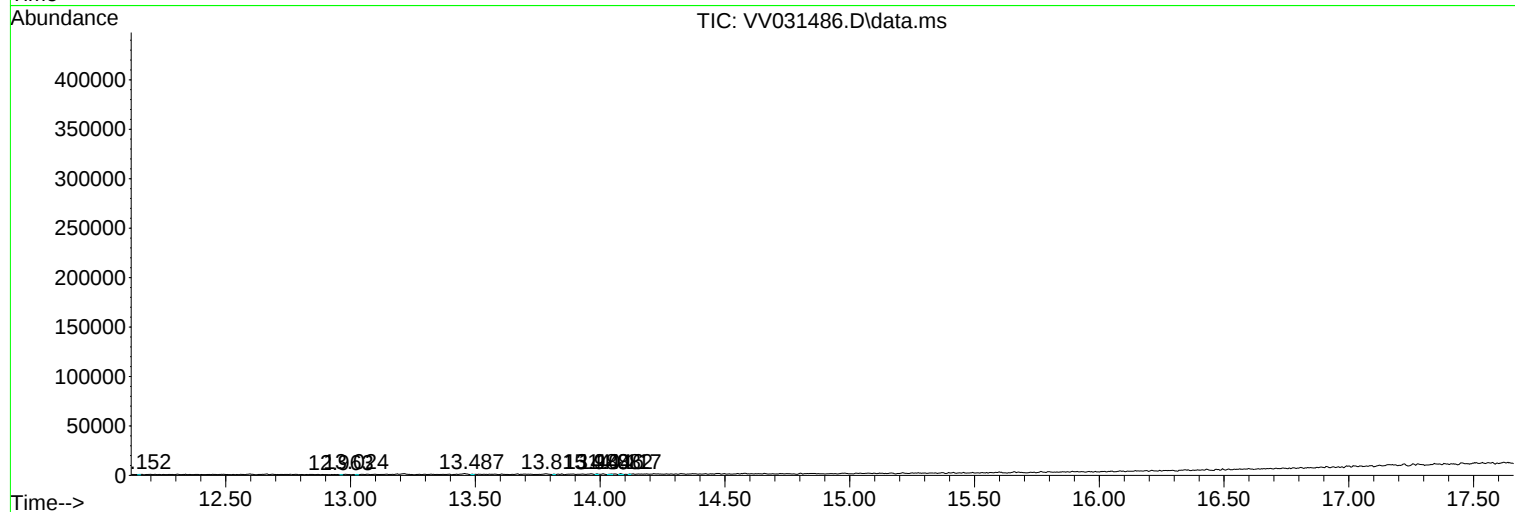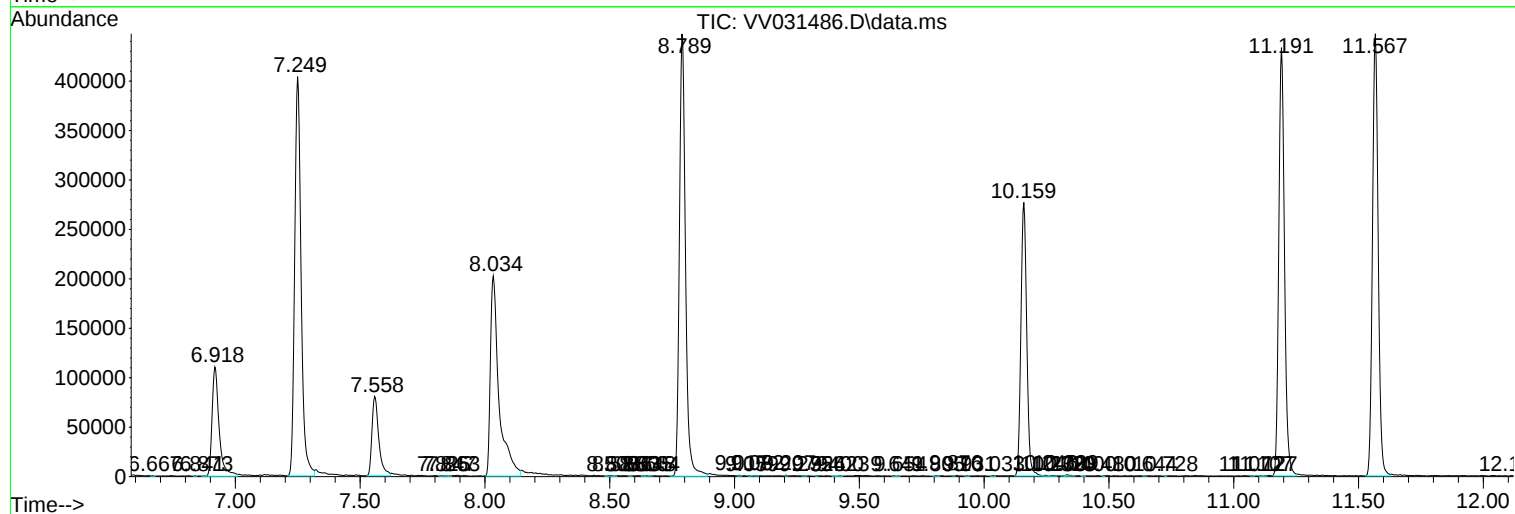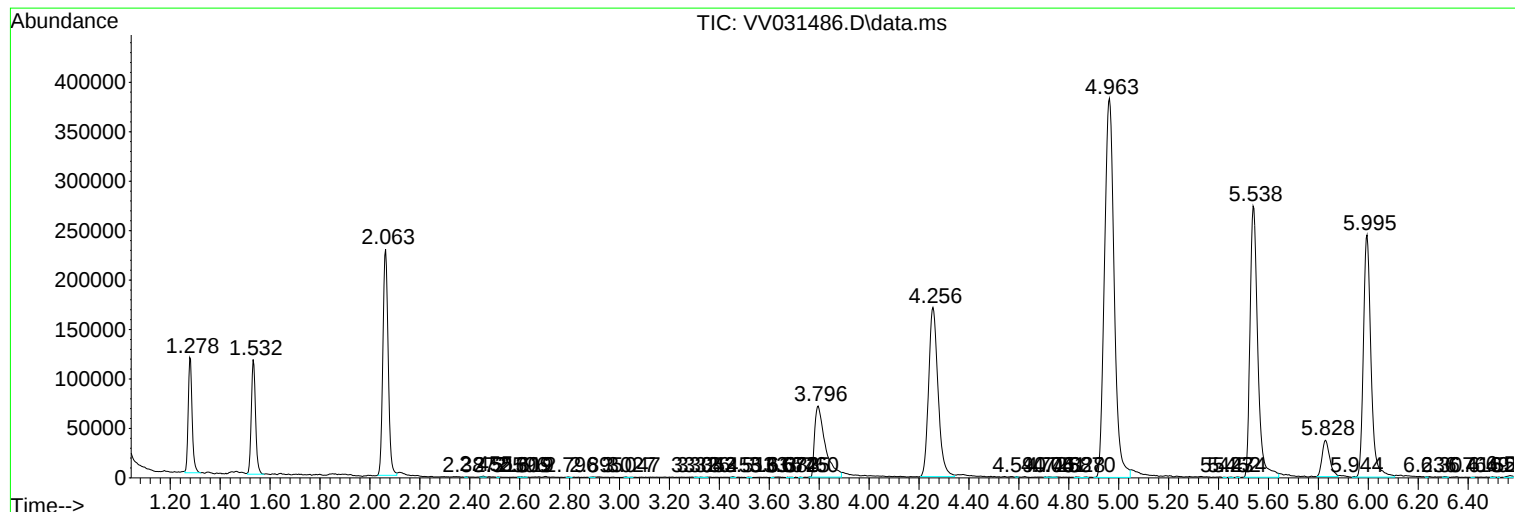

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031486.D
Acq On : 09 Jun 2023 11:03
Operator : SY/MD
Sample : 03098-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031486.D
Acq On : 09 Jun 2023 11:03
Operator : SY/MD
Sample : 03098-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZE7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------