

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031488.D
 Acq On : 09 Jun 2023 11:50
 Operator : SY/MD
 Sample : 03098-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	115636	124845	11.88%	1.624%
2	1.532	146	153	166	rVB	118485	137970	13.13%	1.795%
3	2.063	308	318	332	rBV	229707	335874	31.97%	4.369%
4	2.301	388	392	393	rBV3	550	323	0.03%	0.004%
5	2.439	433	435	436	rBV2	573	275	0.03%	0.004%
6	2.558	469	472	474	rBV3	401	259	0.02%	0.003%
7	2.793	543	545	547	rVV2	396	198	0.02%	0.003%
8	2.806	547	549	557	rVB4	663	677	0.06%	0.009%
9	2.841	557	560	563	rBV2	336	221	0.02%	0.003%
10	2.857	563	565	570	rVB3	471	246	0.02%	0.003%
11	2.892	570	576	582	rBV5	813	895	0.09%	0.012%
12	2.937	588	590	593	rBV2	358	213	0.02%	0.003%
13	3.179	662	665	672	rBV3	377	423	0.04%	0.006%
14	3.211	672	675	680	rVB2	616	377	0.04%	0.005%
15	3.243	683	685	689	rVB2	421	256	0.02%	0.003%
16	3.269	689	693	694	rBV2	347	183	0.02%	0.002%
17	3.423	738	741	742	rBV	386	220	0.02%	0.003%
18	3.465	750	754	756	rVB2	256	197	0.02%	0.003%
19	3.555	779	782	784	rBV	312	216	0.02%	0.003%
20	3.600	792	796	798	rBV2	271	239	0.02%	0.003%
21	3.638	805	808	811	rVB2	337	207	0.02%	0.003%
22	3.658	812	814	819	rVB3	508	248	0.02%	0.003%
23	3.683	819	822	827	rVB3	363	318	0.03%	0.004%
24	3.793	844	856	888	rBV	73482	217194	20.68%	2.825%
25	4.166	970	972	973	rBV	483	195	0.02%	0.003%
26	4.256	984	1000	1027	rBV	173309	455429	43.35%	5.924%
27	4.587	1100	1103	1105	rBV4	419	207	0.02%	0.003%
28	4.680	1129	1132	1134	rBV2	357	221	0.02%	0.003%
29	4.783	1161	1164	1165	rBV	503	211	0.02%	0.003%
30	4.844	1181	1183	1187	rVB2	331	195	0.02%	0.003%
31	4.870	1187	1191	1193	rBV	335	239	0.02%	0.003%
32	4.963	1202	1220	1245	rBV2	391261	1050475	100.00%	13.664%
33	5.429	1363	1365	1369	rVB2	388	262	0.02%	0.003%
34	5.494	1381	1385	1387	rBV	265	182	0.02%	0.002%
35	5.539	1387	1399	1421	rBV	265849	562676	53.56%	7.319%
36	5.828	1478	1489	1515	rVB3	38351	82776	7.88%	1.077%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031488.D
 Acq On : 09 Jun 2023 11:50
 Operator : SY/MD
 Sample : 03098-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.995	1524	1541	1572	rBV	246493	524648	49.94%	6.824%
38	6.256	1614	1622	1624	rBV6	543	759	0.07%	0.010%
39	6.391	1660	1664	1667	rVB4	654	507	0.05%	0.007%
40	6.413	1667	1671	1675	rBV2	482	306	0.03%	0.004%
41	6.452	1681	1683	1686	rBV2	397	282	0.03%	0.004%
42	6.500	1694	1698	1701	rVB3	480	355	0.03%	0.005%
43	6.516	1701	1703	1705	rBV2	324	192	0.02%	0.002%
44	6.567	1712	1719	1724	rBV5	1600	2497	0.24%	0.032%
45	6.703	1757	1761	1765	rBV3	535	508	0.05%	0.007%
46	6.725	1765	1768	1769	rBV	326	180	0.02%	0.002%
47	6.767	1778	1781	1783	rBV	467	188	0.02%	0.002%
48	6.918	1817	1828	1854	rBV	111704	214693	20.44%	2.793%
49	7.249	1919	1931	1958	rBV	409004	741990	70.63%	9.651%
50	7.558	2017	2027	2044	rBV	84853	153376	14.60%	1.995%
51	7.751	2085	2087	2090	rBV3	351	199	0.02%	0.003%
52	7.783	2095	2097	2100	rBV2	361	182	0.02%	0.002%
53	7.911	2134	2137	2139	rBV2	944	629	0.06%	0.008%
54	7.969	2153	2155	2159	rBV2	572	259	0.02%	0.003%
55	8.034	2163	2175	2213	rBV2	212135	495006	47.12%	6.439%
56	8.381	2281	2283	2285	rBV	614	313	0.03%	0.004%
57	8.561	2336	2339	2342	rVB2	592	342	0.03%	0.004%
58	8.645	2363	2365	2369	rVB2	455	267	0.03%	0.003%
59	8.751	2395	2398	2399	rBV	389	186	0.02%	0.002%
60	8.789	2399	2410	2445	rVV	435974	735899	70.05%	9.572%
61	9.008	2475	2478	2481	rBV3	579	408	0.04%	0.005%
62	9.091	2502	2504	2508	rVB3	631	388	0.04%	0.005%
63	9.120	2510	2513	2518	rVB3	742	469	0.04%	0.006%
64	9.143	2518	2520	2522	rBV2	456	176	0.02%	0.002%
65	9.198	2534	2537	2538	rBV2	488	305	0.03%	0.004%
66	9.223	2543	2545	2548	rVB2	449	242	0.02%	0.003%
67	9.571	2651	2653	2655	rBV	273	176	0.02%	0.002%
68	9.738	2703	2705	2708	rBV2	243	176	0.02%	0.002%
69	9.847	2737	2739	2740	rBV	462	185	0.02%	0.002%
70	9.934	2762	2766	2768	rBV	349	248	0.02%	0.003%
71	9.963	2771	2775	2777	rBV2	316	279	0.03%	0.004%
72	10.088	2811	2814	2818	rBV3	372	256	0.02%	0.003%
73	10.117	2820	2823	2824	rBV2	559	270	0.03%	0.004%
74	10.159	2824	2836	2856	rVV	279207	447870	42.63%	5.825%
75	10.419	2912	2917	2921	rBV3	335	346	0.03%	0.005%
76	10.452	2926	2927	2933	rBV2	453	295	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031488.D
 Acq On : 09 Jun 2023 11:50
 Operator : SY/MD
 Sample : 03098-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.474	2933	2934	2940	rBV2	489	458	0.04%	0.006%
78	10.551	2956	2958	2963	rBV3	351	231	0.02%	0.003%
79	10.725	3009	3012	3014	rBV2	453	224	0.02%	0.003%
80	10.738	3014	3016	3021	rVB3	449	371	0.04%	0.005%
81	10.866	3051	3056	3060	rBV3	562	642	0.06%	0.008%
82	10.950	3080	3082	3085	rBV2	494	344	0.03%	0.004%
83	11.072	3118	3120	3125	rVB	401	273	0.03%	0.004%
84	11.101	3125	3129	3131	rBV3	292	231	0.02%	0.003%
85	11.130	3133	3138	3141	rBV2	734	686	0.07%	0.009%
86	11.191	3146	3157	3176	rBV	411867	659539	62.78%	8.579%
87	11.371	3211	3213	3216	rVB	456	196	0.02%	0.003%
88	11.567	3262	3274	3294	rBV	452023	718976	68.44%	9.352%
89	11.831	3354	3356	3358	rBV	478	213	0.02%	0.003%
90	12.294	3499	3500	3503	rBV	337	179	0.02%	0.002%
91	12.349	3515	3517	3521	rBV3	349	227	0.02%	0.003%
92	12.519	3567	3570	3577	rVB4	643	649	0.06%	0.008%
93	12.664	3612	3615	3618	rBV3	547	328	0.03%	0.004%
94	12.741	3635	3639	3640	rBV2	391	265	0.03%	0.003%
95	12.754	3640	3643	3648	rBV3	560	590	0.06%	0.008%
96	12.844	3669	3671	3676	rBV2	323	269	0.03%	0.003%
97	13.358	3828	3831	3835	rBV3	707	488	0.05%	0.006%
98	13.419	3846	3850	3852	rBV2	315	276	0.03%	0.004%
99	13.696	3933	3936	3938	rBV3	584	351	0.03%	0.005%
100	14.246	4103	4107	4112	rBV5	863	1131	0.11%	0.015%




Sum of corrected areas: 7688131

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031488.D
Acq On : 09 Jun 2023 11:50
Operator : SY/MD
Sample : 03098-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

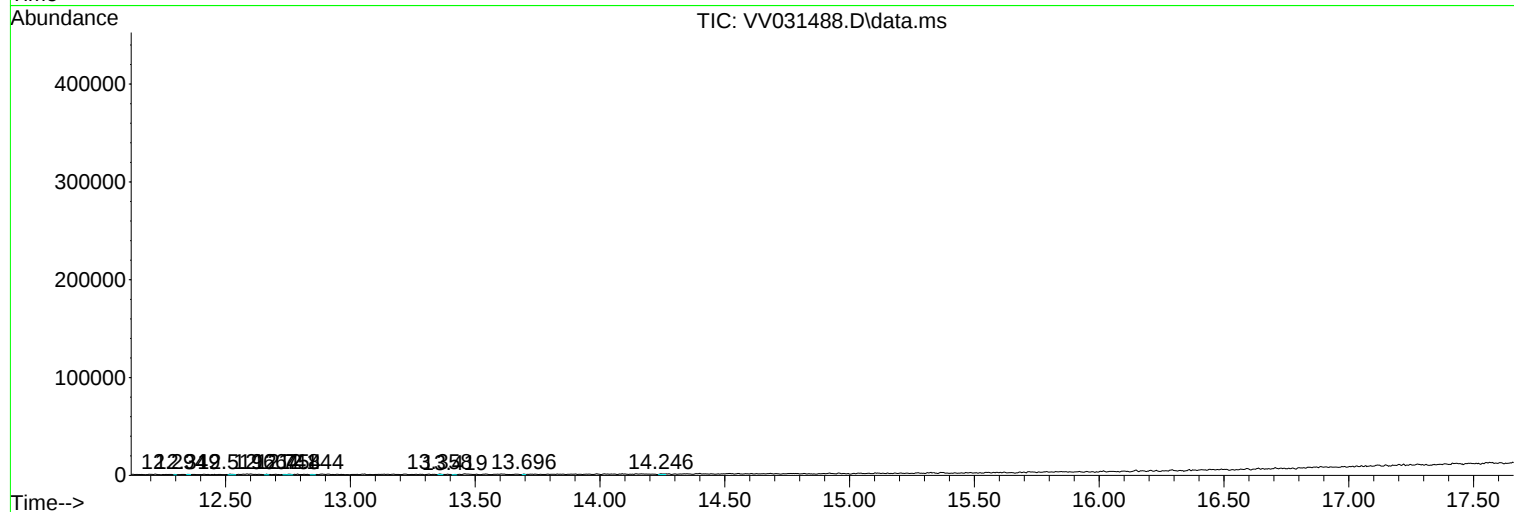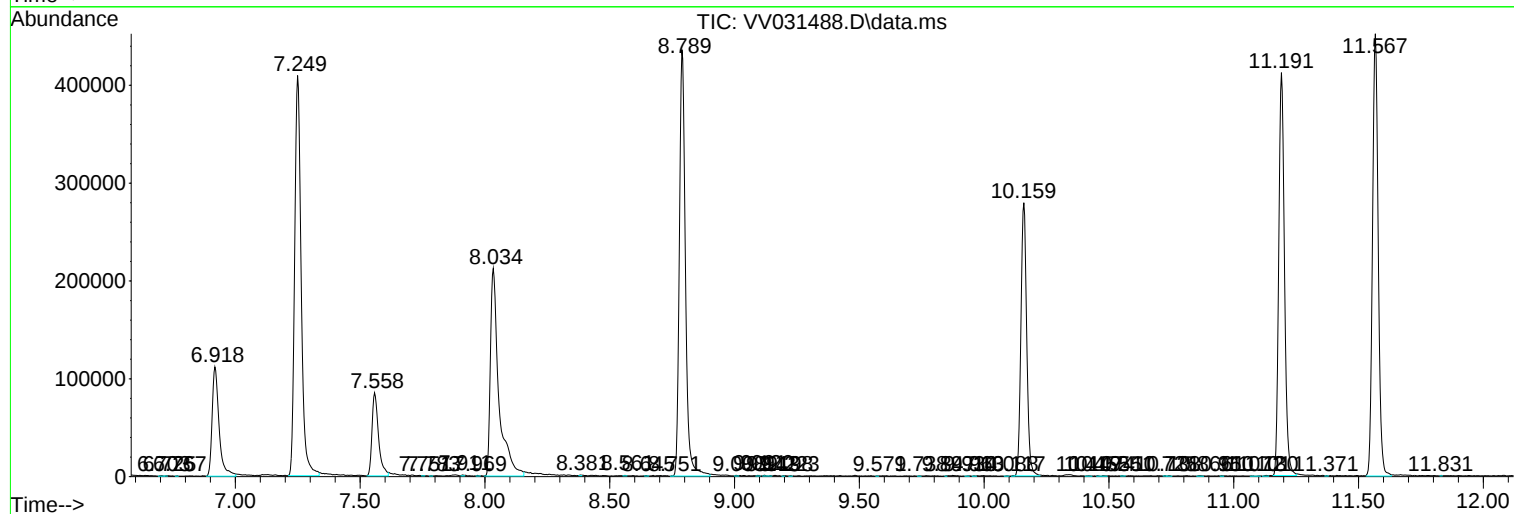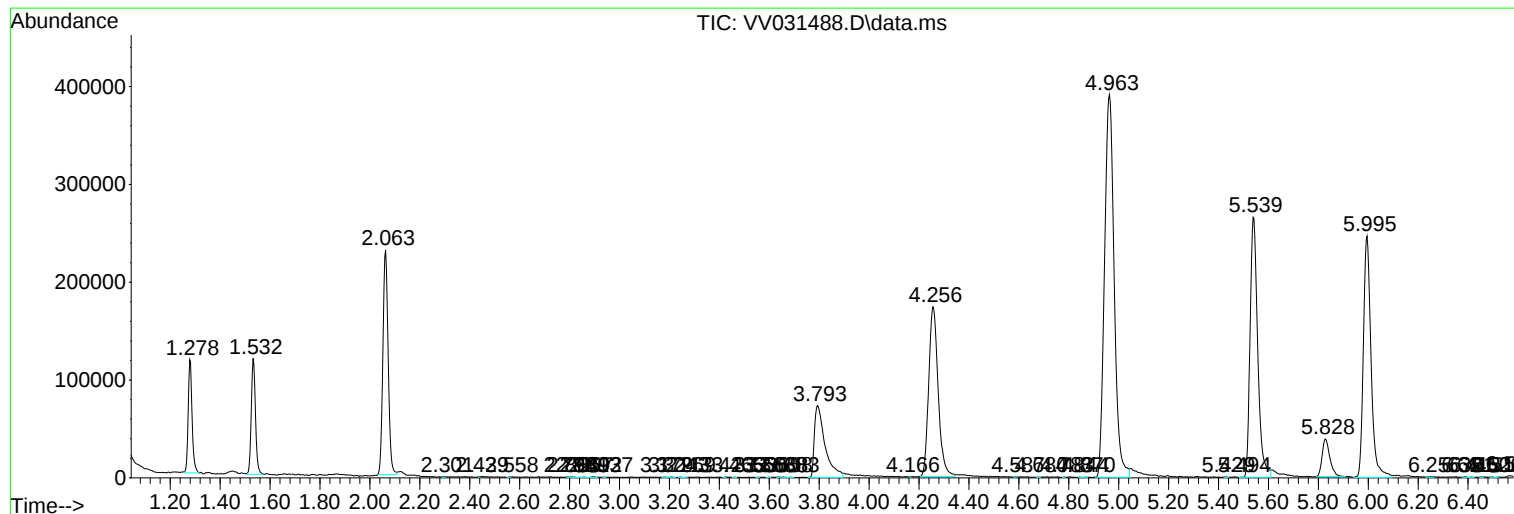

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031488.D
Acq On : 09 Jun 2023 11:50
Operator : SY/MD
Sample : 03098-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031488.D
Acq On : 09 Jun 2023 11:50
Operator : SY/MD
Sample : 03098-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc