

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031489.D
 Acq On : 09 Jun 2023 12:13
 Operator : SY/MD
 Sample : 03098-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031489.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	104564	113104	10.76%	1.491%
2	1.532	146	153	166	rVB	112093	130834	12.45%	1.725%
3	2.063	308	318	335	rBV	218539	321115	30.56%	4.234%
4	2.336	399	403	405	rBV3	482	346	0.03%	0.005%
5	2.455	433	440	442	rBV5	988	1088	0.10%	0.014%
6	2.606	484	487	489	rBV3	330	218	0.02%	0.003%
7	2.696	512	515	517	rBV3	500	308	0.03%	0.004%
8	2.757	529	534	535	rVB2	350	279	0.03%	0.004%
9	2.834	554	558	560	rBV	402	279	0.03%	0.004%
10	2.847	560	562	565	rVV2	345	221	0.02%	0.003%
11	2.880	569	572	574	rBV3	353	187	0.02%	0.002%
12	2.950	587	594	597	rBV3	410	477	0.05%	0.006%
13	3.015	612	614	618	rBV2	333	188	0.02%	0.002%
14	3.098	637	640	641	rBV	462	209	0.02%	0.003%
15	3.146	652	655	657	rBV2	444	275	0.03%	0.004%
16	3.230	678	681	682	rBV	305	183	0.02%	0.002%
17	3.323	707	710	712	rBV2	239	167	0.02%	0.002%
18	3.523	769	772	777	rBV2	306	234	0.02%	0.003%
19	3.552	777	781	785	rVV2	276	292	0.03%	0.004%
20	3.748	840	842	844	rVB	442	174	0.02%	0.002%
21	3.793	844	856	882	rBV	75914	211719	20.15%	2.792%
22	4.256	983	1000	1024	rBV	169894	445421	42.39%	5.873%
23	4.690	1130	1135	1138	rBV3	331	310	0.03%	0.004%
24	4.838	1179	1181	1185	rVB2	509	312	0.03%	0.004%
25	4.857	1185	1187	1188	rBV2	651	262	0.02%	0.003%
26	4.963	1202	1220	1263	rBV2	384196	1050751	100.00%	13.856%
27	5.391	1351	1353	1354	rBV	447	178	0.02%	0.002%
28	5.471	1373	1378	1380	rBV3	570	546	0.05%	0.007%
29	5.539	1387	1399	1421	rBV	271932	568117	54.07%	7.491%
30	5.828	1478	1489	1513	rBV3	39255	86596	8.24%	1.142%
31	5.995	1527	1541	1571	rBV	242879	510643	48.60%	6.734%
32	6.252	1618	1621	1622	rBV2	726	433	0.04%	0.006%
33	6.323	1640	1643	1646	rBV3	422	270	0.03%	0.004%
34	6.355	1649	1653	1656	rBV3	408	226	0.02%	0.003%
35	6.426	1673	1675	1679	rVB2	467	249	0.02%	0.003%
36	6.458	1679	1685	1686	rBV	470	363	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031489.D
 Acq On : 09 Jun 2023 12:13
 Operator : SY/MD
 Sample : 03098-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.561	1712	1717	1718	rBV	1381	1198	0.11%	0.016%
38	6.645	1740	1743	1749	rVB3	707	518	0.05%	0.007%
39	6.741	1769	1773	1774	rBV2	374	266	0.03%	0.004%
40	6.780	1783	1785	1786	rBV	415	179	0.02%	0.002%
41	6.918	1811	1828	1853	rBV2	110682	217780	20.73%	2.872%
42	7.249	1919	1931	1952	rBV	406702	725788	69.07%	9.570%
43	7.558	2018	2027	2045	rBV	81589	147181	14.01%	1.941%
44	7.799	2100	2102	2105	rVB3	388	167	0.02%	0.002%
45	7.876	2120	2126	2129	rBV6	1822	2042	0.19%	0.027%
46	8.034	2165	2175	2206	rVV2	209569	481955	45.87%	6.355%
47	8.394	2283	2287	2290	rBV5	700	509	0.05%	0.007%
48	8.452	2303	2305	2309	rVB3	809	425	0.04%	0.006%
49	8.500	2316	2320	2321	rBV3	479	324	0.03%	0.004%
50	8.532	2327	2330	2331	rBV	568	285	0.03%	0.004%
51	8.622	2356	2358	2363	rVB2	593	365	0.03%	0.005%
52	8.654	2366	2368	2373	rVB4	820	517	0.05%	0.007%
53	8.673	2373	2374	2376	rBV	483	254	0.02%	0.003%
54	8.696	2379	2381	2385	rVB2	525	307	0.03%	0.004%
55	8.789	2398	2410	2432	rBV	428676	725511	69.05%	9.567%
56	8.992	2471	2473	2477	rBV3	370	264	0.03%	0.003%
57	9.034	2483	2486	2488	rBV3	446	257	0.02%	0.003%
58	9.066	2494	2496	2498	rBV	378	191	0.02%	0.003%
59	9.143	2517	2520	2522	rBV	311	232	0.02%	0.003%
60	9.156	2522	2524	2527	rVB2	692	415	0.04%	0.005%
61	9.178	2527	2531	2534	rBV2	452	414	0.04%	0.005%
62	9.239	2546	2550	2554	rBV2	705	515	0.05%	0.007%
63	9.352	2583	2585	2586	rBV2	550	185	0.02%	0.002%
64	9.484	2624	2626	2628	rBV	356	241	0.02%	0.003%
65	9.522	2636	2638	2643	rVB3	641	404	0.04%	0.005%
66	9.554	2646	2648	2649	rBV	472	191	0.02%	0.003%
67	9.622	2666	2669	2672	rVB3	544	360	0.03%	0.005%
68	9.641	2672	2675	2678	rBV3	351	214	0.02%	0.003%
69	9.709	2693	2696	2698	rBV2	307	198	0.02%	0.003%
70	9.792	2719	2722	2724	rBV3	576	305	0.03%	0.004%
71	9.944	2766	2769	2772	rVB2	536	326	0.03%	0.004%
72	9.989	2779	2783	2787	rBV2	381	341	0.03%	0.004%
73	10.159	2824	2836	2862	rBV	276555	443331	42.19%	5.846%
74	10.268	2868	2870	2875	rBV3	807	715	0.07%	0.009%
75	10.336	2882	2891	2903	rVB4	3704	6241	0.59%	0.082%
76	10.452	2924	2927	2931	rBV2	356	286	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031489.D
 Acq On : 09 Jun 2023 12:13
 Operator : SY/MD
 Sample : 03098-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZEP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.538	2951	2954	2957	rVB3	429	273	0.03%	0.004%
78	10.583	2963	2968	2970	rBV2	379	297	0.03%	0.004%
79	10.651	2986	2989	2994	rBV3	333	386	0.04%	0.005%
80	10.792	3029	3033	3037	rBV3	618	519	0.05%	0.007%
81	10.850	3049	3051	3053	rBV	396	235	0.02%	0.003%
82	10.902	3063	3067	3069	rBV3	325	232	0.02%	0.003%
83	10.992	3093	3095	3097	rBV2	348	207	0.02%	0.003%
84	11.034	3105	3108	3111	rBV2	335	211	0.02%	0.003%
85	11.085	3122	3124	3126	rBV3	471	223	0.02%	0.003%
86	11.098	3126	3128	3131	rVB2	531	236	0.02%	0.003%
87	11.191	3144	3157	3177	rBV	418565	660993	62.91%	8.716%
88	11.477	3243	3246	3249	rBV2	513	297	0.03%	0.004%
89	11.567	3261	3274	3294	rBV	445711	707444	67.33%	9.329%
90	12.017	3411	3414	3416	rBV3	721	373	0.04%	0.005%
91	12.246	3483	3485	3488	rBV2	756	426	0.04%	0.006%
92	12.329	3507	3511	3514	rBV3	489	435	0.04%	0.006%
93	12.345	3514	3516	3518	rBV	549	255	0.02%	0.003%
94	12.490	3559	3561	3567	rBV3	398	325	0.03%	0.004%
95	12.712	3627	3630	3631	rBV	370	254	0.02%	0.003%
96	12.963	3706	3708	3714	rBV2	592	572	0.05%	0.008%
97	13.210	3783	3785	3786	rBV2	622	290	0.03%	0.004%
98	13.294	3808	3811	3812	rBV	419	211	0.02%	0.003%
99	13.625	3909	3914	3916	rBV4	910	801	0.08%	0.011%
100	13.773	3958	3960	3962	rBV2	544	346	0.03%	0.005%




Sum of corrected areas: 7583612

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031489.D
Acq On : 09 Jun 2023 12:13
Operator : SY/MD
Sample : 03098-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

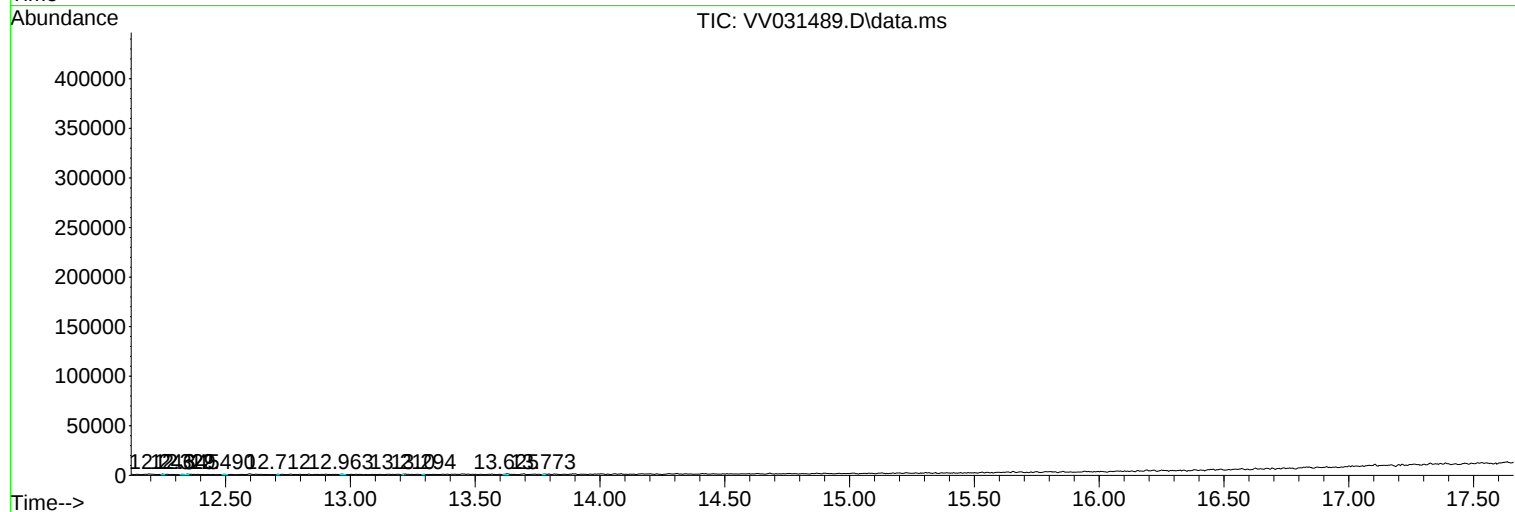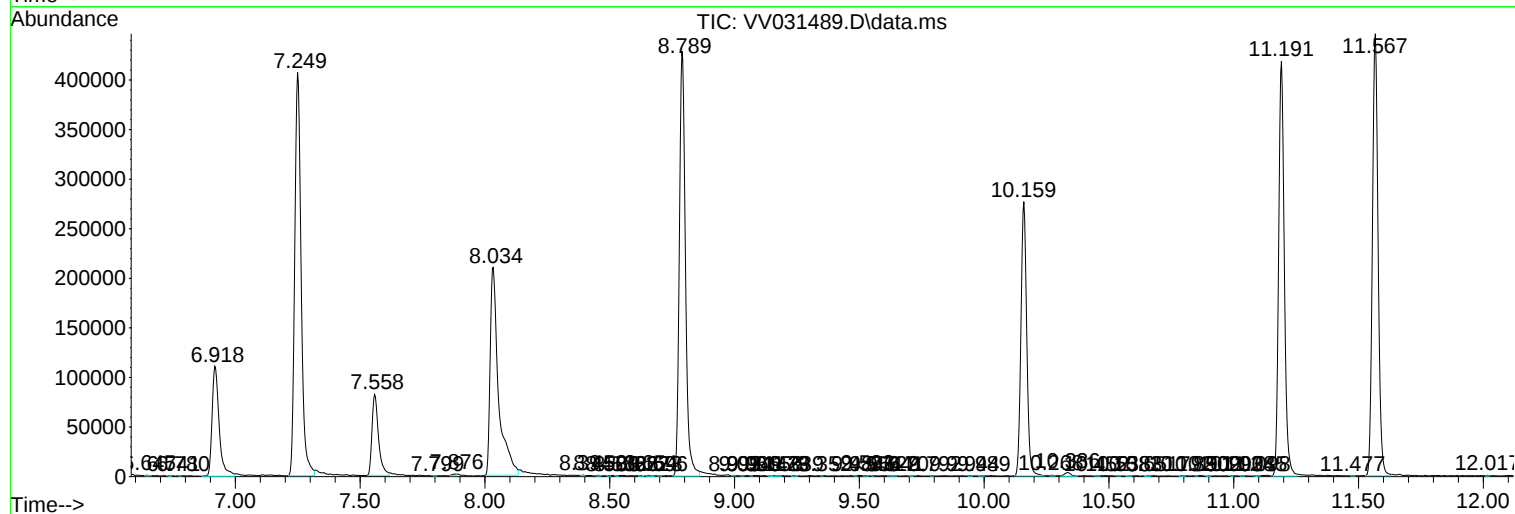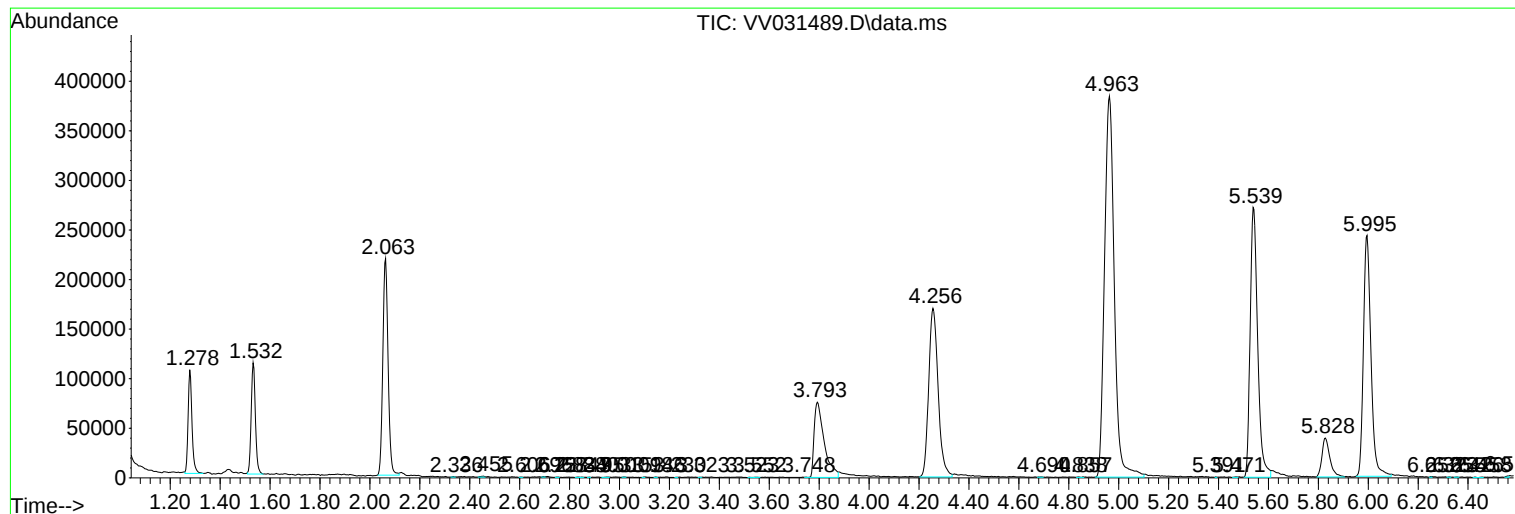

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031489.D
Acq On : 09 Jun 2023 12:13
Operator : SY/MD
Sample : 03098-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031489.D
Acq On : 09 Jun 2023 12:13
Operator : SY/MD
Sample : 03098-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZEP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc