

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031492.D
 Acq On : 09 Jun 2023 13:25
 Operator : SY/MD
 Sample : VIBLK216
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	96151	103958	10.58%	1.423%
2	1.532	147	153	168	rVB	100549	118393	12.05%	1.621%
3	2.063	308	318	333	rBV	187759	276255	28.12%	3.782%
4	2.452	433	439	448	rVB3	3039	4607	0.47%	0.063%
5	2.693	510	514	515	rBV2	743	445	0.05%	0.006%
6	2.761	532	535	536	rBV	336	135	0.01%	0.002%
7	2.883	572	573	576	rBV	321	153	0.02%	0.002%
8	2.921	581	585	587	rBV3	424	299	0.03%	0.004%
9	2.954	592	595	597	rBV	217	152	0.02%	0.002%
10	2.970	598	600	604	rVB2	531	319	0.03%	0.004%
11	3.098	638	640	642	rBV	487	262	0.03%	0.004%
12	3.204	670	673	674	rBV	257	165	0.02%	0.002%
13	3.365	720	723	725	rBV2	545	300	0.03%	0.004%
14	3.378	725	727	732	rVB2	570	343	0.03%	0.005%
15	3.494	758	763	767	rVB3	241	270	0.03%	0.004%
16	3.513	767	769	773	rBV	247	209	0.02%	0.003%
17	3.535	774	776	779	rVB3	396	206	0.02%	0.003%
18	3.555	779	782	784	rBV	359	237	0.02%	0.003%
19	3.635	805	807	810	rBV2	332	201	0.02%	0.003%
20	3.683	820	822	826	rBV2	355	208	0.02%	0.003%
21	3.796	847	857	892	rBV	89546	280117	28.51%	3.835%
22	4.256	986	1000	1024	rBV	159071	407517	41.48%	5.579%
23	4.741	1148	1151	1155	rBV5	507	514	0.05%	0.007%
24	4.786	1163	1165	1167	rBV	353	164	0.02%	0.002%
25	4.873	1189	1192	1193	rBV2	250	140	0.01%	0.002%
26	4.960	1203	1219	1247	rBV2	361847	982505	100.00%	13.451%
27	5.355	1340	1342	1346	rVB4	455	214	0.02%	0.003%
28	5.381	1346	1350	1352	rBV2	346	263	0.03%	0.004%
29	5.391	1352	1353	1356	rVB2	304	145	0.01%	0.002%
30	5.436	1364	1367	1369	rVB	682	326	0.03%	0.004%
31	5.455	1371	1373	1374	rBV	322	136	0.01%	0.002%
32	5.539	1386	1399	1423	rBV	239892	507391	51.64%	6.946%
33	5.828	1478	1489	1503	rBV3	41815	88023	8.96%	1.205%
34	5.995	1527	1541	1572	rBV	230718	492884	50.17%	6.748%
35	6.285	1629	1631	1633	rVB	381	142	0.01%	0.002%
36	6.304	1633	1637	1640	rBV3	454	363	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060923\
 Data File : VW031492.D
 Acq On : 09 Jun 2023 13:25
 Operator : SY/MD
 Sample : VIBLK216
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.336	1645	1647	1650	rBV2	310	197	0.02%	0.003%
38	6.355	1650	1653	1654	rBV2	484	212	0.02%	0.003%
39	6.423	1672	1674	1677	rBV3	583	353	0.04%	0.005%
40	6.487	1692	1694	1698	rVB	230	149	0.02%	0.002%
41	6.513	1698	1702	1703	rBV	360	224	0.02%	0.003%
42	6.568	1710	1719	1721	rBV5	1591	2191	0.22%	0.030%
43	6.674	1750	1752	1757	rVB4	635	539	0.05%	0.007%
44	6.822	1795	1798	1801	rBV3	479	328	0.03%	0.004%
45	6.847	1804	1806	1808	rBV	442	274	0.03%	0.004%
46	6.918	1815	1828	1855	rBV	111680	214145	21.80%	2.932%
47	7.088	1877	1881	1882	rBV2	676	417	0.04%	0.006%
48	7.249	1920	1931	1954	rBV	370121	656802	66.85%	8.992%
49	7.558	2016	2027	2054	rBV2	81403	156754	15.95%	2.146%
50	7.834	2111	2113	2116	rBV3	394	210	0.02%	0.003%
51	8.034	2163	2175	2219	rBV2	227037	541946	55.16%	7.420%
52	8.330	2264	2267	2269	rBV3	617	368	0.04%	0.005%
53	8.432	2297	2299	2301	rBV2	670	277	0.03%	0.004%
54	8.468	2306	2310	2311	rBV3	436	362	0.04%	0.005%
55	8.526	2324	2328	2332	rBV4	572	615	0.06%	0.008%
56	8.545	2332	2334	2336	rVV2	630	262	0.03%	0.004%
57	8.670	2371	2373	2376	rBV3	541	289	0.03%	0.004%
58	8.731	2388	2392	2394	rBV2	622	480	0.05%	0.007%
59	8.789	2399	2410	2430	rBV	382954	653507	66.51%	8.947%
60	8.956	2459	2462	2476	rVB7	2358	4169	0.42%	0.057%
61	9.008	2476	2478	2481	rBV3	652	373	0.04%	0.005%
62	9.047	2487	2490	2491	rBV2	526	276	0.03%	0.004%
63	9.346	2582	2583	2587	rBV	384	238	0.02%	0.003%
64	9.413	2601	2604	2605	rBV2	468	253	0.03%	0.003%
65	9.490	2618	2628	2630	rBV5	1799	2263	0.23%	0.031%
66	9.792	2720	2722	2724	rBV	338	181	0.02%	0.002%
67	9.876	2741	2748	2759	rVB7	2037	3203	0.33%	0.044%
68	9.921	2760	2762	2765	rBV2	299	204	0.02%	0.003%
69	10.043	2798	2800	2801	rBV	380	137	0.01%	0.002%
70	10.082	2806	2812	2816	rBV3	784	575	0.06%	0.008%
71	10.111	2819	2821	2824	rBV	356	217	0.02%	0.003%
72	10.159	2824	2836	2852	rBV	269083	433145	44.09%	5.930%
73	10.329	2884	2889	2898	rBV3	1347	1800	0.18%	0.025%
74	10.484	2931	2937	2946	rBV6	1939	2923	0.30%	0.040%
75	10.574	2963	2965	2970	rVB2	352	174	0.02%	0.002%
76	10.600	2970	2973	2977	rBV3	220	170	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031492.D
 Acq On : 09 Jun 2023 13:25
 Operator : SY/MD
 Sample : VIBLK216
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK216

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.725	3009	3012	3014	rBV	302	207	0.02%	0.003%
78	10.805	3033	3037	3040	rBV2	413	326	0.03%	0.004%
79	11.014	3099	3102	3103	rBV	300	173	0.02%	0.002%
80	11.130	3131	3138	3146	rBV4	4342	6318	0.64%	0.086%
81	11.191	3146	3157	3178	rBV	378616	595408	60.60%	8.151%
82	11.342	3202	3204	3208	rBV3	656	387	0.04%	0.005%
83	11.487	3246	3249	3252	rBV	423	240	0.02%	0.003%
84	11.567	3262	3274	3294	rBV	402890	647950	65.95%	8.871%
85	11.738	3325	3327	3328	rBV	427	169	0.02%	0.002%
86	11.837	3355	3358	3363	rVB3	624	471	0.05%	0.006%
87	11.860	3363	3365	3368	rBV	489	257	0.03%	0.004%
88	11.956	3393	3395	3399	rVB2	674	308	0.03%	0.004%
89	12.130	3447	3449	3454	rBV3	605	336	0.03%	0.005%
90	12.316	3505	3507	3511	rBV3	436	271	0.03%	0.004%
91	12.477	3555	3557	3559	rBV2	515	258	0.03%	0.004%
92	12.593	3586	3593	3602	rVB4	7818	11840	1.21%	0.162%
93	12.706	3625	3628	3630	rBV2	429	239	0.02%	0.003%
94	12.757	3642	3644	3648	rBV3	403	288	0.03%	0.004%
95	13.210	3776	3785	3793	rBV3	10705	16332	1.66%	0.224%
96	13.291	3807	3810	3815	rBV4	539	485	0.05%	0.007%
97	13.368	3831	3834	3837	rBV3	533	433	0.04%	0.006%
98	13.448	3850	3859	3871	rBV	32036	50986	5.19%	0.698%
99	13.689	3925	3934	3944	rVB3	13851	21175	2.16%	0.290%
100	14.146	4073	4076	4077	rBV2	785	317	0.03%	0.004%




Sum of corrected areas: 7304337

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031492.D
Acq On : 09 Jun 2023 13:25
Operator : SY/MD
Sample : VIBLK216
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

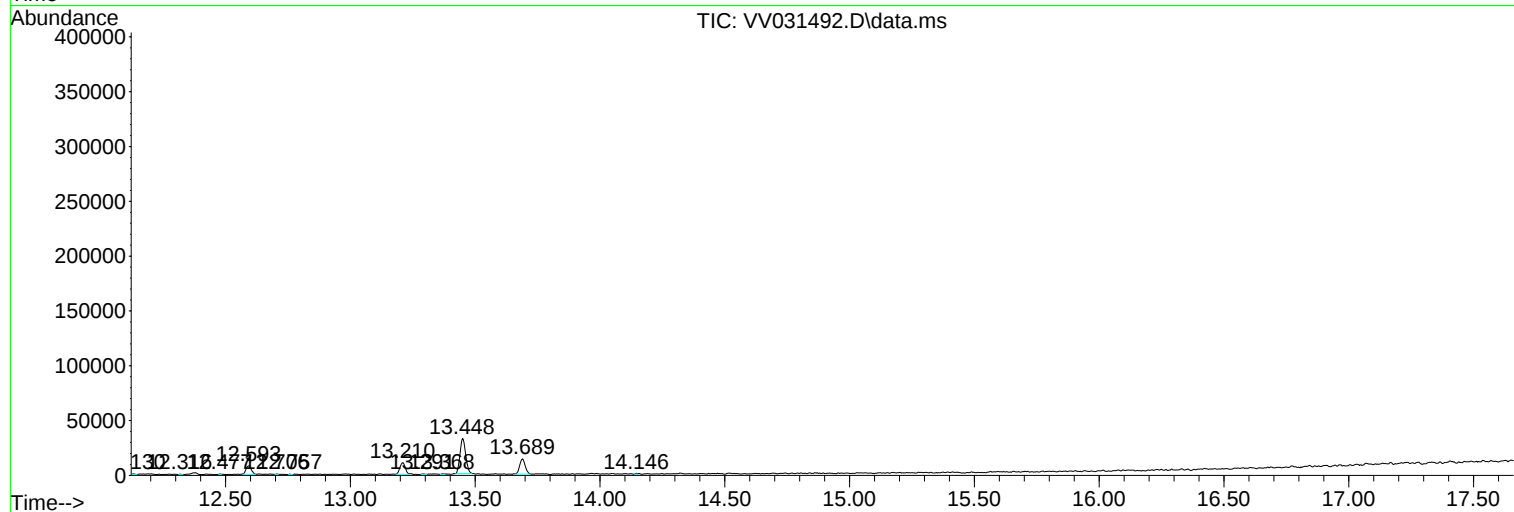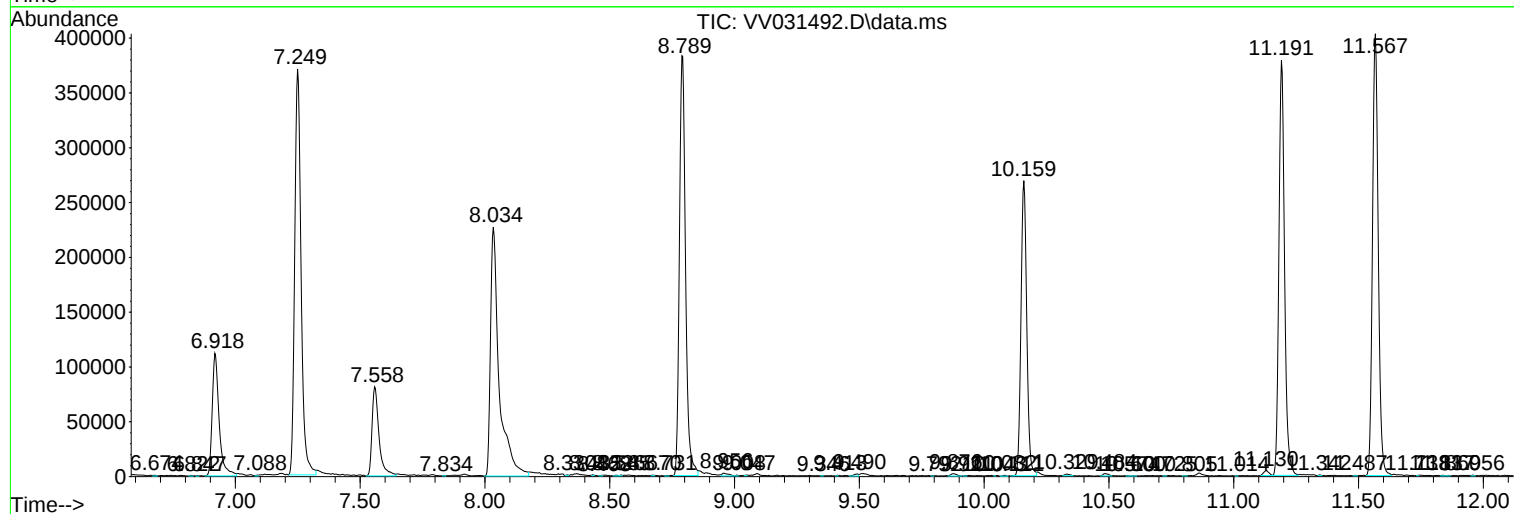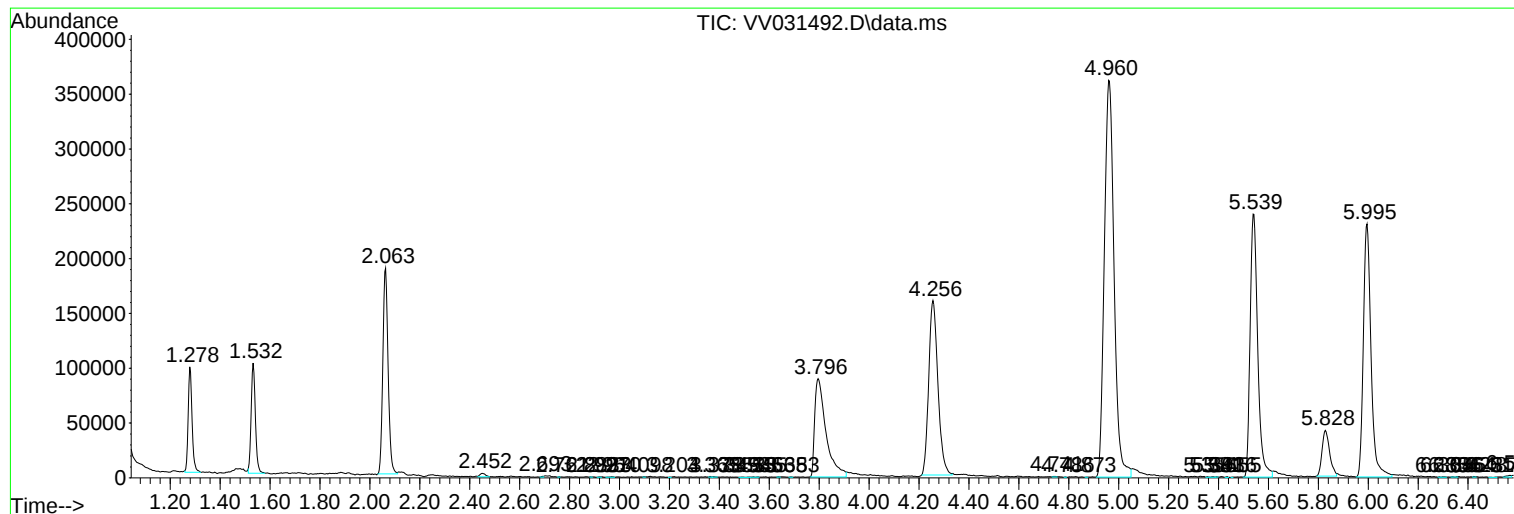

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031492.D
Acq On : 09 Jun 2023 13:25
Operator : SY/MD
Sample : VIBLK216
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031492.D
Acq On : 09 Jun 2023 13:25
Operator : SY/MD
Sample : VIBLK216
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK216

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------