

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031493.D
 Acq On : 09 Jun 2023 14:14
 Operator : SY/MD
 Sample : 03098-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031493.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	103931	110939	10.80%	1.434%
2	1.532	146	153	167	rVB	110684	131586	12.81%	1.700%
3	2.063	308	318	331	rBV	215709	315355	30.69%	4.075%
4	2.352	406	408	411	rBV3	569	260	0.03%	0.003%
5	2.449	432	438	450	rVB5	3027	5300	0.52%	0.068%
6	2.625	490	493	494	rBV	449	213	0.02%	0.003%
7	2.690	511	513	515	rBV2	472	210	0.02%	0.003%
8	2.725	522	524	527	rVB2	454	200	0.02%	0.003%
9	2.815	550	552	554	rBV	285	129	0.01%	0.002%
10	2.847	560	562	564	rVB	352	136	0.01%	0.002%
11	2.873	568	570	573	rVB3	520	228	0.02%	0.003%
12	2.944	589	592	595	rVB3	385	250	0.02%	0.003%
13	2.973	599	601	603	rBV	222	123	0.01%	0.002%
14	3.050	621	625	627	rBV2	624	410	0.04%	0.005%
15	3.146	653	655	657	rVB	394	168	0.02%	0.002%
16	3.162	658	660	662	rBV2	268	115	0.01%	0.001%
17	3.214	671	676	680	rBV3	422	500	0.05%	0.006%
18	3.275	692	695	699	rBV2	400	314	0.03%	0.004%
19	3.342	714	716	719	rVB2	196	109	0.01%	0.001%
20	3.358	719	721	725	rBV3	307	138	0.01%	0.002%
21	3.381	725	728	729	rBV	252	138	0.01%	0.002%
22	3.481	756	759	761	rBV	278	190	0.02%	0.002%
23	3.522	769	772	775	rBV3	288	241	0.02%	0.003%
24	3.571	785	787	792	rVB2	584	323	0.03%	0.004%
25	3.600	792	796	797	rBV2	270	158	0.02%	0.002%
26	3.645	808	810	811	rBV	332	160	0.02%	0.002%
27	3.658	811	814	817	rVV2	478	333	0.03%	0.004%
28	3.674	817	819	824	rVB3	284	159	0.02%	0.002%
29	3.793	847	856	890	rBV	84960	248660	24.20%	3.213%
30	4.256	984	1000	1026	rBV2	170290	442158	43.04%	5.714%
31	4.686	1128	1134	1135	rBV3	395	316	0.03%	0.004%
32	4.699	1137	1138	1142	rVB	297	182	0.02%	0.002%
33	4.741	1147	1151	1153	rVV2	782	659	0.06%	0.009%
34	4.760	1155	1157	1159	rBV	532	253	0.02%	0.003%
35	4.854	1184	1186	1188	rBV	364	164	0.02%	0.002%
36	4.963	1201	1220	1241	rBV2	385831	1027413	100.00%	13.276%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031493.D
 Acq On : 09 Jun 2023 14:14
 Operator : SY/MD
 Sample : 03098-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.284	1316	1320	1322	rBV3	534	421	0.04%	0.005%
38	5.538	1387	1399	1420	rBV	280447	588557	57.29%	7.605%
39	5.828	1478	1489	1505	rBV2	42950	91206	8.88%	1.179%
40	5.995	1528	1541	1572	rBV	243944	514182	50.05%	6.644%
41	6.272	1625	1627	1632	rVB4	652	402	0.04%	0.005%
42	6.307	1636	1638	1640	rVB	398	181	0.02%	0.002%
43	6.345	1649	1650	1654	rBV3	429	238	0.02%	0.003%
44	6.407	1666	1669	1670	rBV2	355	208	0.02%	0.003%
45	6.458	1683	1685	1688	rVB2	675	304	0.03%	0.004%
46	6.493	1694	1696	1701	rVB2	510	224	0.02%	0.003%
47	6.526	1701	1706	1709	rBV4	496	479	0.05%	0.006%
48	6.561	1711	1717	1722	rBV4	1840	2522	0.25%	0.033%
49	6.722	1764	1767	1768	rBV	248	124	0.01%	0.002%
50	6.825	1795	1799	1802	rBV3	341	331	0.03%	0.004%
51	6.873	1811	1814	1816	rBV2	288	195	0.02%	0.003%
52	6.918	1817	1828	1855	rBV2	111675	217305	21.15%	2.808%
53	7.249	1920	1931	1955	rBV	407117	724269	70.49%	9.359%
54	7.558	2018	2027	2052	rBV	81619	150140	14.61%	1.940%
55	7.796	2099	2101	2102	rBV2	362	151	0.01%	0.002%
56	7.844	2114	2116	2120	rVB3	513	346	0.03%	0.004%
57	7.870	2120	2124	2125	rBV2	360	249	0.02%	0.003%
58	7.911	2133	2137	2138	rBV2	738	409	0.04%	0.005%
59	8.034	2164	2175	2213	rBV2	226578	520174	50.63%	6.722%
60	8.410	2289	2292	2295	rBV4	952	695	0.07%	0.009%
61	8.503	2316	2321	2324	rBV3	602	556	0.05%	0.007%
62	8.522	2324	2327	2328	rBV2	495	284	0.03%	0.004%
63	8.590	2346	2348	2349	rBV2	325	115	0.01%	0.001%
64	8.657	2367	2369	2374	rBV3	556	360	0.04%	0.005%
65	8.693	2379	2380	2384	rBV3	301	207	0.02%	0.003%
66	8.789	2398	2410	2436	rBV	450857	766781	74.63%	9.908%
67	9.030	2482	2485	2487	rBV3	677	367	0.04%	0.005%
68	9.381	2592	2594	2597	rBV2	351	179	0.02%	0.002%
69	9.410	2601	2603	2604	rBV	362	106	0.01%	0.001%
70	9.580	2654	2656	2660	rBV2	313	255	0.02%	0.003%
71	9.657	2679	2680	2682	rVB	630	175	0.02%	0.002%
72	9.702	2692	2694	2698	rVB2	362	230	0.02%	0.003%
73	10.024	2790	2794	2797	rBV3	933	812	0.08%	0.010%
74	10.159	2823	2836	2858	rBV	278194	444222	43.24%	5.740%
75	10.320	2880	2886	2887	rBV3	718	551	0.05%	0.007%
76	10.397	2909	2910	2912	rBV2	257	102	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031493.D
 Acq On : 09 Jun 2023 14:14
 Operator : SY/MD
 Sample : 03098-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.426	2917	2919	2924	rVB3	567	318	0.03%	0.004%
78	10.451	2924	2927	2929	rBV2	334	232	0.02%	0.003%
79	10.564	2960	2962	2965	rBV2	350	254	0.02%	0.003%
80	10.641	2984	2986	2987	rBV	407	128	0.01%	0.002%
81	10.670	2992	2995	2998	rBV3	394	338	0.03%	0.004%
82	10.709	3006	3007	3009	rBV2	262	102	0.01%	0.001%
83	10.744	3016	3018	3021	rBV	299	201	0.02%	0.003%
84	10.786	3029	3031	3033	rBV	307	182	0.02%	0.002%
85	10.924	3072	3074	3076	rBV	224	101	0.01%	0.001%
86	11.062	3113	3117	3118	rBV	290	223	0.02%	0.003%
87	11.127	3133	3137	3144	rBV6	1894	2389	0.23%	0.031%
88	11.191	3146	3157	3180	rVV	438903	696734	67.81%	9.003%
89	11.422	3227	3229	3230	rBV	423	181	0.02%	0.002%
90	11.567	3262	3274	3297	rBV	449456	716483	69.74%	9.258%
91	11.799	3341	3346	3354	rBV4	460	767	0.07%	0.010%
92	11.898	3375	3377	3379	rBV2	377	181	0.02%	0.002%
93	12.284	3494	3497	3498	rBV2	507	327	0.03%	0.004%
94	12.387	3527	3529	3531	rBV2	492	252	0.02%	0.003%
95	12.628	3603	3604	3608	rBV3	452	285	0.03%	0.004%
96	13.014	3722	3724	3729	rBV3	372	175	0.02%	0.002%
97	13.599	3904	3906	3911	rVB	600	406	0.04%	0.005%
98	13.818	3972	3974	3978	rBV3	541	415	0.04%	0.005%
99	13.879	3990	3993	3997	rBV2	935	832	0.08%	0.011%
100	14.307	4124	4126	4127	rBV	853	349	0.03%	0.005%




Sum of corrected areas: 7738659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031493.D
Acq On : 09 Jun 2023 14:14
Operator : SY/MD
Sample : 03098-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

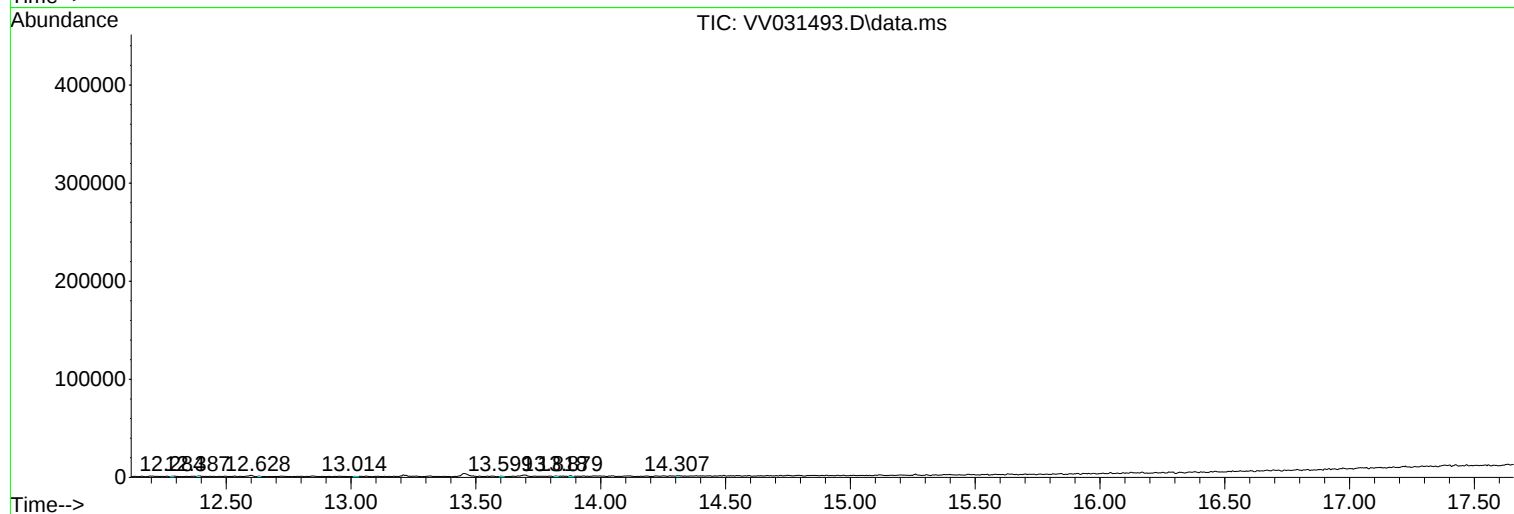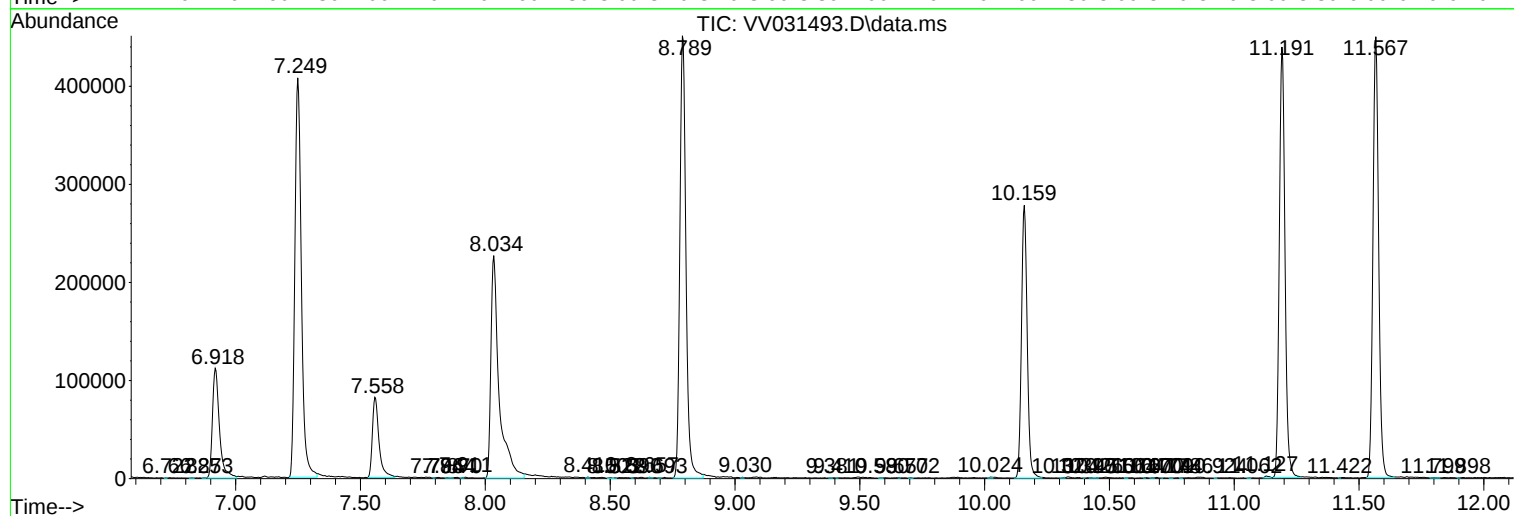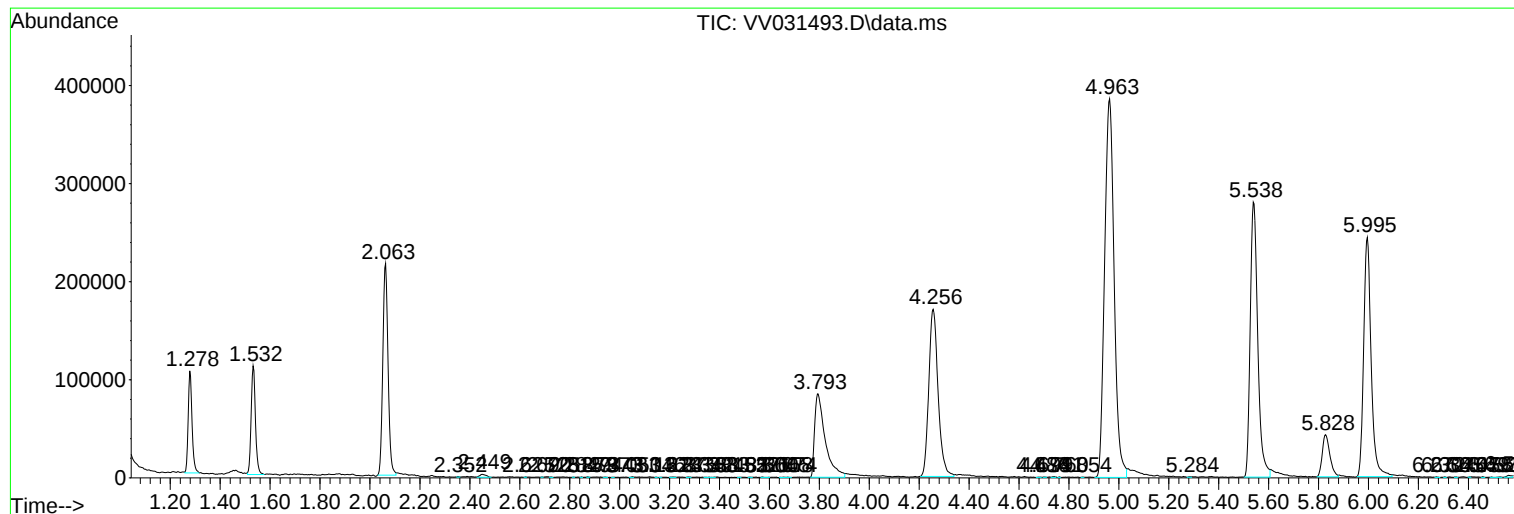

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031493.D
Acq On : 09 Jun 2023 14:14
Operator : SY/MD
Sample : 03098-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031493.D
Acq On : 09 Jun 2023 14:14
Operator : SY/MD
Sample : 03098-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc