

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031494.D
 Acq On : 09 Jun 2023 15:08
 Operator : SY/MD
 Sample : 03078-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESQX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	109227	119604	11.14%	1.484%
2	1.532	146	153	166	rVB	116714	137393	12.80%	1.704%
3	2.059	308	317	331	rBV	223482	323024	30.09%	4.007%
4	2.503	450	455	459	rBV3	625	694	0.06%	0.009%
5	2.635	495	496	499	rVB	585	199	0.02%	0.002%
6	2.658	499	503	506	rBV2	563	419	0.04%	0.005%
7	2.757	531	534	535	rBV2	452	172	0.02%	0.002%
8	2.838	558	559	563	rVB2	452	225	0.02%	0.003%
9	2.889	570	575	576	rBV	325	204	0.02%	0.003%
10	2.950	590	594	595	rBV	251	129	0.01%	0.002%
11	2.963	595	598	599	rVV2	323	146	0.01%	0.002%
12	2.985	602	605	608	rVB2	452	330	0.03%	0.004%
13	3.018	608	615	616	rBV	467	466	0.04%	0.006%
14	3.108	640	643	646	rBV3	621	374	0.03%	0.005%
15	3.178	663	665	671	rVB2	367	223	0.02%	0.003%
16	3.204	671	673	676	rBV2	425	279	0.03%	0.003%
17	3.252	686	688	690	rBV2	343	161	0.01%	0.002%
18	3.407	733	736	740	rVB	336	243	0.02%	0.003%
19	3.426	740	742	743	rBV	245	125	0.01%	0.002%
20	3.468	752	755	759	rVB2	433	317	0.03%	0.004%
21	3.500	760	765	768	rBV2	204	241	0.02%	0.003%
22	3.558	780	783	785	rBV2	238	150	0.01%	0.002%
23	3.641	807	809	812	rBV	495	275	0.03%	0.003%
24	3.744	838	841	843	rBV	373	240	0.02%	0.003%
25	3.793	846	856	897	rVV	78853	242336	22.57%	3.006%
26	4.252	982	999	1023	rBV	170541	457883	42.65%	5.680%
27	4.664	1123	1127	1130	rBV3	515	424	0.04%	0.005%
28	4.706	1135	1140	1142	rBV4	577	460	0.04%	0.006%
29	4.731	1146	1148	1152	rBV	359	260	0.02%	0.003%
30	4.770	1158	1160	1162	rBV	368	171	0.02%	0.002%
31	4.883	1193	1195	1198	rBV	347	235	0.02%	0.003%
32	4.960	1202	1219	1258	rBV2	392178	1073482	100.00%	13.317%
33	5.294	1321	1323	1324	rBV2	565	180	0.02%	0.002%
34	5.365	1343	1345	1347	rBV3	407	140	0.01%	0.002%
35	5.416	1358	1361	1363	rBV2	411	251	0.02%	0.003%
36	5.461	1371	1375	1376	rBV3	401	245	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031494.D
 Acq On : 09 Jun 2023 15:08
 Operator : SY/MD
 Sample : 03078-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESQX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.484	1380	1382	1385	rVB2	616	306	0.03%	0.004%
38	5.535	1385	1398	1423	rBV	309212	655588	61.07%	8.133%
39	5.825	1476	1488	1510	rBV2	61429	131062	12.21%	1.626%
40	5.992	1526	1540	1575	rBV	252165	535053	49.84%	6.638%
41	6.336	1645	1647	1650	rBV2	406	195	0.02%	0.002%
42	6.374	1657	1659	1662	rBV	225	128	0.01%	0.002%
43	6.436	1676	1678	1681	rBV2	327	136	0.01%	0.002%
44	6.506	1697	1700	1703	rVB3	489	330	0.03%	0.004%
45	6.561	1712	1717	1722	rBV3	1614	2412	0.22%	0.030%
46	6.638	1738	1741	1743	rBV3	600	401	0.04%	0.005%
47	6.709	1760	1763	1767	rBV2	541	531	0.05%	0.007%
48	6.866	1810	1812	1816	rBV	469	328	0.03%	0.004%
49	6.915	1816	1827	1854	rBV	114348	224072	20.87%	2.780%
50	7.246	1918	1930	1958	rBV	407301	744558	69.36%	9.237%
51	7.558	2015	2027	2049	rBV	85754	158631	14.78%	1.968%
52	7.937	2142	2145	2146	rBV	312	170	0.02%	0.002%
53	7.979	2153	2158	2162	rBV4	581	521	0.05%	0.006%
54	8.034	2162	2175	2212	rBV2	209282	506868	47.22%	6.288%
55	8.445	2300	2303	2305	rBV2	607	433	0.04%	0.005%
56	8.455	2305	2306	2310	rVV3	562	341	0.03%	0.004%
57	8.551	2333	2336	2340	rBV3	788	594	0.06%	0.007%
58	8.612	2351	2355	2358	rBV2	473	348	0.03%	0.004%
59	8.667	2367	2372	2375	rBV3	732	498	0.05%	0.006%
60	8.731	2388	2392	2393	rBV2	415	301	0.03%	0.004%
61	8.789	2398	2410	2433	rBV	503208	830610	77.38%	10.304%
62	9.024	2481	2483	2485	rBV	385	170	0.02%	0.002%
63	9.185	2529	2533	2535	rBV	320	284	0.03%	0.004%
64	9.194	2535	2536	2538	rBV	428	175	0.02%	0.002%
65	9.384	2593	2595	2597	rBV	294	135	0.01%	0.002%
66	9.423	2605	2607	2608	rBV	360	144	0.01%	0.002%
67	9.458	2616	2618	2620	rBV3	425	207	0.02%	0.003%
68	9.558	2646	2649	2651	rBV3	489	346	0.03%	0.004%
69	9.644	2674	2676	2679	rBV2	452	210	0.02%	0.003%
70	9.673	2682	2685	2687	rBV3	284	226	0.02%	0.003%
71	9.795	2720	2723	2726	rBV	403	309	0.03%	0.004%
72	9.860	2739	2743	2745	rBV2	453	415	0.04%	0.005%
73	9.873	2745	2747	2753	rVB3	936	675	0.06%	0.008%
74	9.998	2784	2786	2788	rBV3	298	180	0.02%	0.002%
75	10.104	2817	2819	2823	rBV2	404	191	0.02%	0.002%
76	10.159	2823	2836	2859	rBV	240203	388111	36.15%	4.815%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
 Data File : VV031494.D
 Acq On : 09 Jun 2023 15:08
 Operator : SY/MD
 Sample : 03078-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ESQX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.284	2871	2875	2878	rBV3	564	468	0.04%	0.006%
78	10.332	2883	2890	2901	rVB3	3860	6347	0.59%	0.079%
79	10.413	2913	2915	2917	rBV	320	129	0.01%	0.002%
80	10.850	3048	3051	3053	rBV2	539	391	0.04%	0.005%
81	10.988	3092	3094	3098	rBV	380	258	0.02%	0.003%
82	11.027	3101	3106	3107	rBV2	502	418	0.04%	0.005%
83	11.069	3117	3119	3123	rVB2	332	165	0.02%	0.002%
84	11.191	3145	3157	3185	rBV	485773	769625	71.69%	9.548%
85	11.442	3233	3235	3237	rVV2	534	233	0.02%	0.003%
86	11.567	3261	3274	3295	rBV	459065	725952	67.63%	9.006%
87	11.673	3305	3307	3311	rBV3	700	528	0.05%	0.007%
88	11.754	3330	3332	3335	rBB2	367	149	0.01%	0.002%
89	11.770	3335	3337	3338	rBV	373	137	0.01%	0.002%
90	12.239	3481	3483	3485	rBV	412	164	0.02%	0.002%
91	12.731	3633	3636	3638	rBV	508	317	0.03%	0.004%
92	12.818	3662	3663	3666	rBV2	386	226	0.02%	0.003%
93	12.856	3673	3675	3678	rBV2	410	283	0.03%	0.004%
94	12.905	3688	3690	3692	rBV2	520	205	0.02%	0.003%
95	13.053	3733	3736	3738	rBV	476	299	0.03%	0.004%
96	13.217	3782	3787	3792	rVB5	1555	1784	0.17%	0.022%
97	13.455	3854	3861	3869	rBV7	1970	3444	0.32%	0.043%
98	13.583	3900	3901	3902	rBV7	384	132	0.01%	0.002%
99	13.975	4021	4023	4025	rBV	771	455	0.04%	0.006%
100	14.464	4173	4175	4180	rBV4	994	728	0.07%	0.009%


Sum of corrected areas: 8060730

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031494.D
Acq On : 09 Jun 2023 15:08
Operator : SY/MD
Sample : 03078-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESQX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

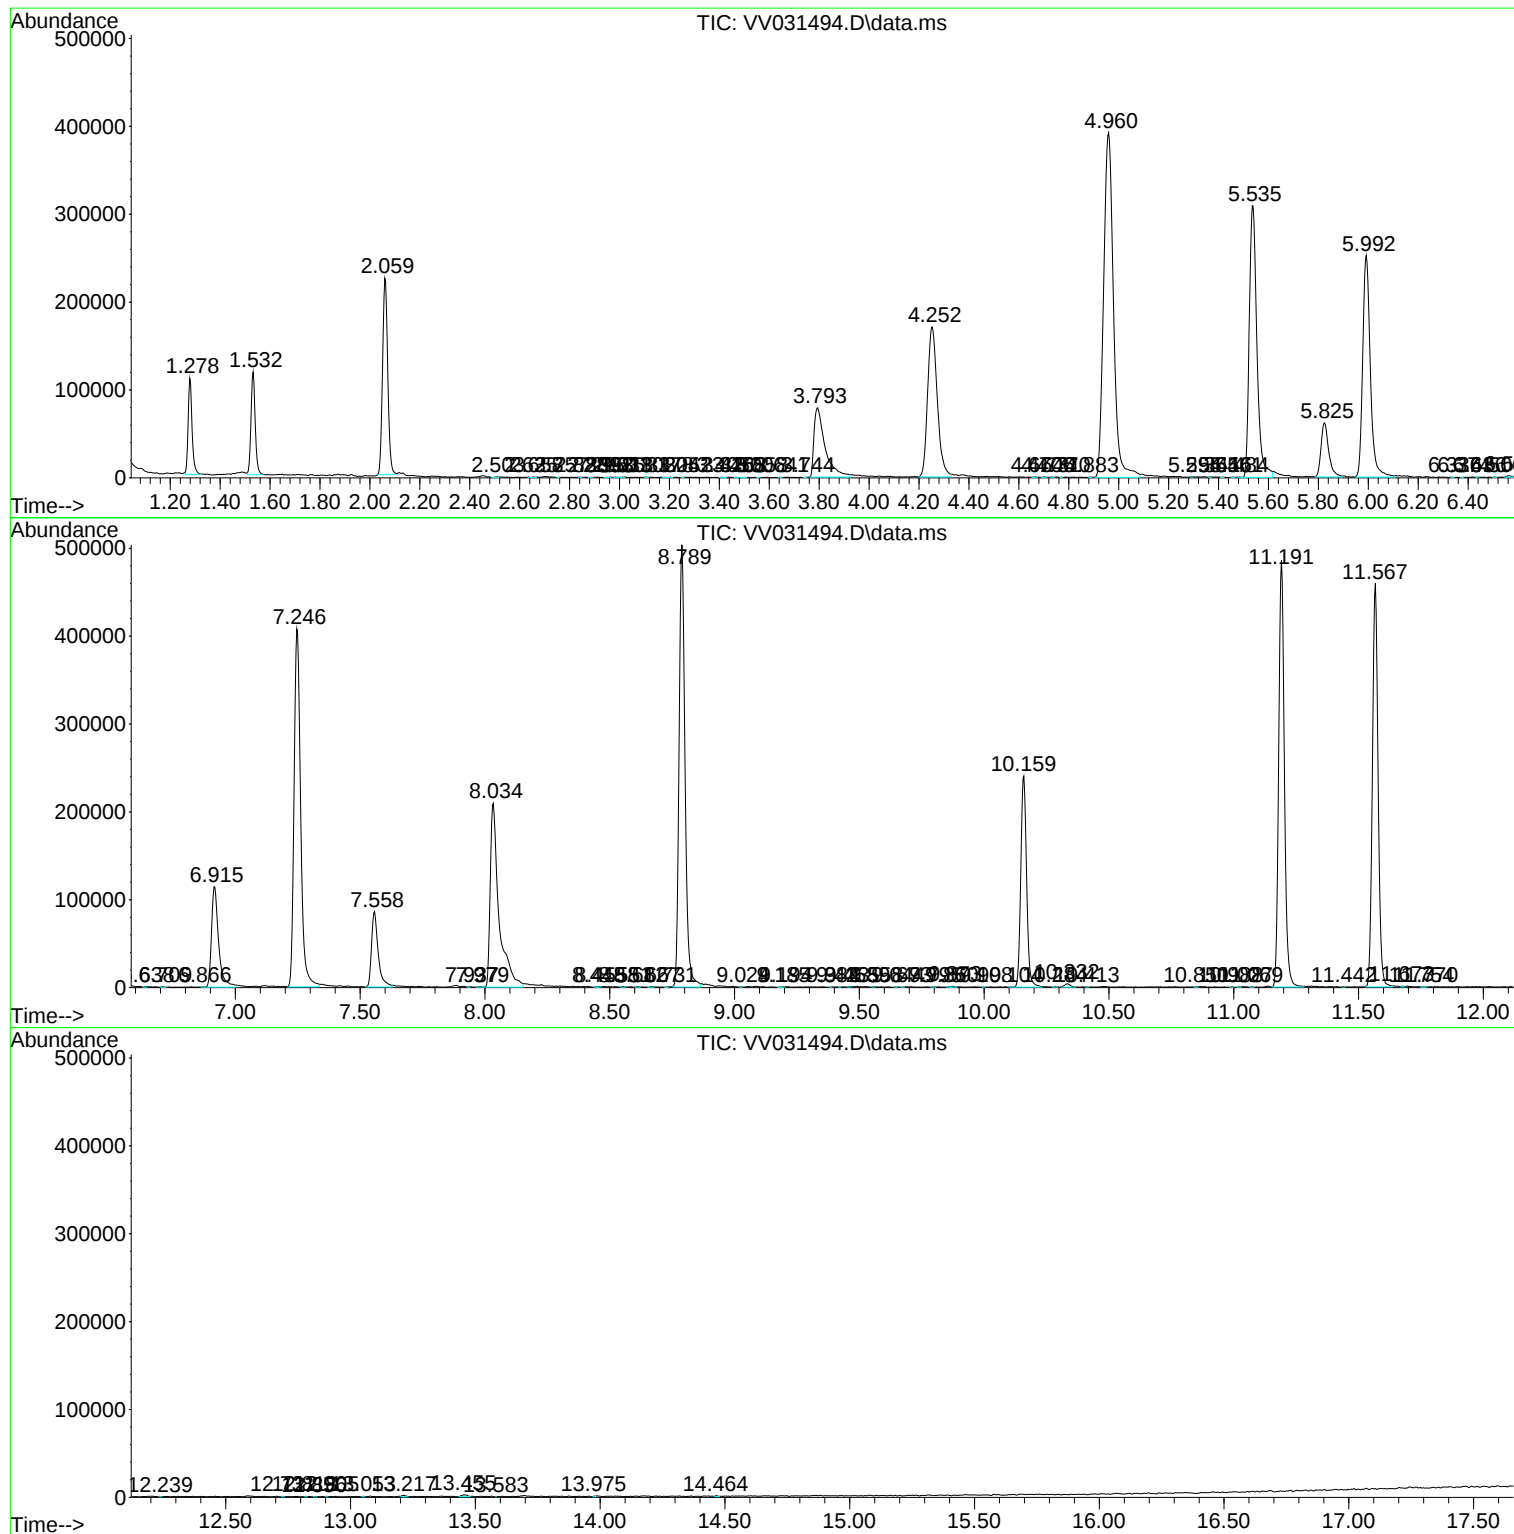

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031494.D
Acq On : 09 Jun 2023 15:08
Operator : SY/MD
Sample : 03078-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESQX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031494.D
Acq On : 09 Jun 2023 15:08
Operator : SY/MD
Sample : 03078-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ESQX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc