
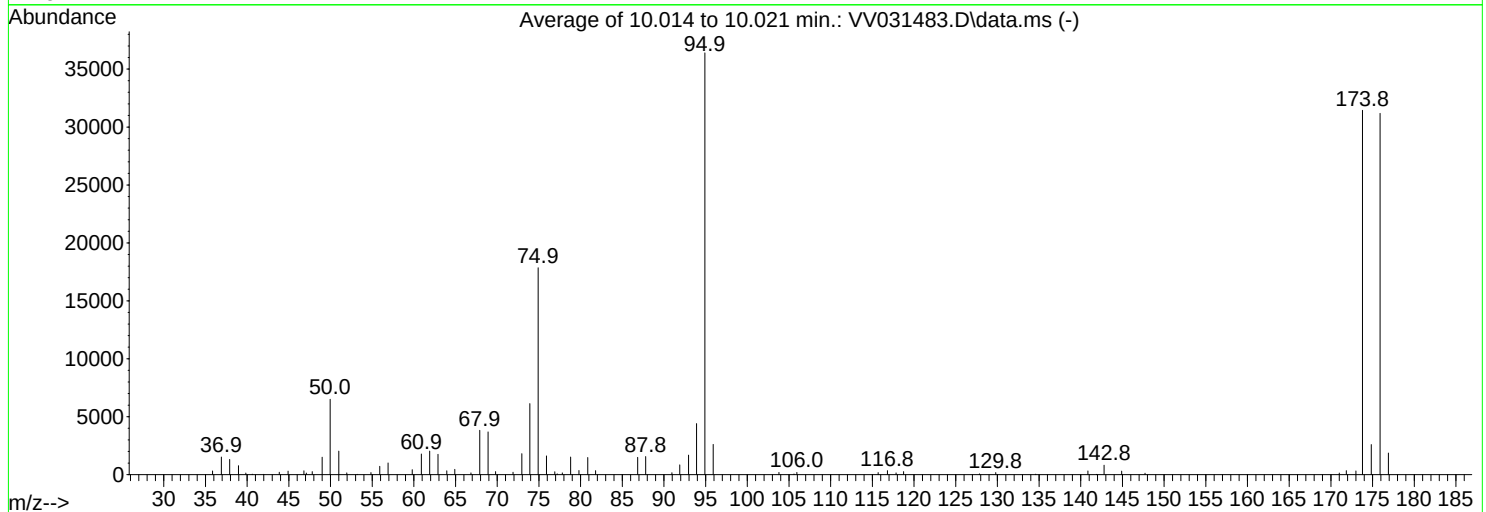


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060923\
Data File : VV031483.D
Acq On : 09 Jun 2023 08:55
Operator : SY/MD
Sample : BFB384
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB384

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Title : VOC Analysis
Last Update : Sat Jun 10 01:38:32 2023

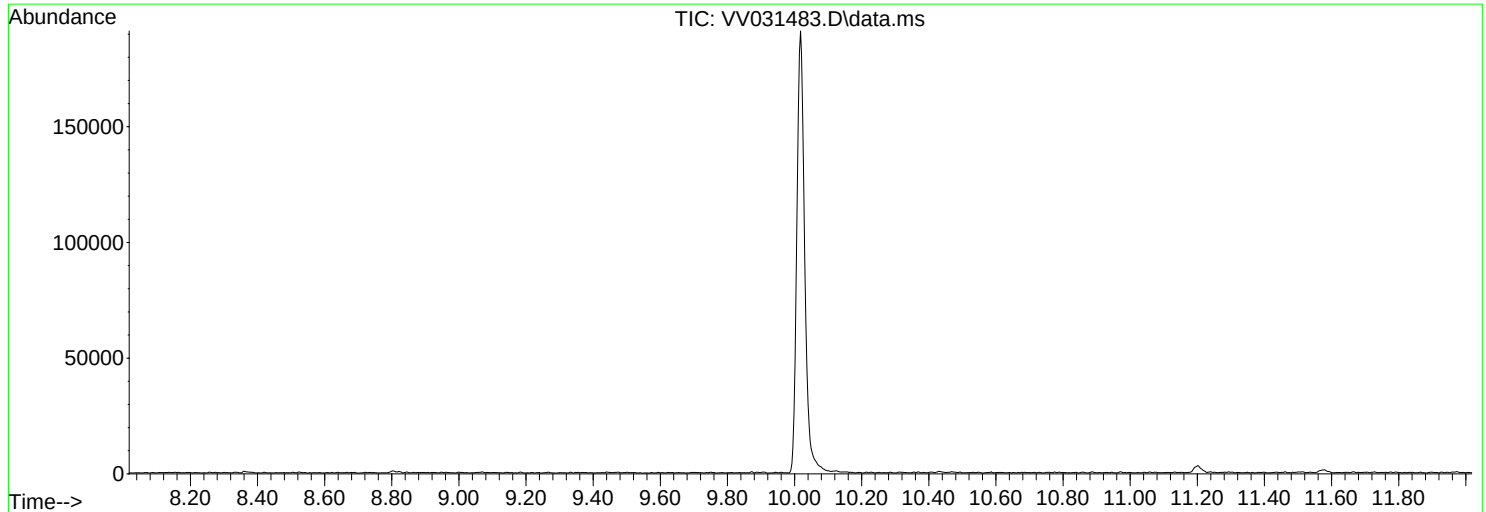

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	6510	PASS
75	95	30	80	49.0	17853	PASS
95	95	100	100	100.0	36405	PASS
96	95	5	9	7.2	2617	PASS
173	174	0.00	2	1.0	321	PASS
174	95	50	120	86.4	31443	PASS
175	174	5	9	8.3	2598	PASS
176	174	95	105	99.2	31184	PASS
177	176	5	10	6.0	1869	PASS

m/z	Abundance
39.90	175.0
43.80	269.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
35.90	294.0
36.90	1449.0
37.90	1446.0
39.00	787.0
39.80	274.0
43.90	504.0
44.90	314.0
47.10	412.0
47.80	220.0
49.00	1461.0
50.00	6692.0
51.00	1953.0
52.00	157.0
54.90	189.0
55.90	721.0
56.90	1000.0
59.80	429.0
60.90	1882.0
61.90	2166.0
62.90	1777.0
64.00	348.0
64.90	350.0
67.00	129.0
67.90	3746.0
68.90	3617.0
69.80	289.0
71.90	188.0
73.00	1710.0
73.90	5966.0
74.90	17760.0
75.90	1650.0
76.90	249.0
77.80	181.0
78.80	1484.0
79.80	343.0
80.90	1520.0
81.80	360.0
86.80	1603.0
87.80	1602.0
91.00	159.0
91.90	913.0
92.90	1661.0
93.90	4240.0
94.90	36536.0
95.90	2486.0
103.80	182.0
105.60	161.0
106.00	201.0
115.70	234.0
116.80	332.0
117.80	146.0
118.80	265.0
127.90	117.0
129.80	170.0
140.80	270.0
142.80	830.0
144.80	280.0
147.70	115.0
171.00	133.0
171.80	327.0
173.00	482.0
173.80	30280.0
174.80	2545.0
175.90	29992.0
176.90	1795.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
35.90	301.0
36.90	1567.0
37.90	1297.0
38.90	786.0
39.90	345.0
42.00	104.0
43.90	496.0
44.90	319.0
46.80	466.0
47.80	287.0
49.00	1559.0
49.90	6735.0
51.00	2074.0
51.90	151.0
53.20	102.0
54.90	205.0
55.90	778.0
56.90	1049.0
59.80	468.0
60.90	1817.0
61.90	2125.0
62.90	1831.0
64.00	335.0
64.90	462.0
66.80	157.0
67.90	3918.0
68.90	3775.0
69.80	275.0
71.90	226.0
72.90	1898.0
73.90	6345.0
74.90	18312.0
75.90	1678.0
76.90	259.0
77.80	160.0
78.80	1516.0
79.80	384.0
80.80	1511.0
81.80	351.0
86.80	1502.0
87.80	1667.0
91.00	151.0
91.90	864.0
92.90	1700.0
93.90	4618.0
94.90	37712.0
95.90	2759.0
103.80	202.0
105.90	224.0
115.70	205.0
116.80	352.0
117.90	171.0
118.80	259.0
129.80	170.0
140.80	307.0
142.80	870.0
144.90	311.0
147.70	130.0
171.00	143.0
171.90	356.0
173.00	482.0
173.80	32656.0
174.80	2754.0
175.90	32408.0
176.90	1971.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384

m/z	Abundance
35.80	368.0
36.90	1561.0
37.90	1175.0
38.90	765.0
39.90	340.0
40.60	132.0
44.00	429.0
44.90	275.0
46.80	540.0
47.80	296.0
49.00	1508.0
49.90	6104.0
51.00	2079.0
51.90	132.0
54.80	159.0
55.90	638.0
56.90	988.0
59.80	372.0
60.90	1645.0
61.90	1802.0
62.90	1666.0
63.90	305.0
64.90	554.0
66.80	159.0
67.90	3809.0
68.90	3660.0
69.80	226.0
71.90	211.0
72.90	1808.0
73.90	6085.0
74.90	17488.0
75.90	1508.0
76.90	232.0
77.20	227.0
77.80	136.0
78.80	1542.0
79.80	361.0
80.80	1392.0
81.80	315.0
86.90	1356.0
87.80	1414.0
90.90	173.0
91.90	757.0
93.00	1687.0
93.90	4367.0
94.90	34968.0
95.90	2607.0
103.80	190.0
105.90	169.0
115.70	116.0
116.80	356.0
117.90	140.0
118.70	263.0
127.80	111.0
129.80	198.0
134.60	114.0
140.90	372.0
141.90	101.0
142.80	742.0
145.00	335.0
147.70	124.0
171.00	147.0
171.90	367.0
173.80	31392.0
174.90	2494.0
175.90	31152.0
176.90	1842.0

Instrument :
MSVOA_V
ClientSampleId :
BFB384