




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038763.D
Acq On : 09 Jun 2025 11:32
Operator : SY/MD
Sample : VSTD00519
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD005219

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 08:50:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 08:48:48 2025
Response via : Initial Calibration

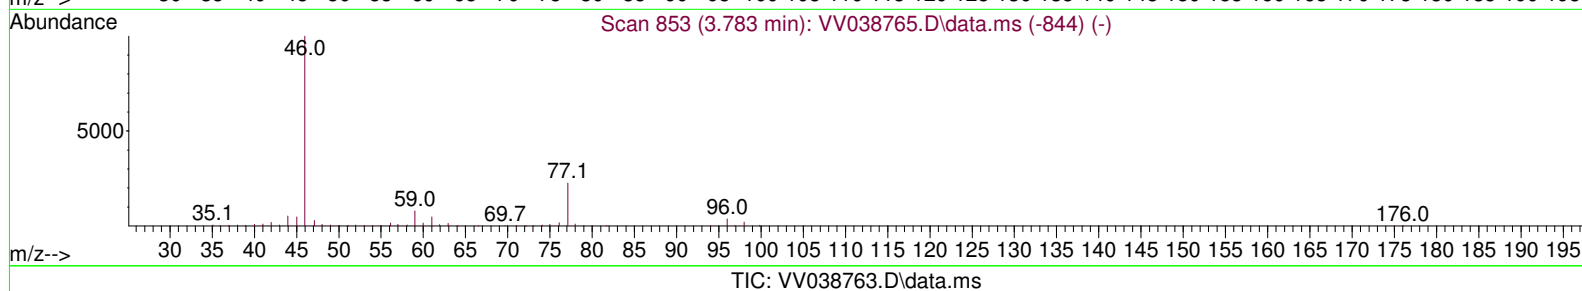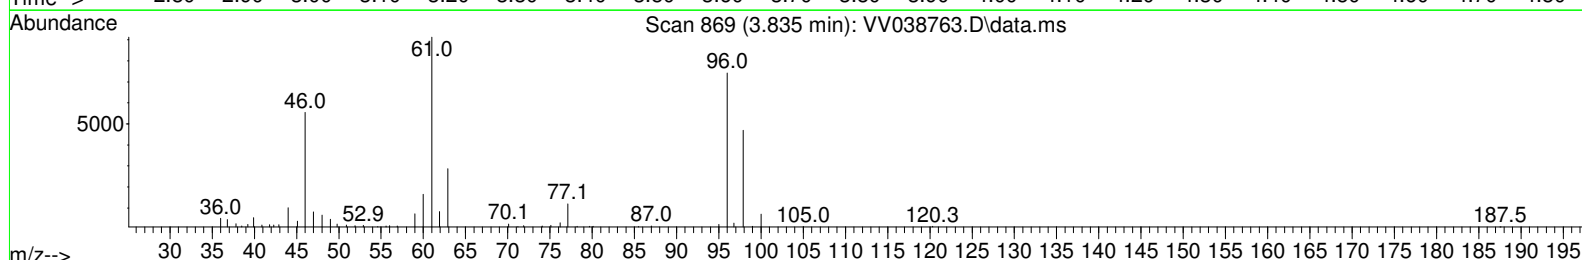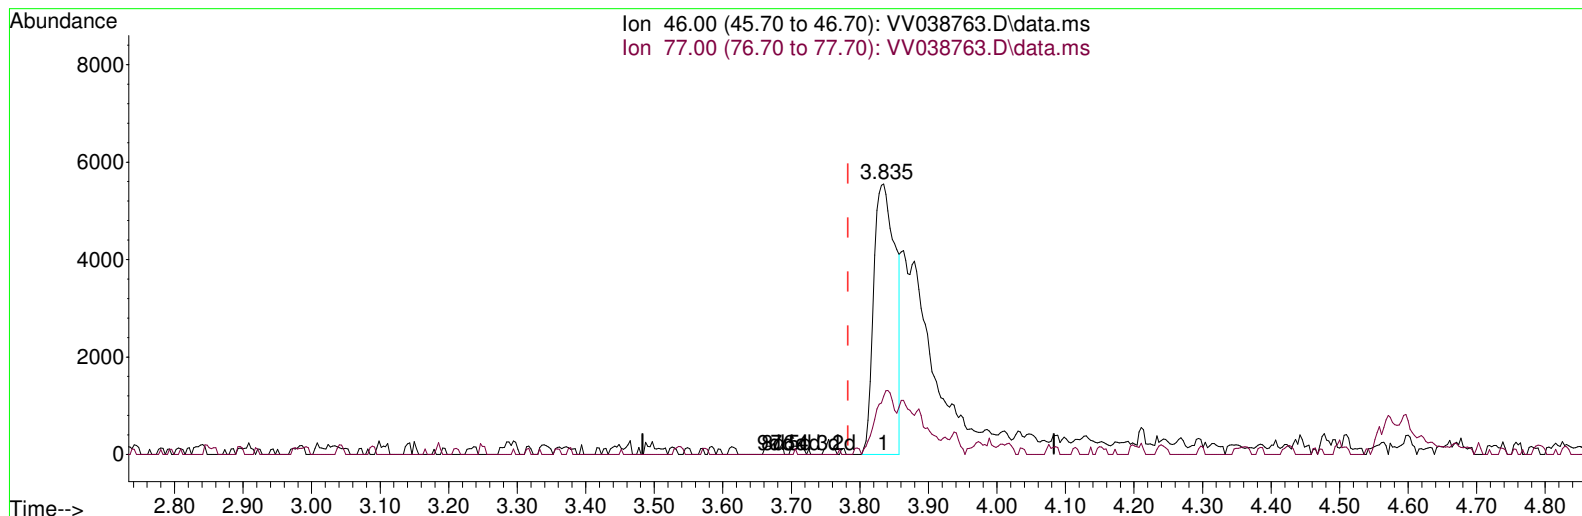

(21) 2-Butanone-d5 (S)

3.835min (+ 0.052) 7.69 ug/L

response 12133

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.30	20.94
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038763.D
Acq On : 09 Jun 2025 11:32
Operator : SY/MD
Sample : VSTD00519
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD005219

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 08:50:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 08:48:48 2025
Response via : Initial Calibration

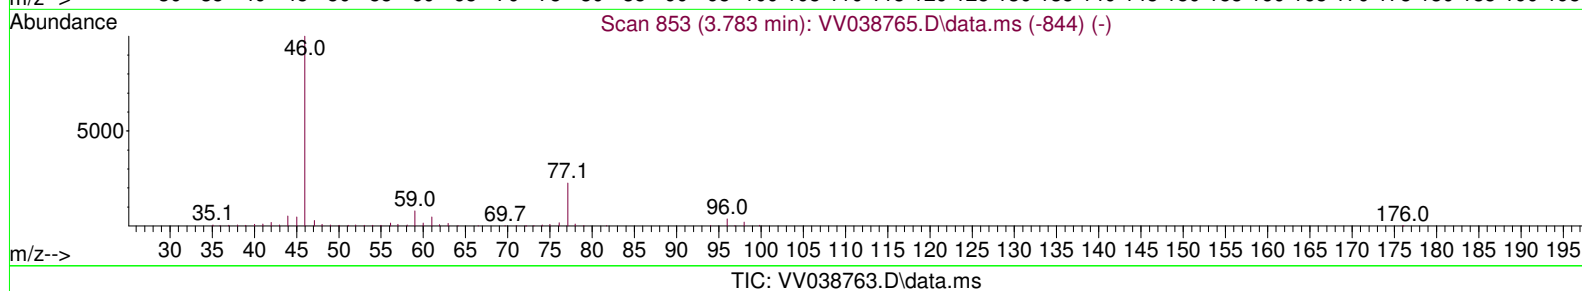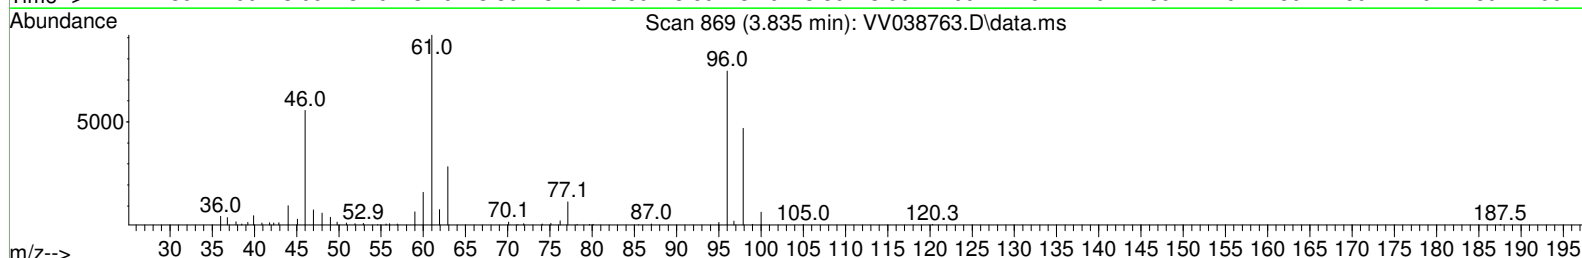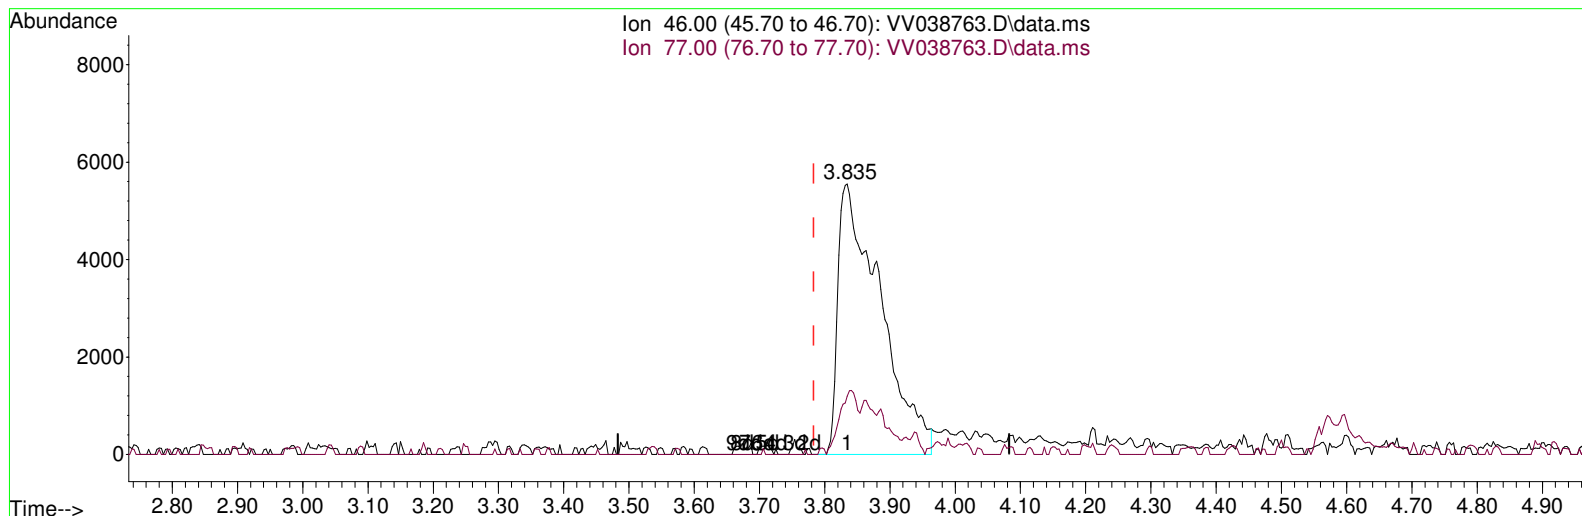

(21) 2-Butanone-d5 (S)

3.835min (+ 0.052) 15.82 ug/L m

response 24964

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.30	10.18#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038763.D
Acq On : 09 Jun 2025 11:32
Operator : SY/MD
Sample : VSTD00519
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD005219

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 08:50:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 08:48:48 2025
Response via : Initial Calibration

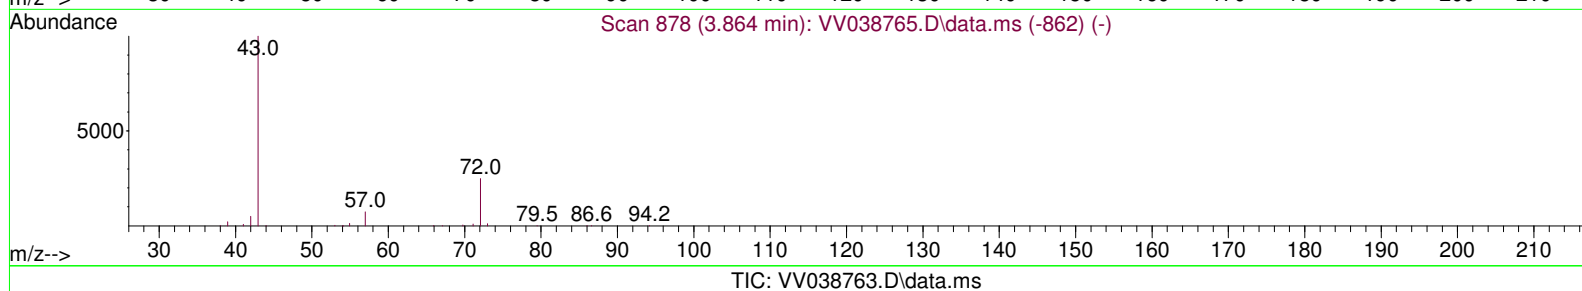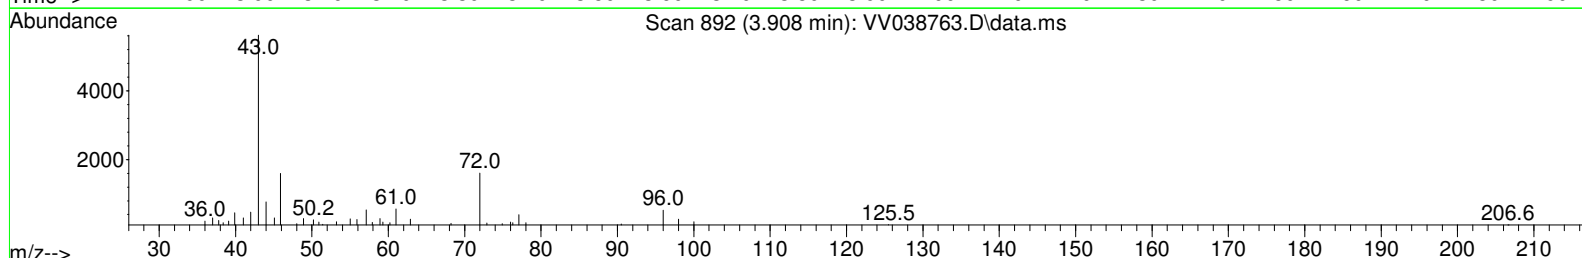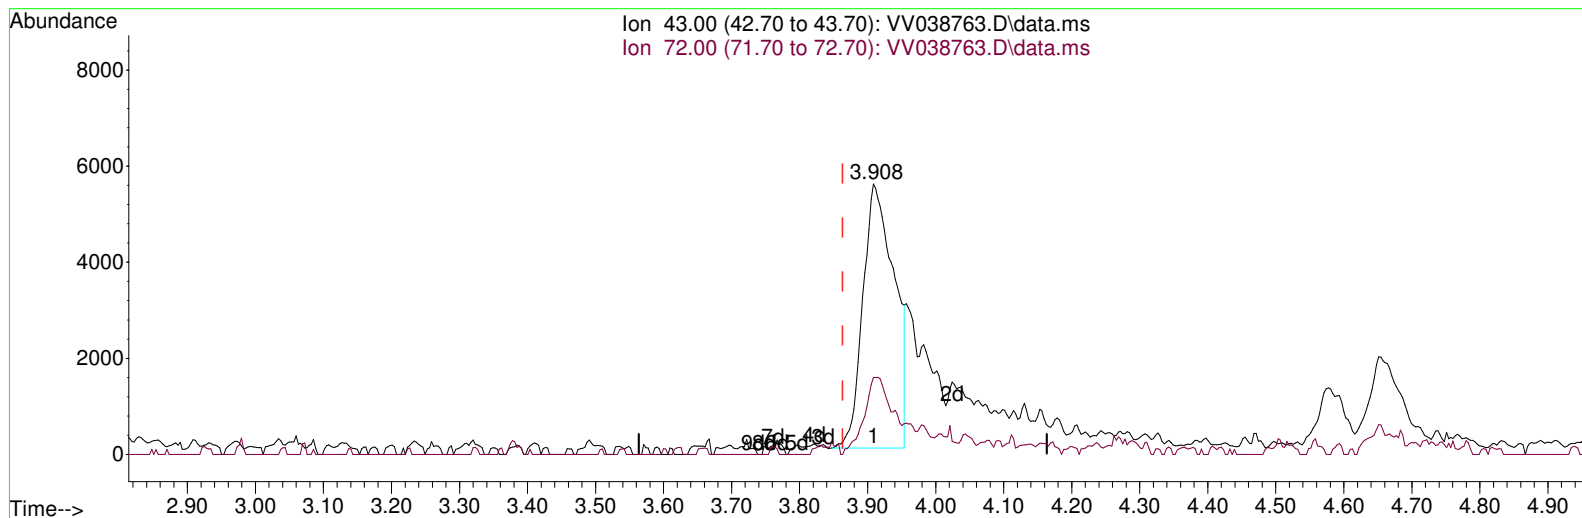

(22) 2-Butanone (T)

3.908min (+ 0.045) 9.61 ug/L

response 17525

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	22.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038763.D
Acq On : 09 Jun 2025 11:32
Operator : SY/MD
Sample : VSTD00519
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD005219

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 08:50:29 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 08:48:48 2025
Response via : Initial Calibration

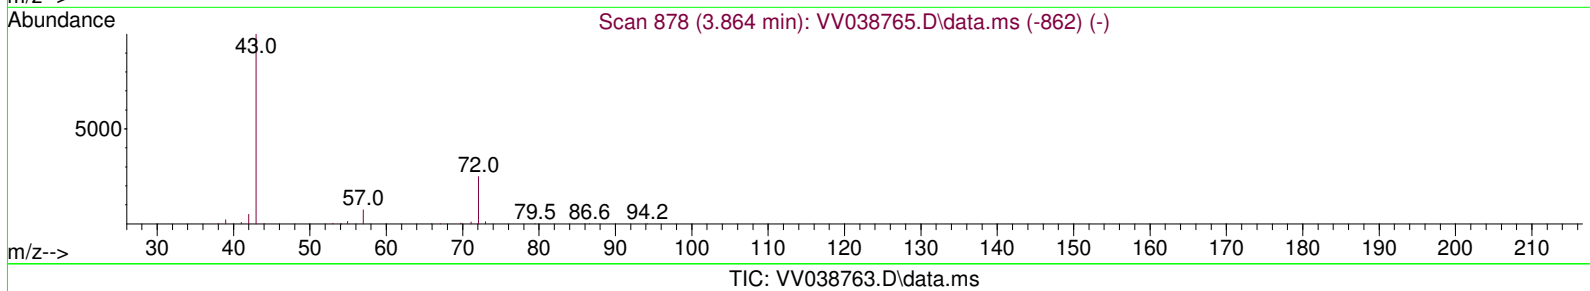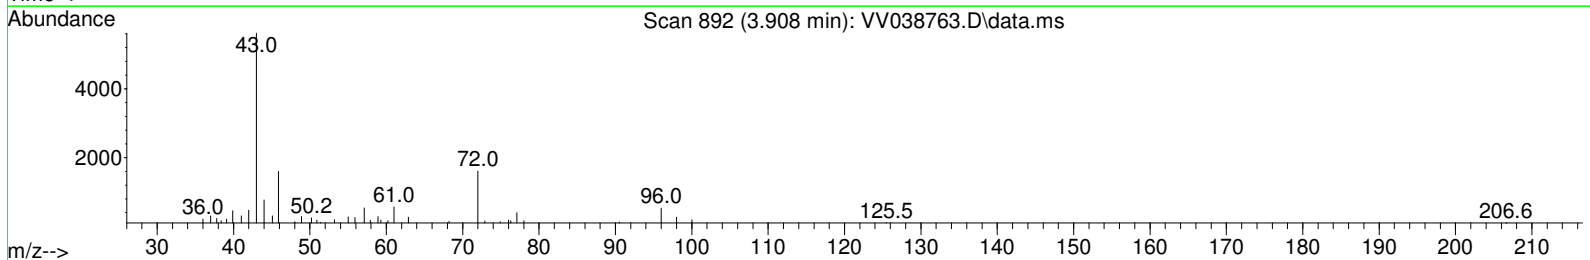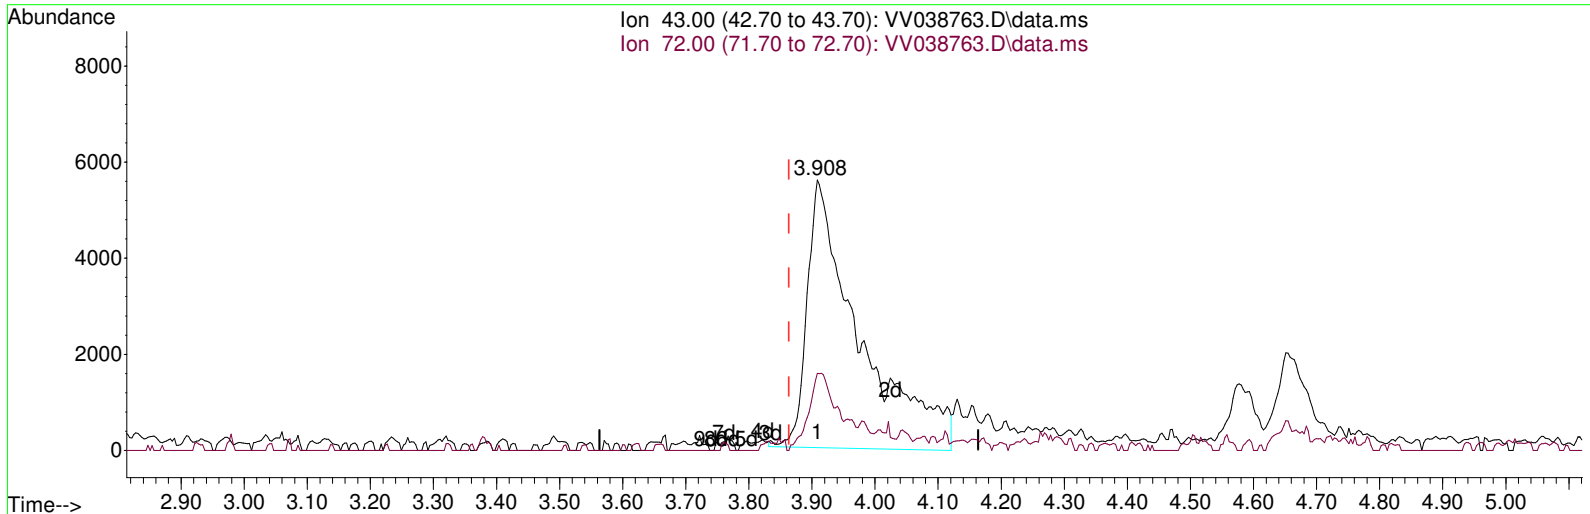

(22) 2-Butanone (T)

3.908min (+ 0.045) 17.61 ug/L m

response 32109

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	12.32#
0.00	0.00	0.00
0.00	0.00	0.00