




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

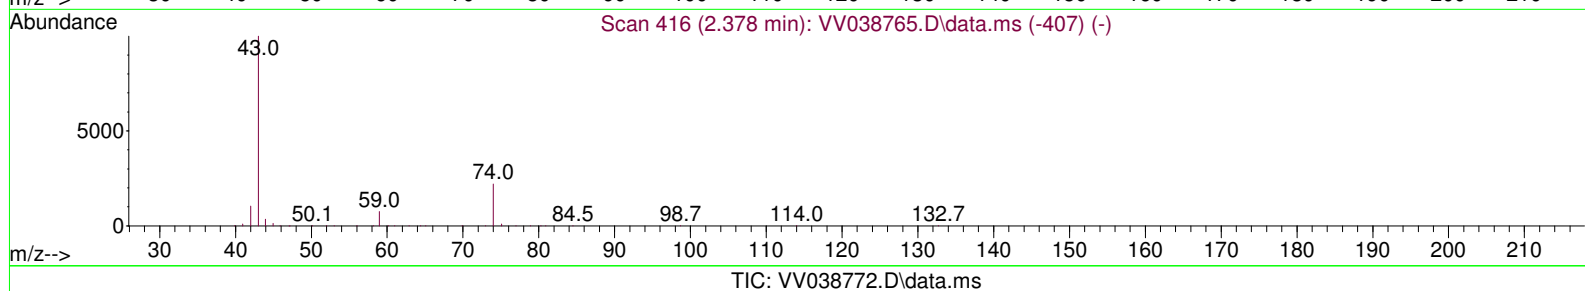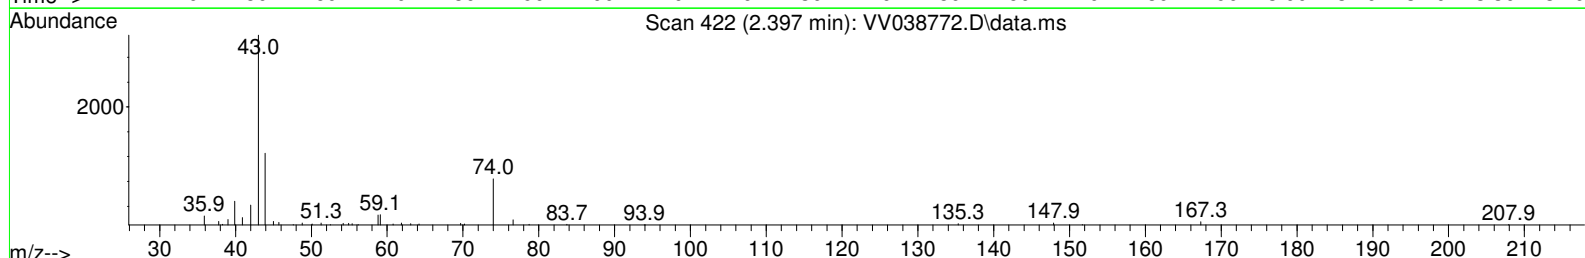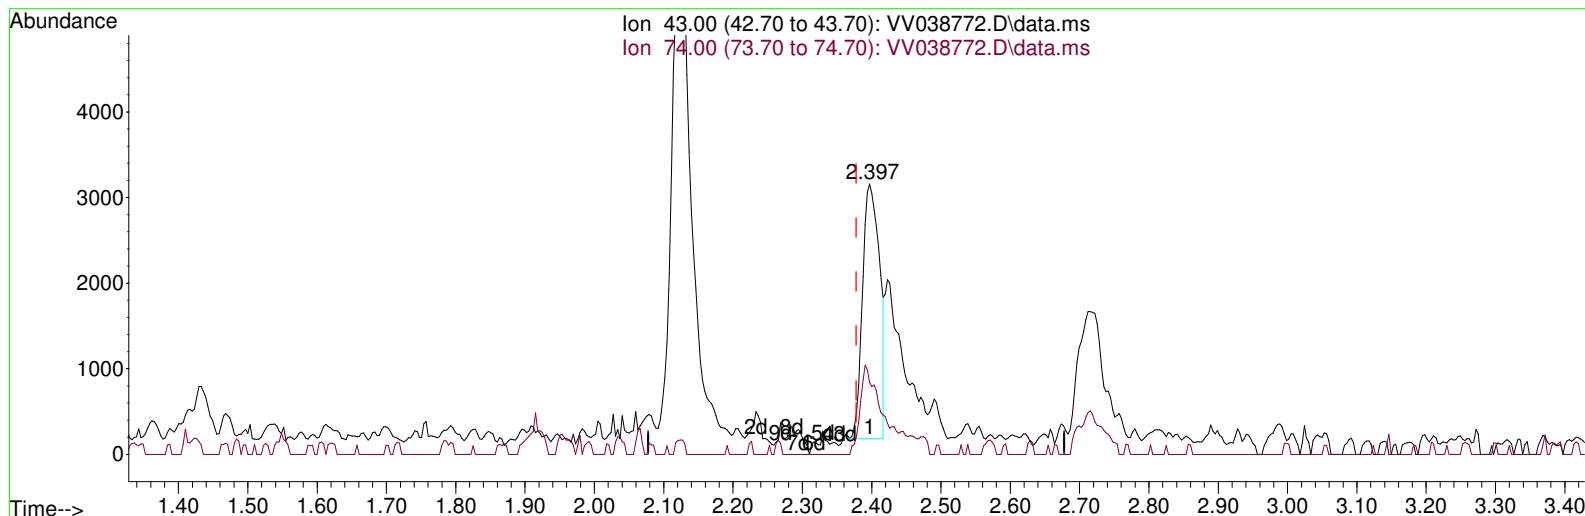

(15) Methyl Acetate (T)

2.397min (+ 0.019) 0.82 ug/L

response 5087

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.80	22.63
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

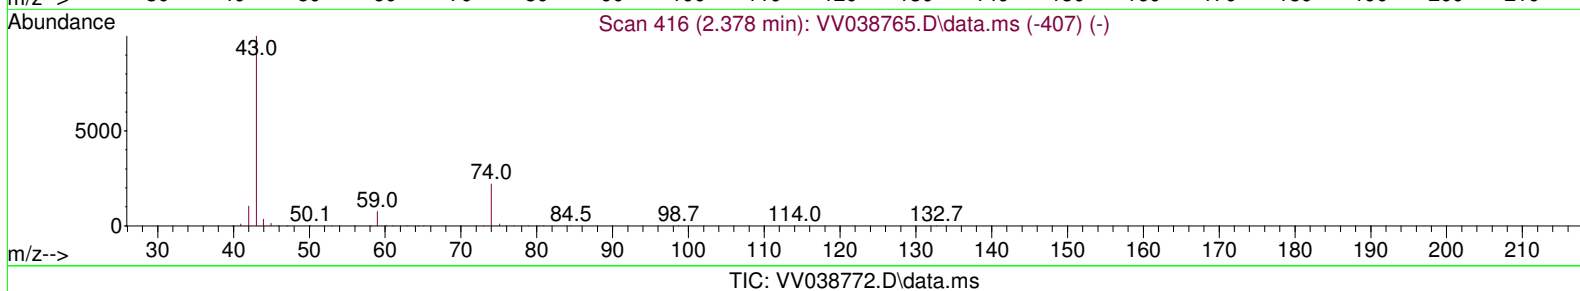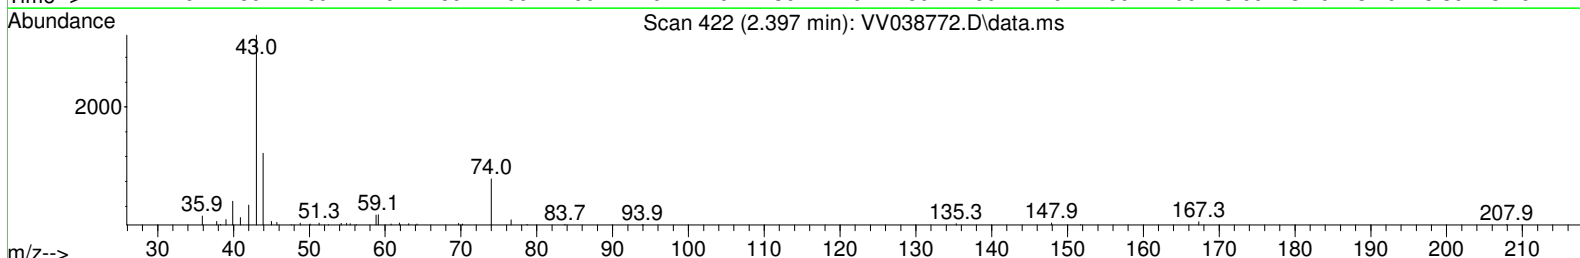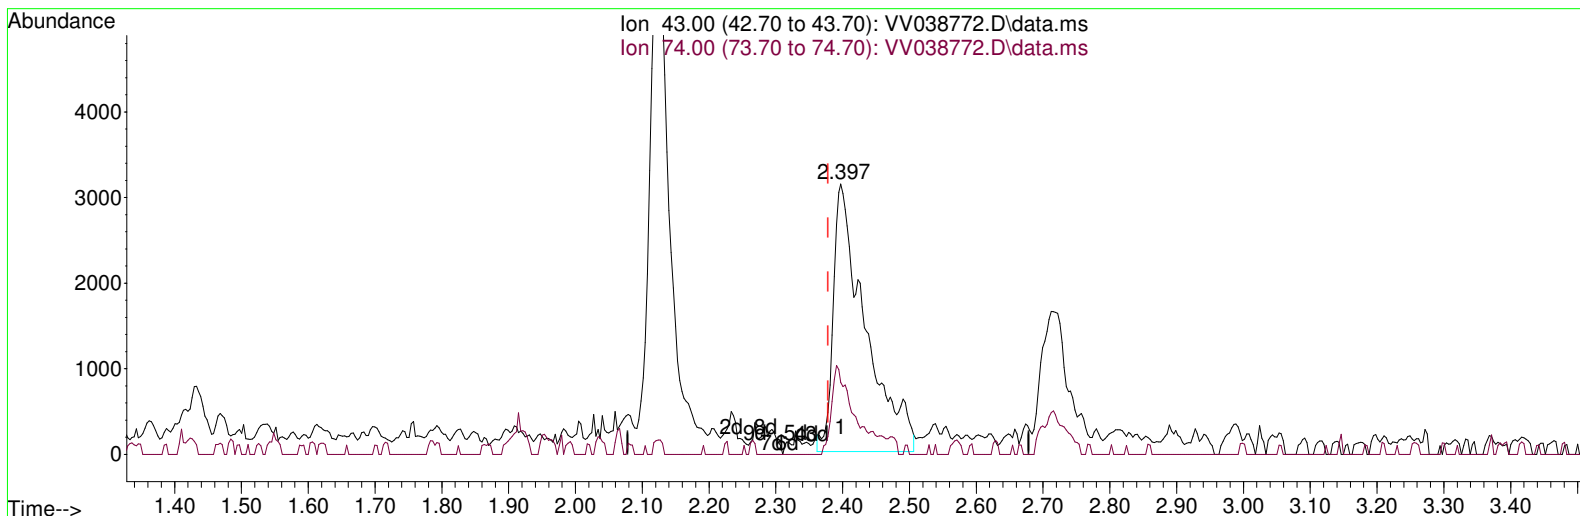

(15) Methyl Acetate (T)

2.397min (+ 0.019) 1.67 ug/L m

response 10386

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	25.80	11.08#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

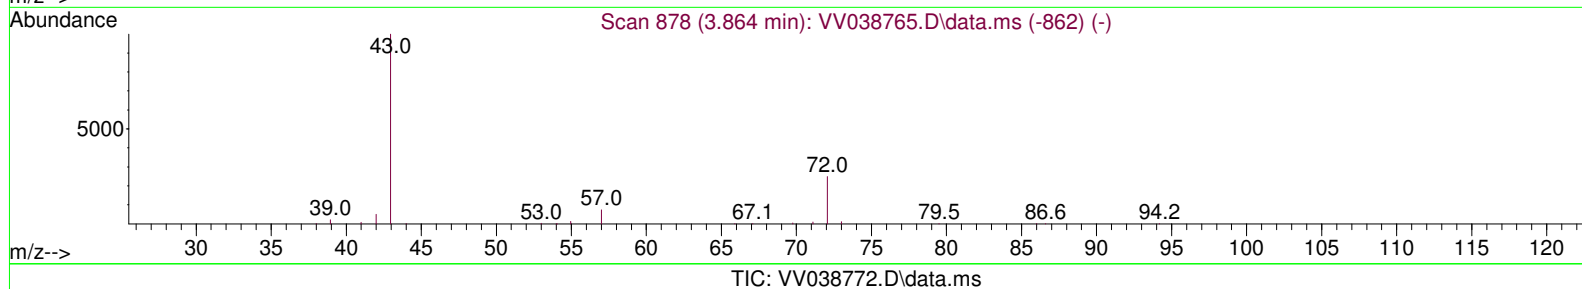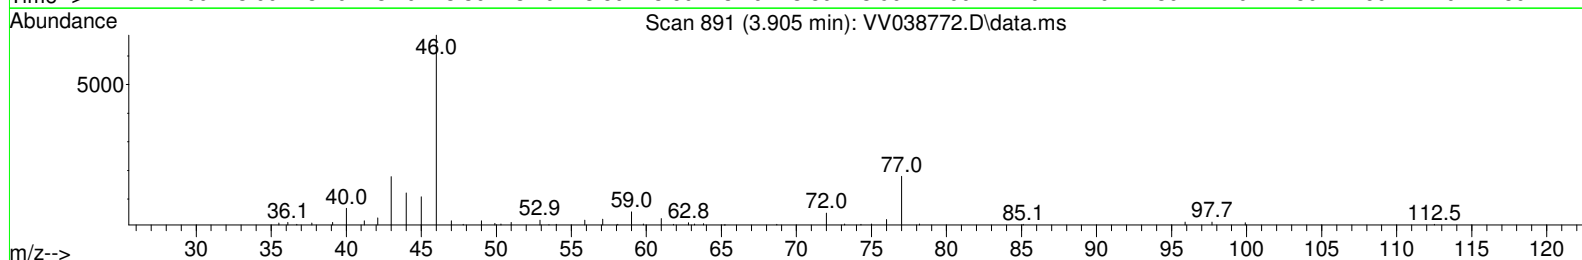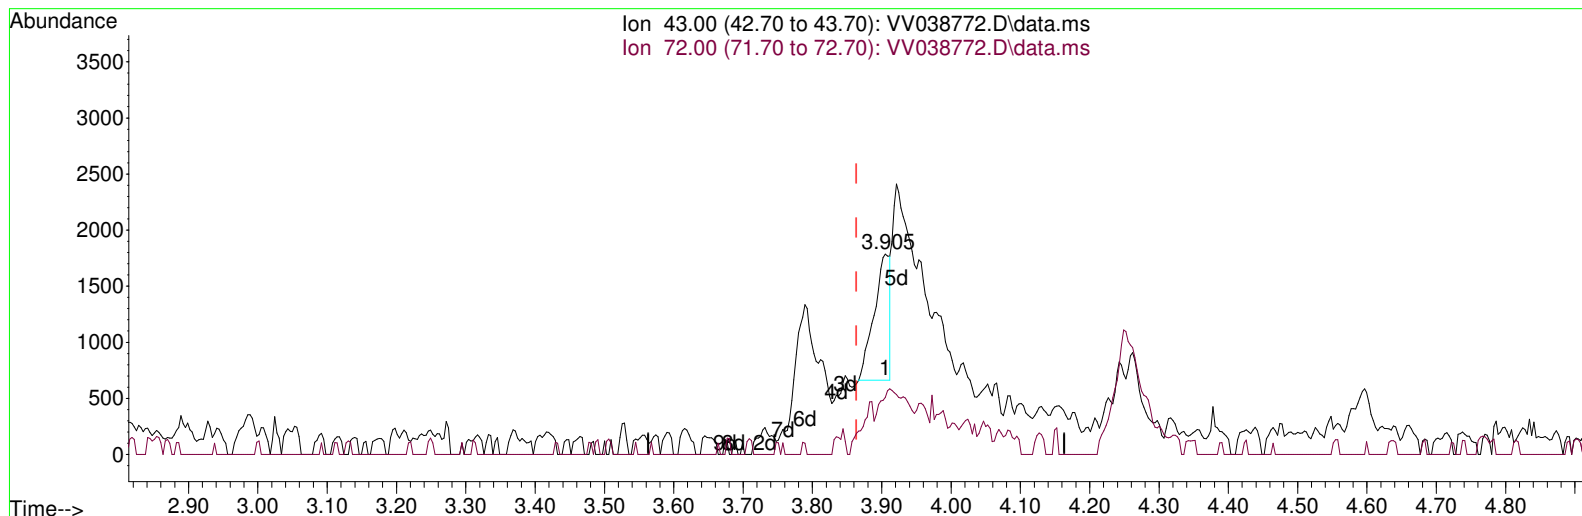

(22) 2-Butanone (T)

3.905min (+ 0.042) 0.48 ug/L

response 1772

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	27.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

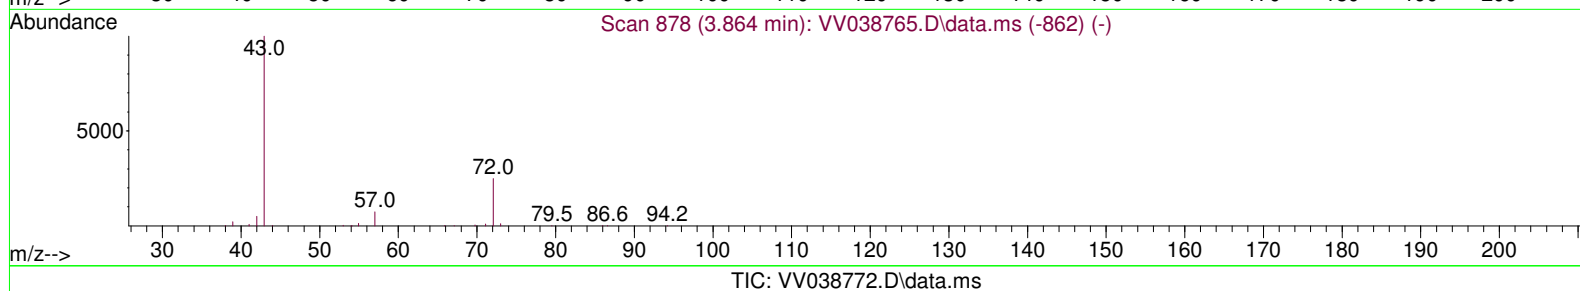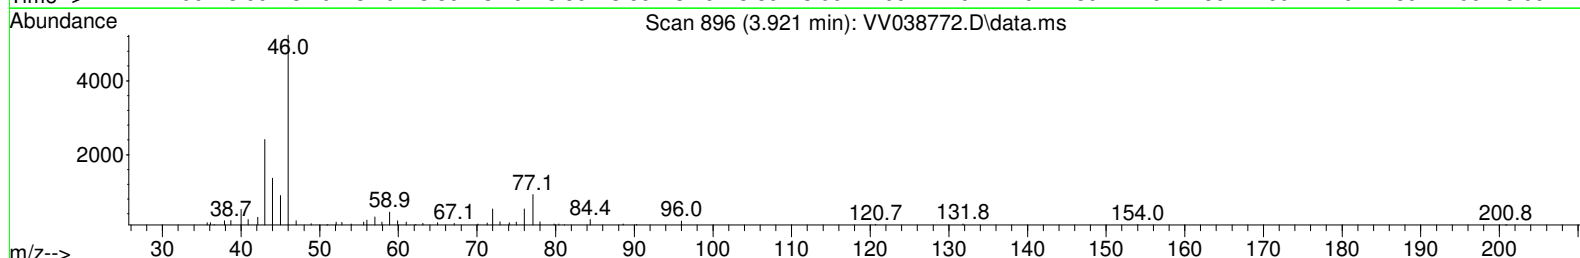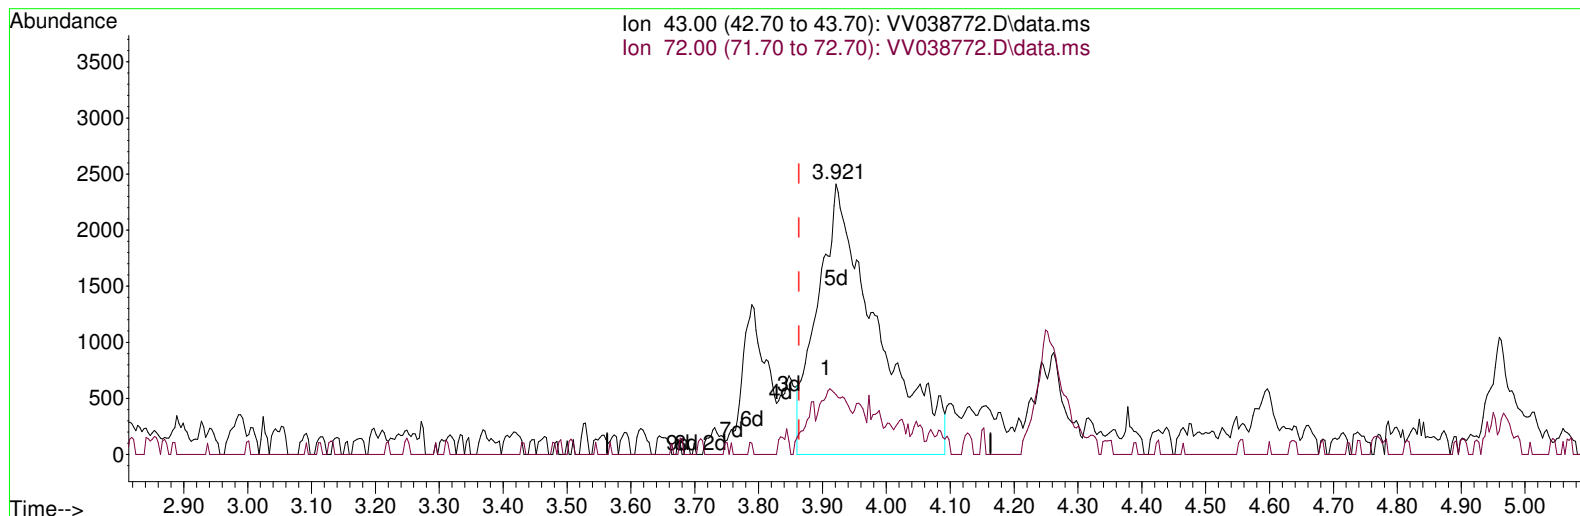

(22) 2-Butanone (T)

3.921min (+ 0.058) 4.23 ug/L m

response 15499

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	25.00	3.13#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

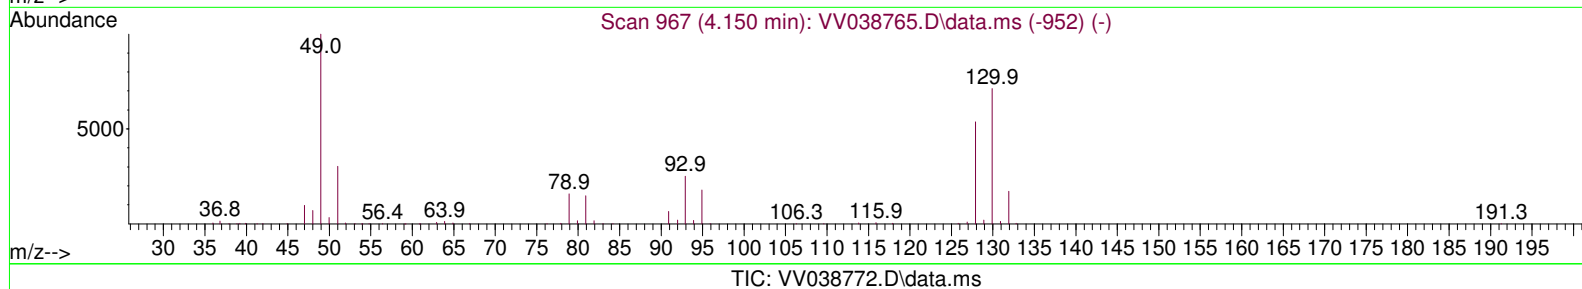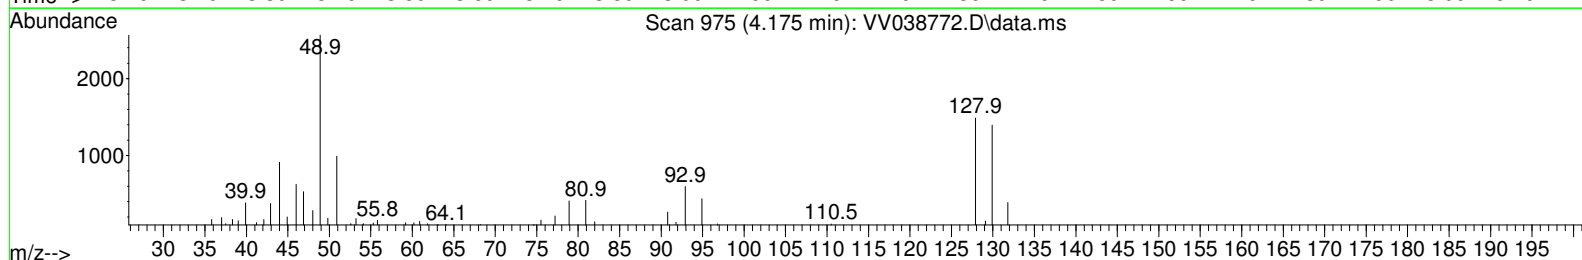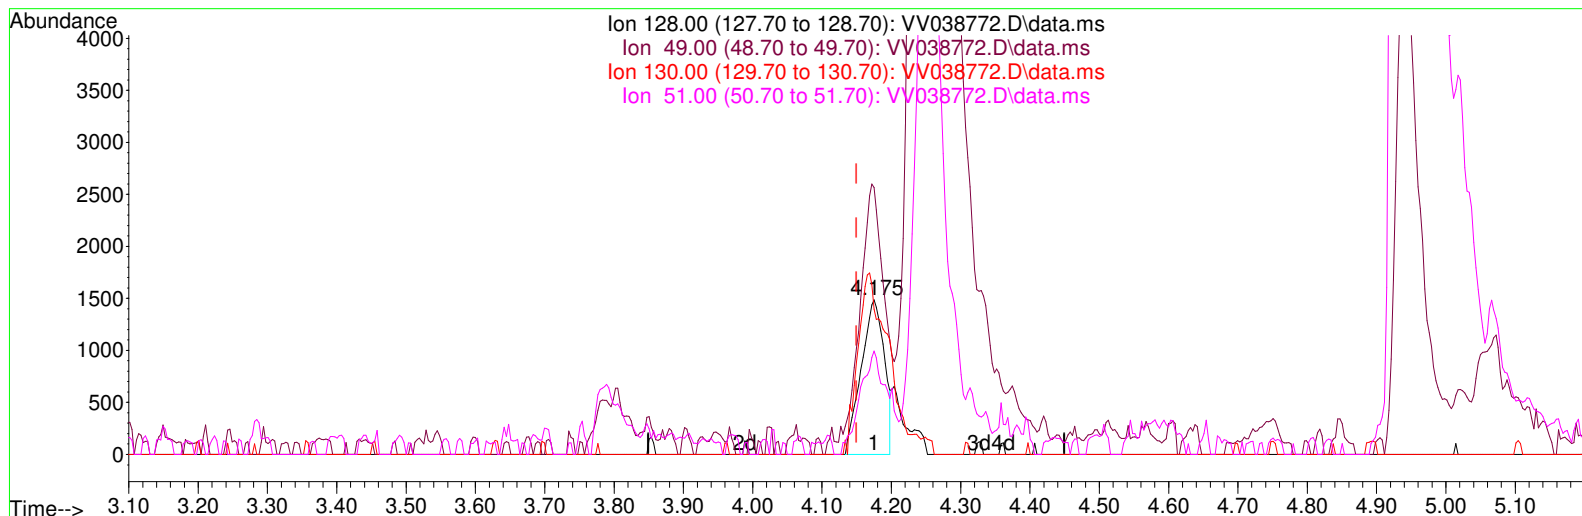

(23) Bromochloromethane (T)

4.175min (+ 0.026) 1.29 ug/L

response 3434

Ion	Exp%	Act%
128.00	100.00	100.00
49.00	152.50	172.79
130.00	133.20	94.07
51.00	50.30	66.87#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

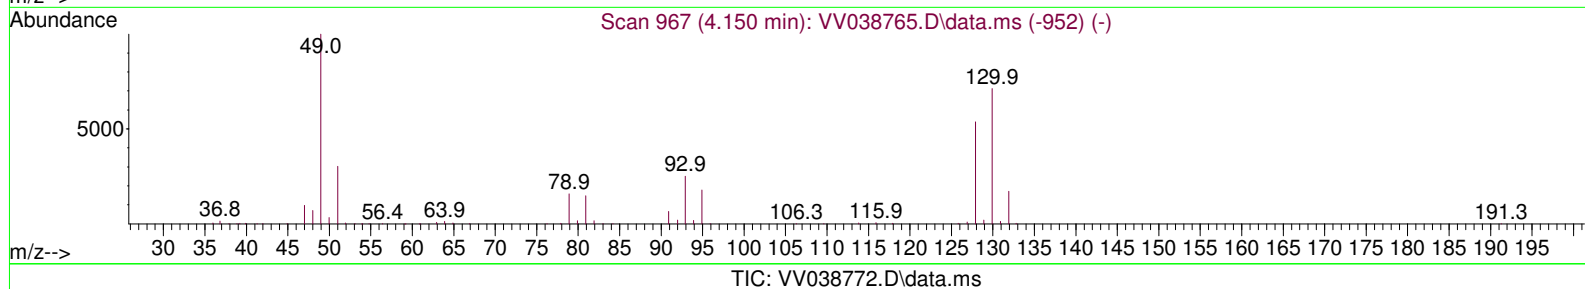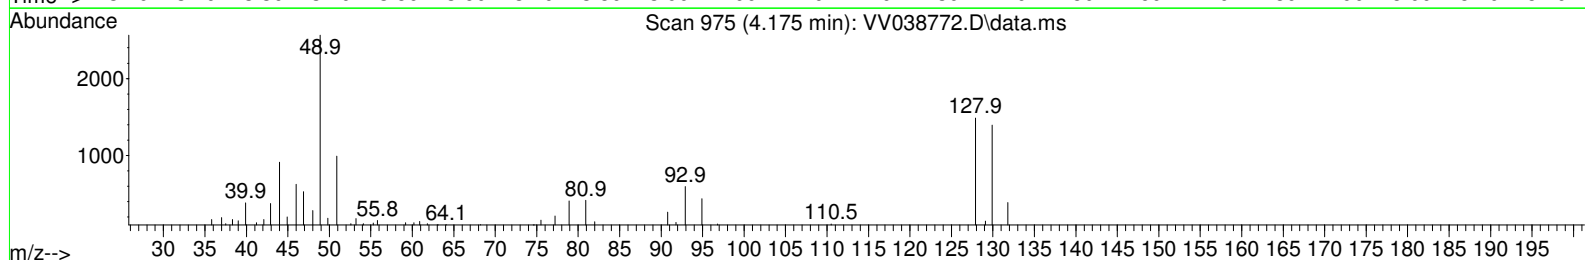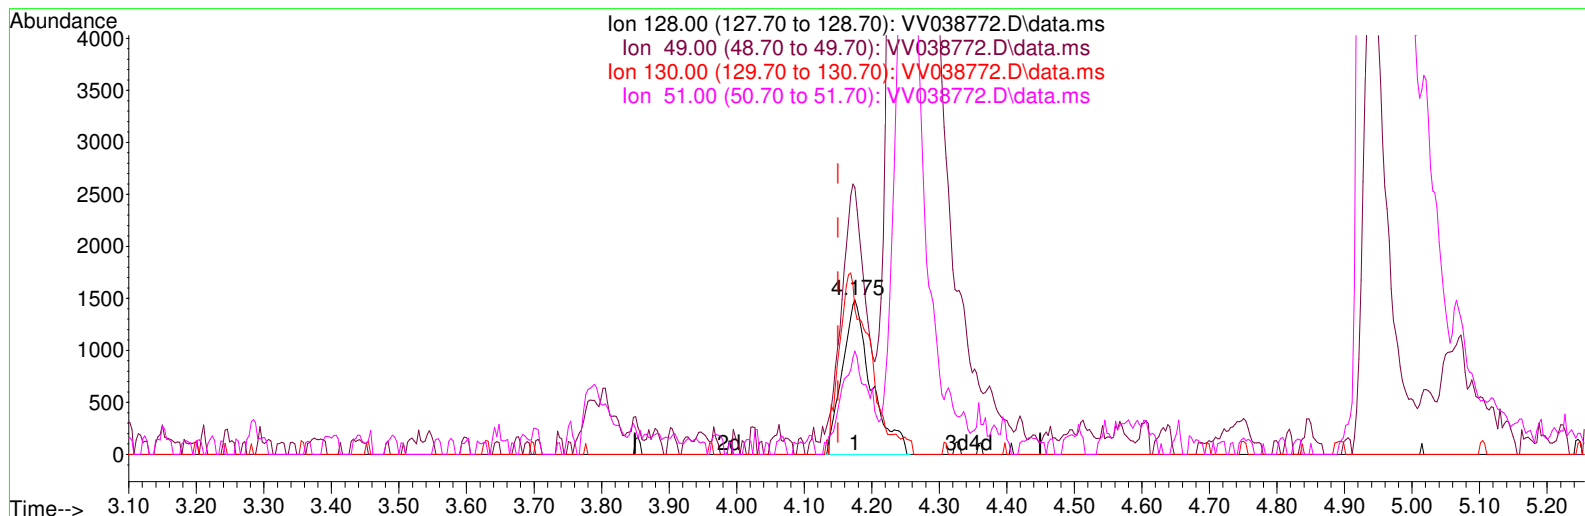

(23) Bromochloromethane (T)

4.175min (+ 0.026) 1.66 ug/L m

response 4419

Ion	Exp%	Act%
-----	------	------

128.00	100.00	100.00
--------	--------	--------

49.00	152.50	172.79
-------	--------	--------

130.00	133.20	94.07
--------	--------	-------

51.00	50.30	66.87#
-------	-------	--------




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

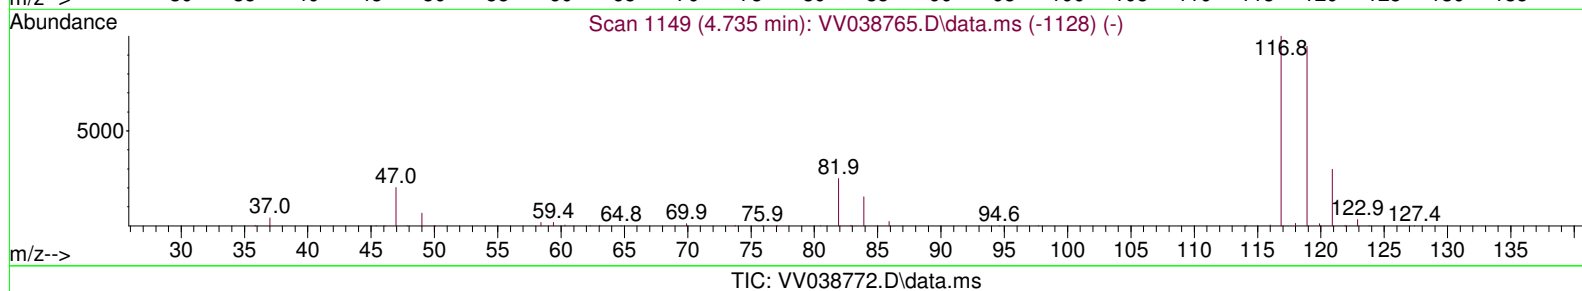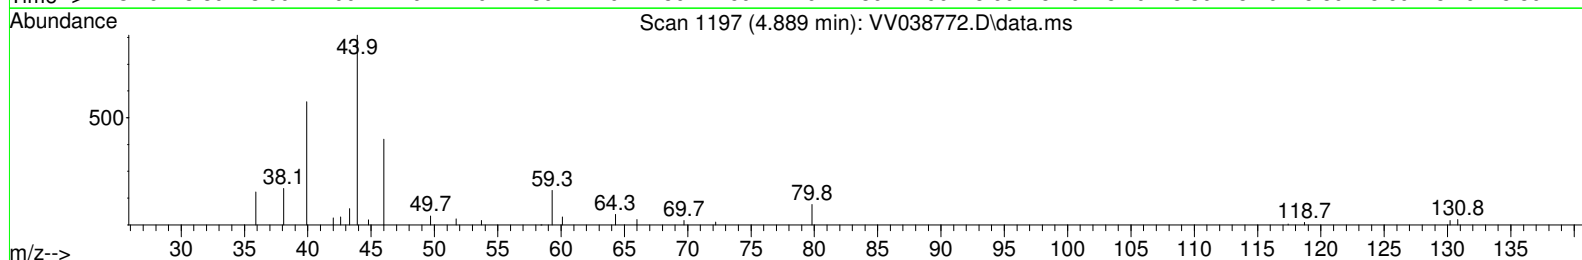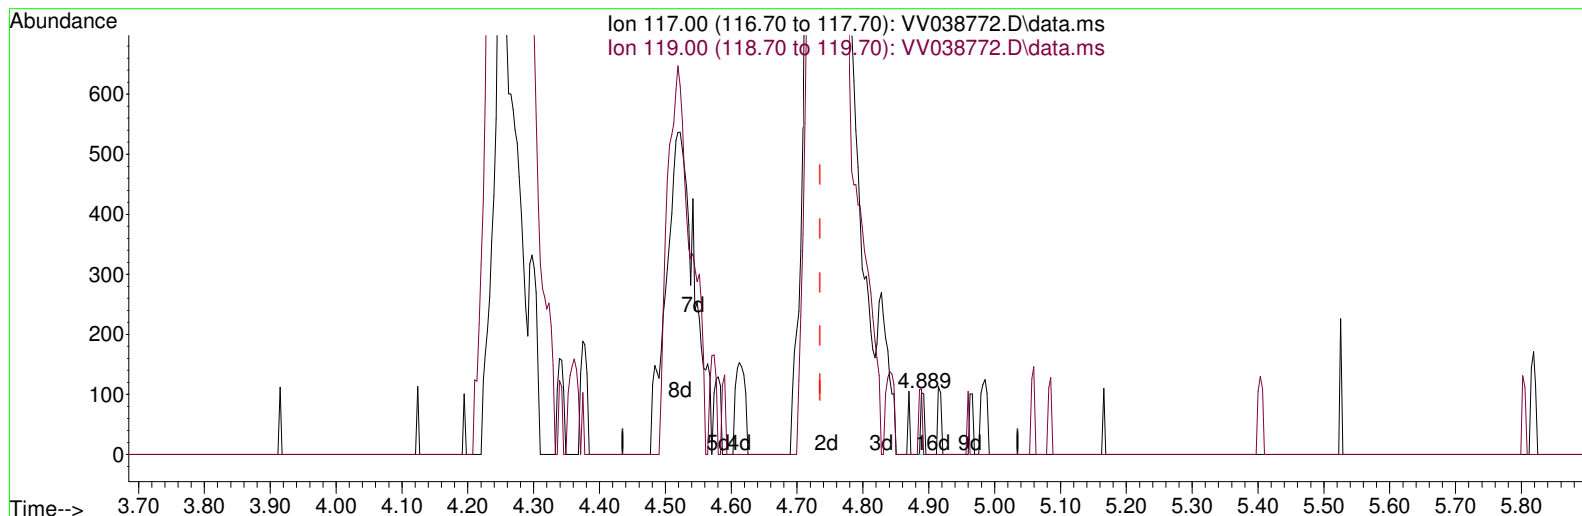

(31) Carbon tetrachloride (T)

4.889min (+ 0.154) 0.01 ug/L

response 39

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	97.10	107.69
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

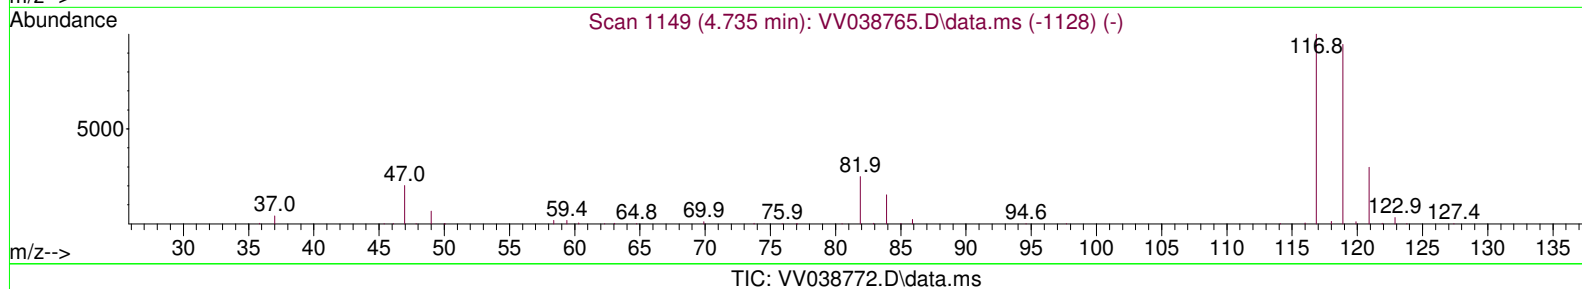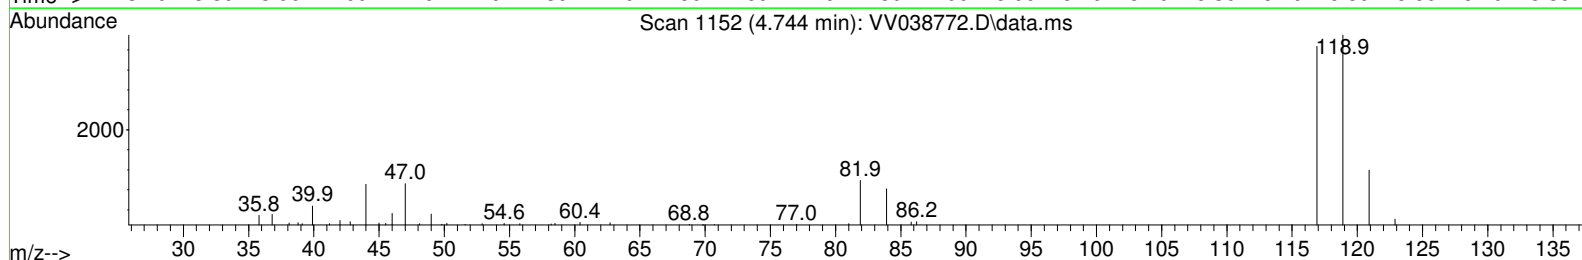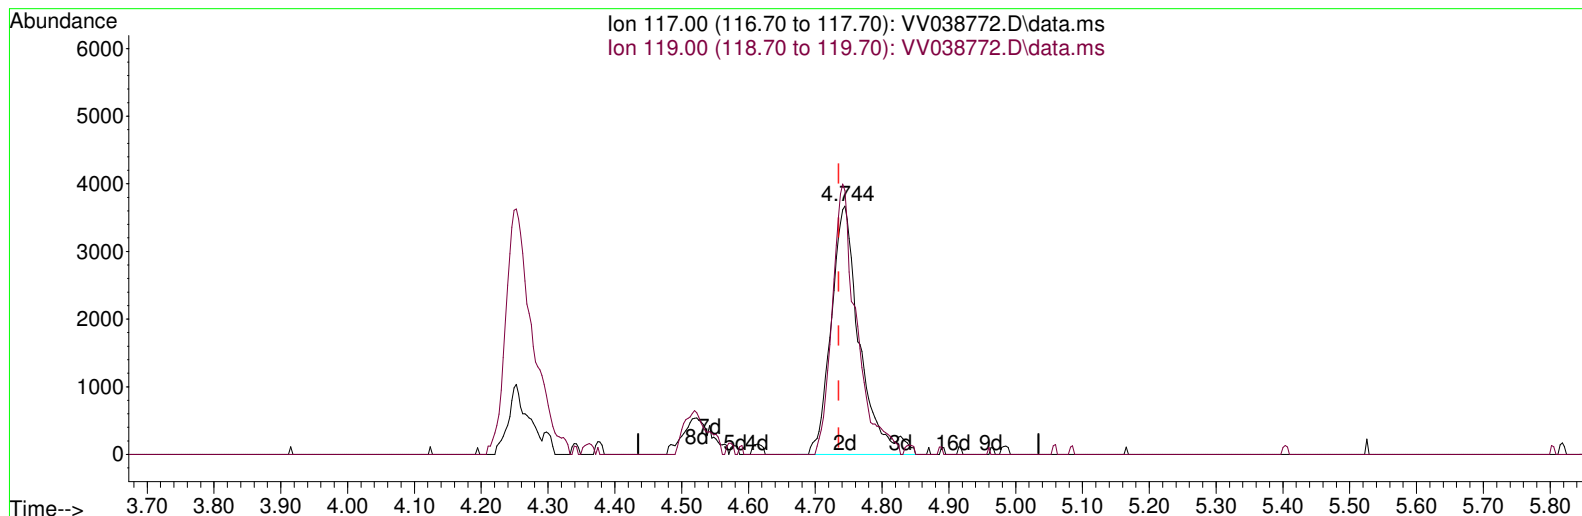

TIC: VV038772.D\data.ms

(31) Carbon tetrachloride (T)

4.744min (+ 0.009) 1.53 ug/L m

response 10811

Ion	Exp%	Act%
117.00	100.00	100.00
119.00	97.10	0.39#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

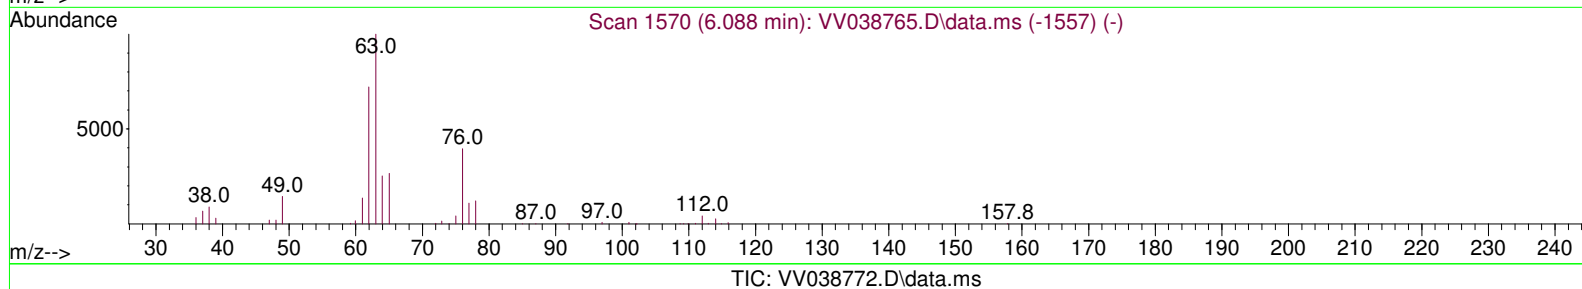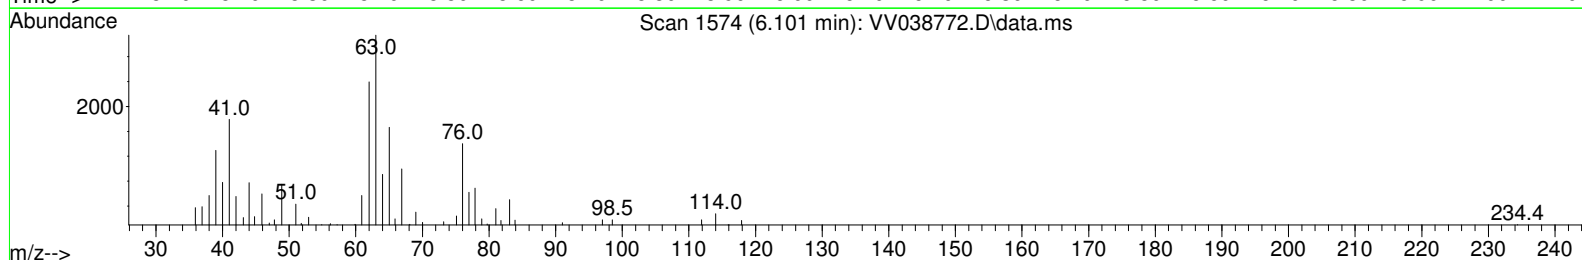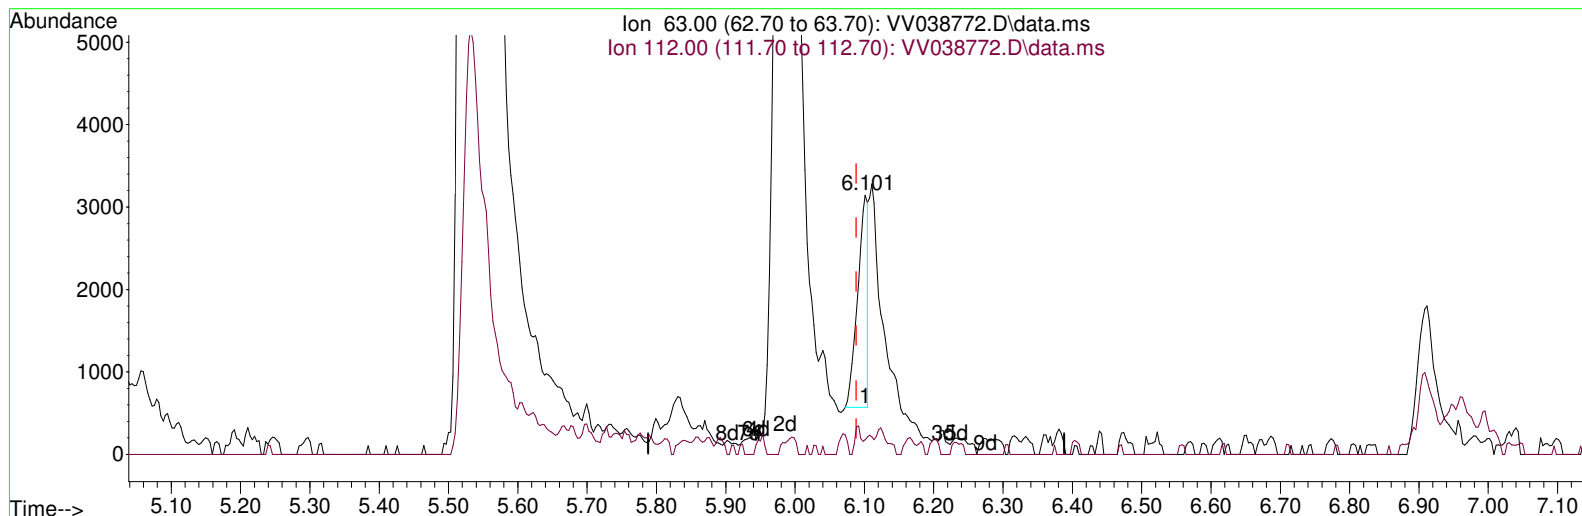

(37) 1,2-Dichloropropane (T)

6.101min (+ 0.013) 0.47 ug/L

response 2664

Ion	Exp%	Act%
63.00	100.00	100.00
112.00	4.70	6.12#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038772.D
Acq On : 09 Jun 2025 17:50
Operator : SY/MD
Sample : Q2117-05
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-MED-SOIL-QT2-2025-03

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 06/11/2025
Supervised By :Mahesh Dadoda 06/11/2025

Quant Time: Jun 10 09:11:48 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 10 09:06:39 2025
Response via : Initial Calibration

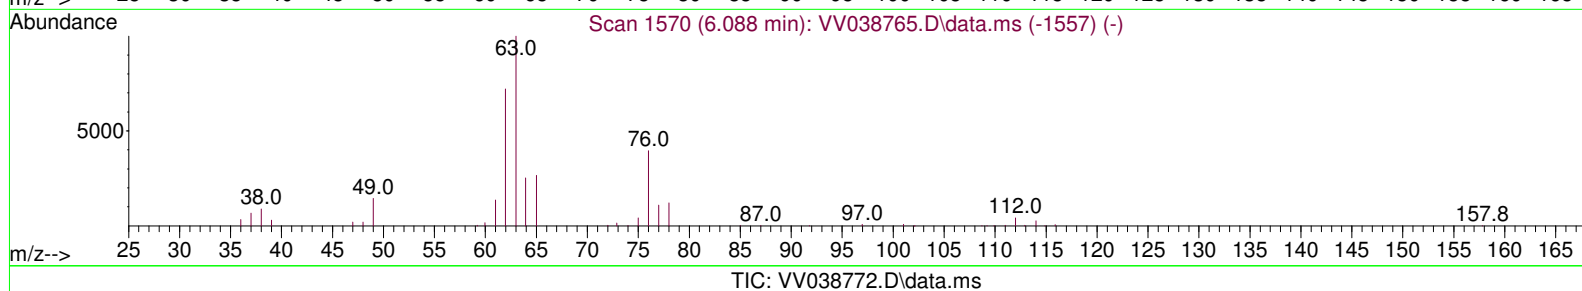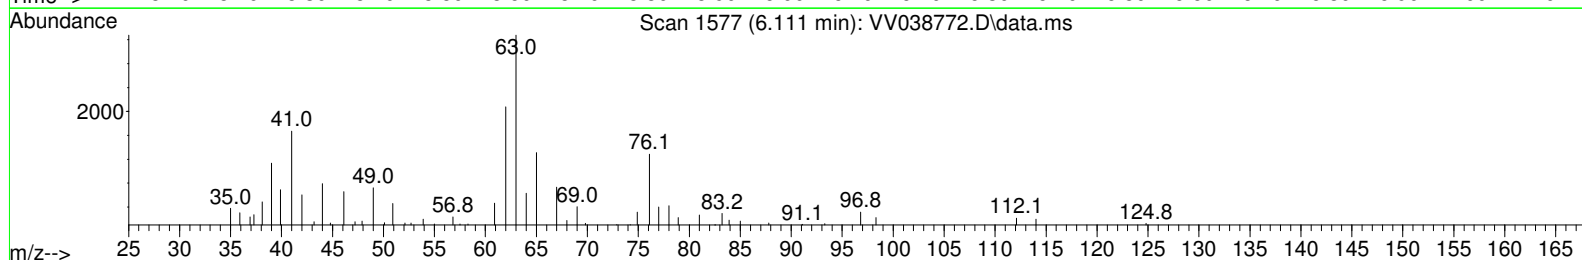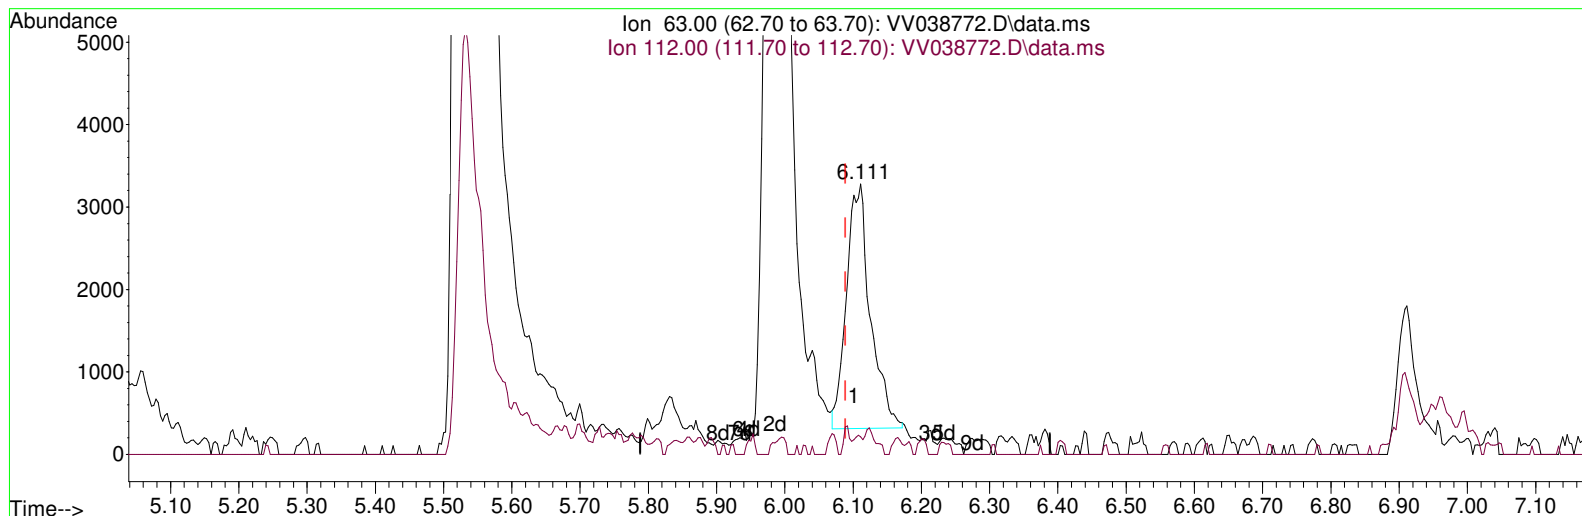

(37) 1,2-Dichloropropane (T)

6.111min (+ 0.022) 1.28 ug/L m

response 7210

Ion	Exp%	Act%
63.00	100.00	100.00
112.00	4.70	2.26#
0.00	0.00	0.00
0.00	0.00	0.00