
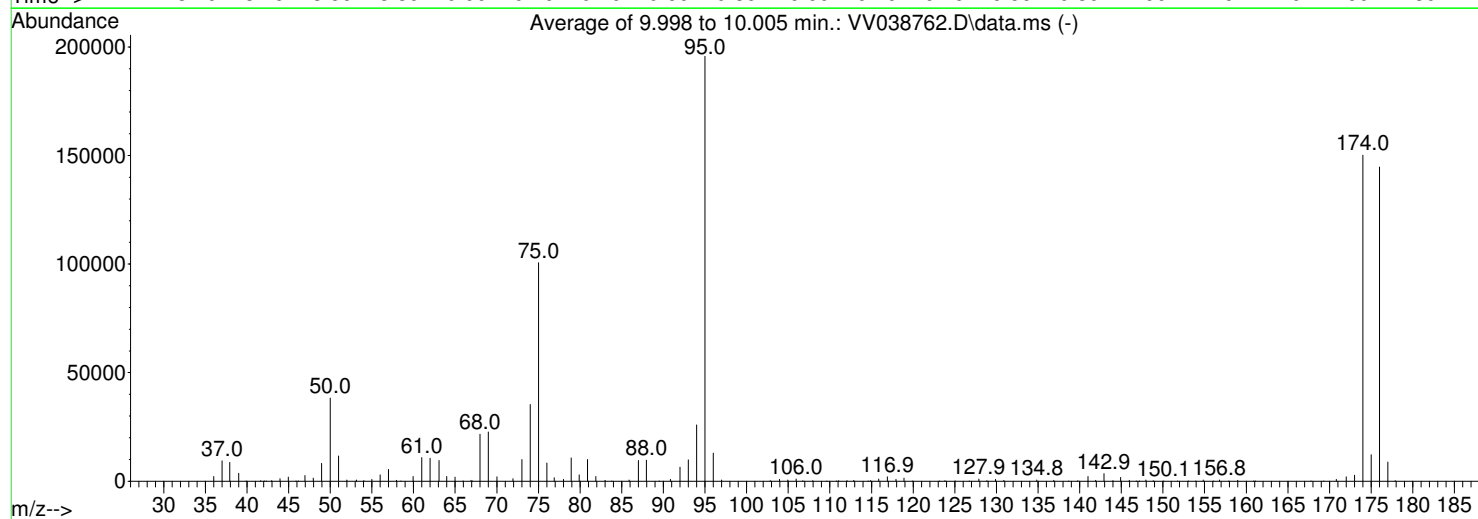


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060925\
Data File : VV038762.D
Acq On : 09 Jun 2025 11:04
Operator : SY/MD
Sample : BFB202
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB202

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060925WMA.M
Title : VOC Analysis
Last Update : Tue Jun 10 09:06:39 2025

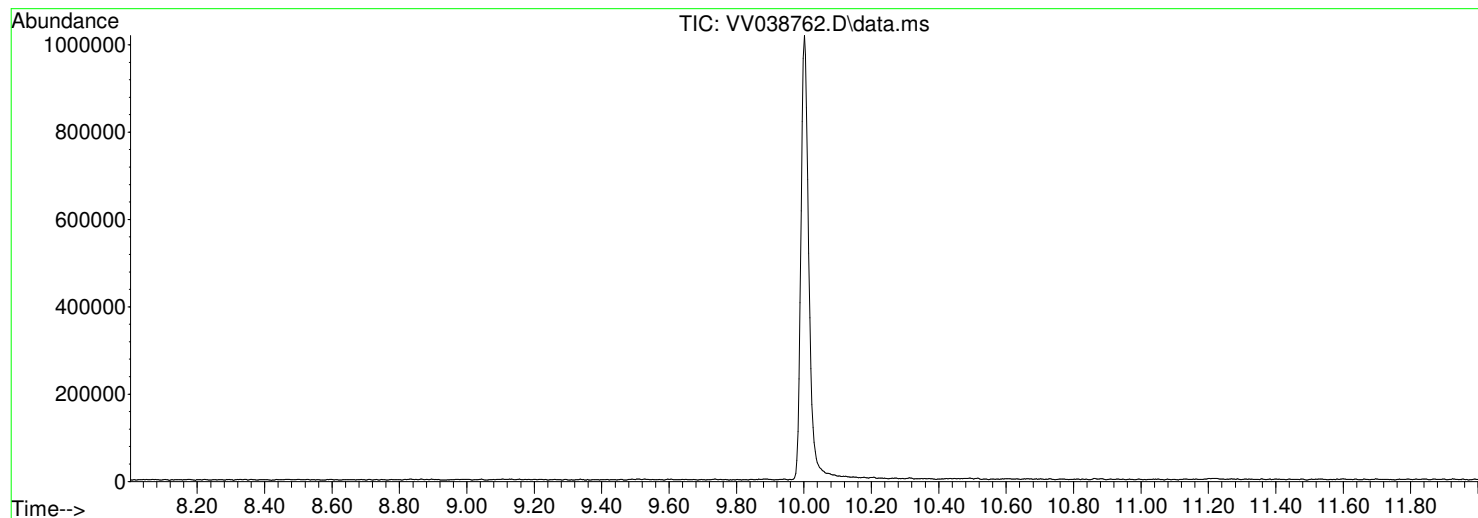

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	38285	PASS
75	95	30	80	51.4	100670	PASS
95	95	100	100	100.0	195733	PASS
96	95	5	9	6.6	12951	PASS
173	174	0.00	2	1.8	2729	PASS
174	95	50	120	76.8	150229	PASS
175	174	5	9	8.1	12195	PASS
176	174	95	105	96.3	144640	PASS
177	176	5	10	6.1	8757	PASS

m/z	Abundance
36.10	127.0
37.20	114.0
37.80	131.0
39.20	184.0
39.80	547.0
40.80	162.0
41.20	114.0
43.90	1083.0
44.90	104.0
45.60	107.0
46.30	134.0
46.90	121.0
48.80	115.0
50.20	112.0
52.00	117.0
54.30	105.0
63.40	116.0
66.10	109.0
71.00	113.0
75.20	117.0
77.20	201.0
79.50	157.0
115.10	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	2019.0
37.00	9389.0
38.00	8336.0
39.00	3791.0
40.00	599.0
41.60	148.0
42.10	152.0
43.00	174.0
44.00	2273.0
45.00	1885.0
46.20	437.0
47.00	2773.0
48.00	1363.0
49.00	8219.0
50.00	38528.0
51.00	11527.0
52.00	567.0
53.10	515.0
54.10	271.0
55.00	759.0
56.00	2855.0
57.00	5307.0
58.00	240.0
59.90	2310.0
61.00	10765.0
62.00	10421.0
63.10	9754.0
64.00	2245.0
65.00	1706.0
65.90	227.0
66.90	481.0
68.00	21208.0
69.00	22488.0
70.00	2016.0
70.90	155.0
72.00	1131.0
73.00	10070.0
74.00	34312.0
75.00	99976.0
76.00	8366.0
76.90	1353.0
78.00	941.0
78.90	10939.0
79.90	2906.0
80.90	10081.0
81.90	2187.0
83.00	322.0
85.90	559.0
87.00	9696.0
87.90	9072.0
90.80	937.0
92.00	6177.0
93.00	9593.0
94.00	25616.0
95.00	193216.0
96.00	13007.0
97.00	454.0
102.90	218.0
103.90	848.0
104.90	453.0
106.00	946.0
106.80	247.0
107.90	175.0
109.60	134.0
110.80	231.0
112.10	230.0
112.80	276.0
114.60	201.0
115.80	932.0
116.90	1834.0
118.00	805.0
118.90	1287.0
123.10	129.0
123.80	194.0
125.00	135.0
127.90	867.0
128.90	272.0
129.90	828.0
130.90	242.0
134.80	454.0
136.90	307.0
139.70	184.0
141.00	2145.0
141.90	338.0
142.90	3389.0
144.00	287.0
144.90	1539.0
146.00	288.0
147.20	199.0
148.00	506.0
148.90	236.0
150.10	130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

151.80	127.0
153.00	125.0
154.10	167.0
154.80	419.0
156.10	136.0
156.80	395.0
159.00	343.0
160.80	195.0
167.80	125.0
169.30	157.0
170.80	878.0
172.00	1818.0
173.00	2677.0
174.00	144128.0
175.00	12134.0
176.00	138688.0
177.00	8208.0
177.90	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	2237.0
37.00	9825.0
38.00	9073.0
39.00	3826.0
40.00	581.0
41.70	228.0
43.00	167.0
44.00	2194.0
45.00	2035.0
46.20	421.0
47.00	2773.0
48.00	1408.0
49.00	8610.0
50.00	39536.0
51.00	11836.0
52.00	750.0
53.10	513.0
54.00	296.0
55.00	845.0
56.00	2955.0
57.00	5586.0
57.90	315.0
60.00	2240.0
61.00	11099.0
62.00	11037.0
63.10	9787.0
64.00	2248.0
65.00	1946.0
65.90	272.0
66.90	471.0
68.00	22336.0
69.00	23400.0
70.00	2164.0
70.90	126.0
72.00	1028.0
73.00	10309.0
74.00	36488.0
75.00	103680.0
76.00	8643.0
76.90	1610.0
78.00	894.0
78.90	11002.0
79.90	3012.0
80.90	10064.0
81.90	2200.0
83.00	393.0
85.90	505.0
87.00	9800.0
87.90	9932.0
90.80	893.0
92.00	6527.0
93.00	10156.0
94.00	26952.0
95.00	202624.0
96.00	13513.0
97.00	513.0
102.80	238.0
103.90	881.0
104.90	475.0
105.90	1029.0
106.80	230.0
107.90	193.0
109.60	145.0
111.00	265.0
112.00	257.0
112.80	302.0
114.80	254.0
115.90	1006.0
116.90	1976.0
117.90	905.0
118.90	1460.0
119.90	101.0
123.20	160.0
123.80	280.0
125.00	145.0
126.70	132.0
127.90	981.0
128.90	237.0
129.90	809.0
130.90	322.0
134.80	445.0
136.90	326.0
139.80	173.0
141.00	2186.0
141.90	412.0
142.90	3566.0
144.00	240.0
144.90	1737.0
146.00	356.0
147.20	200.0
147.90	524.0
148.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

150.10	138.0
151.70	123.0
153.10	115.0
153.90	119.0
154.90	450.0
156.10	157.0
156.80	515.0
157.90	116.0
159.00	359.0
160.90	148.0
169.30	166.0
170.80	787.0
172.00	1943.0
173.00	2878.0
174.00	154944.0
175.00	12680.0
176.00	149696.0
177.00	8873.0
177.90	244.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

m/z	Abundance
36.00	2349.0
37.00	9443.0
38.00	8821.0
39.00	3695.0
40.00	627.0
41.70	264.0
42.30	138.0
42.90	209.0
44.00	1953.0
45.00	2060.0
45.90	404.0
47.00	2393.0
47.90	1404.0
49.00	8258.0
50.00	37128.0
51.00	11394.0
52.00	777.0
53.20	414.0
54.00	293.0
55.00	759.0
56.00	2795.0
57.00	5287.0
57.90	478.0
58.50	103.0
60.00	2001.0
61.00	10443.0
62.00	10280.0
63.00	8974.0
64.00	1901.0
65.00	1855.0
66.00	276.0
67.10	472.0
68.00	21168.0
69.00	21840.0
70.00	1885.0
71.90	1018.0
73.00	9587.0
74.00	35208.0
75.00	98704.0
76.00	8195.0
76.90	1585.0
78.00	821.0
79.00	10131.0
79.90	2829.0
80.90	9529.0
81.90	2108.0
83.00	415.0
83.80	118.0
85.90	440.0
87.00	9005.0
88.00	9974.0
89.50	102.0
90.90	814.0
92.00	6366.0
93.00	9486.0
94.00	24936.0
95.00	191360.0
96.00	12333.0
97.00	620.0
102.80	247.0
104.00	821.0
105.00	466.0
105.90	946.0
106.70	180.0
108.00	284.0
109.70	135.0
111.10	263.0
112.00	212.0
112.90	354.0
114.90	309.0
115.90	907.0
116.90	1983.0
117.90	959.0
118.90	1531.0
123.20	129.0
123.80	331.0
125.10	130.0
126.80	169.0
127.90	1026.0
128.80	243.0
129.90	732.0
130.90	369.0
134.90	472.0
136.90	375.0
138.70	102.0
139.80	227.0
141.00	1980.0
141.90	460.0
142.90	3453.0
144.00	191.0
144.90	1782.0
145.90	395.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202

146.80	181.0
147.90	445.0
148.70	118.0
150.10	141.0
151.70	122.0
153.80	100.0
154.90	490.0
156.10	171.0
156.80	528.0
157.90	154.0
159.00	325.0
161.10	187.0
169.30	112.0
170.80	656.0
172.00	2065.0
173.00	2633.0
174.00	151616.0
175.00	11771.0
176.00	145536.0
177.00	9190.0
177.90	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB202