

Data File : VV011399.D
Acq On : 11 Jun 2019 17:59
Operator : SY/MD
Sample : K3226-17RE
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCP1

Quant Time: Jun 12 02:54:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 02:48:56 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	146361	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	138194	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	55066	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	35103	3.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	63.40%
7) Chloroethane-d5	1.55	69	32359	3.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.20%
11) 1,1-Dichloroethene-d2	2.12	63	59385	2.68	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	53.60%#
20) 2-Butanone-d5	3.94	46	140676	56.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.68%
24) Chloroform-d	4.40	84	80712	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.80%
26) 1,2-Dichloroethane-d4	5.08	65	46963	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
32) Benzene-d6	5.09	84	151543	3.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.40%
36) 1,2-Dichloropropane-d6	6.12	67	50059	3.93	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.60%
41) Toluene-d8	7.36	98	129731	3.42	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	68.40%#
43) trans-1,3-Dichloropropene-	7.66	79	13620	2.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	56.20%
46) 2-Hexanone-d5	8.13	63	102436	49.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.90%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	40373	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	45246	4.16	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	83.20%

Target Compounds

						Qvalue
3) Chloromethane	1.25	50	1740	0.125	ug/L	93
5) Vinyl chloride	1.32	62	145318	10.792	ug/L	98
8) Chloroethane	1.32	64	62365	7.248	ug/L #	51
12) 1,1-Dichloroethene	2.13	96	6170	0.669	ug/L #	1
13) Acetone	2.19	43	3422	2.044	ug/L	95
14) Carbon disulfide	2.31	76	2601	0.093	ug/L #	43
17) Methyl tert-butyl Ether	2.81	73	5796	0.235	ug/L #	89
18) trans-1,2-Dichloroethene	2.78	96	503694	48.786	ug/L	94
22) cis-1,2-Dichloroethene	3.95	96	2703432	236.437	ug/L	98
34) Trichloroethene	5.96	95	3845340	338.496	ug/L	98
35) Methylcyclohexane	6.12	83	13186	0.702	ug/L #	16
37) 1,2-Dichloropropane	6.12	63	6446	0.589	ug/L #	88
39) cis-1,3-Dichloropropene	7.03	75	1418	0.089	ug/L #	15
42) Toluene	7.43	91	11958	0.255	ug/L	97
48) 2-Hexanone	8.13	43	15136	3.114	ug/L #	69
53) m,p-xylene	9.18	106	2500	0.130	ug/L	75

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV061019\
Quantitation Report (Not Reviewed)

Data File : VV011399.D
Acq On : 11 Jun 2019 17:59
Operator : SY/MD
Sample : K3226-17RE
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCP1

Quant Time: Jun 12 02:54:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 02:48:56 2019
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV011399.D
Acq On : 11 Jun 2019 17:59
Operator : SY/MD
Sample : K3226-17RE
Misc : 25ML/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCP1

Quant Time: Jun 12 02:54:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 02:48:56 2019
Response via : Initial Calibration

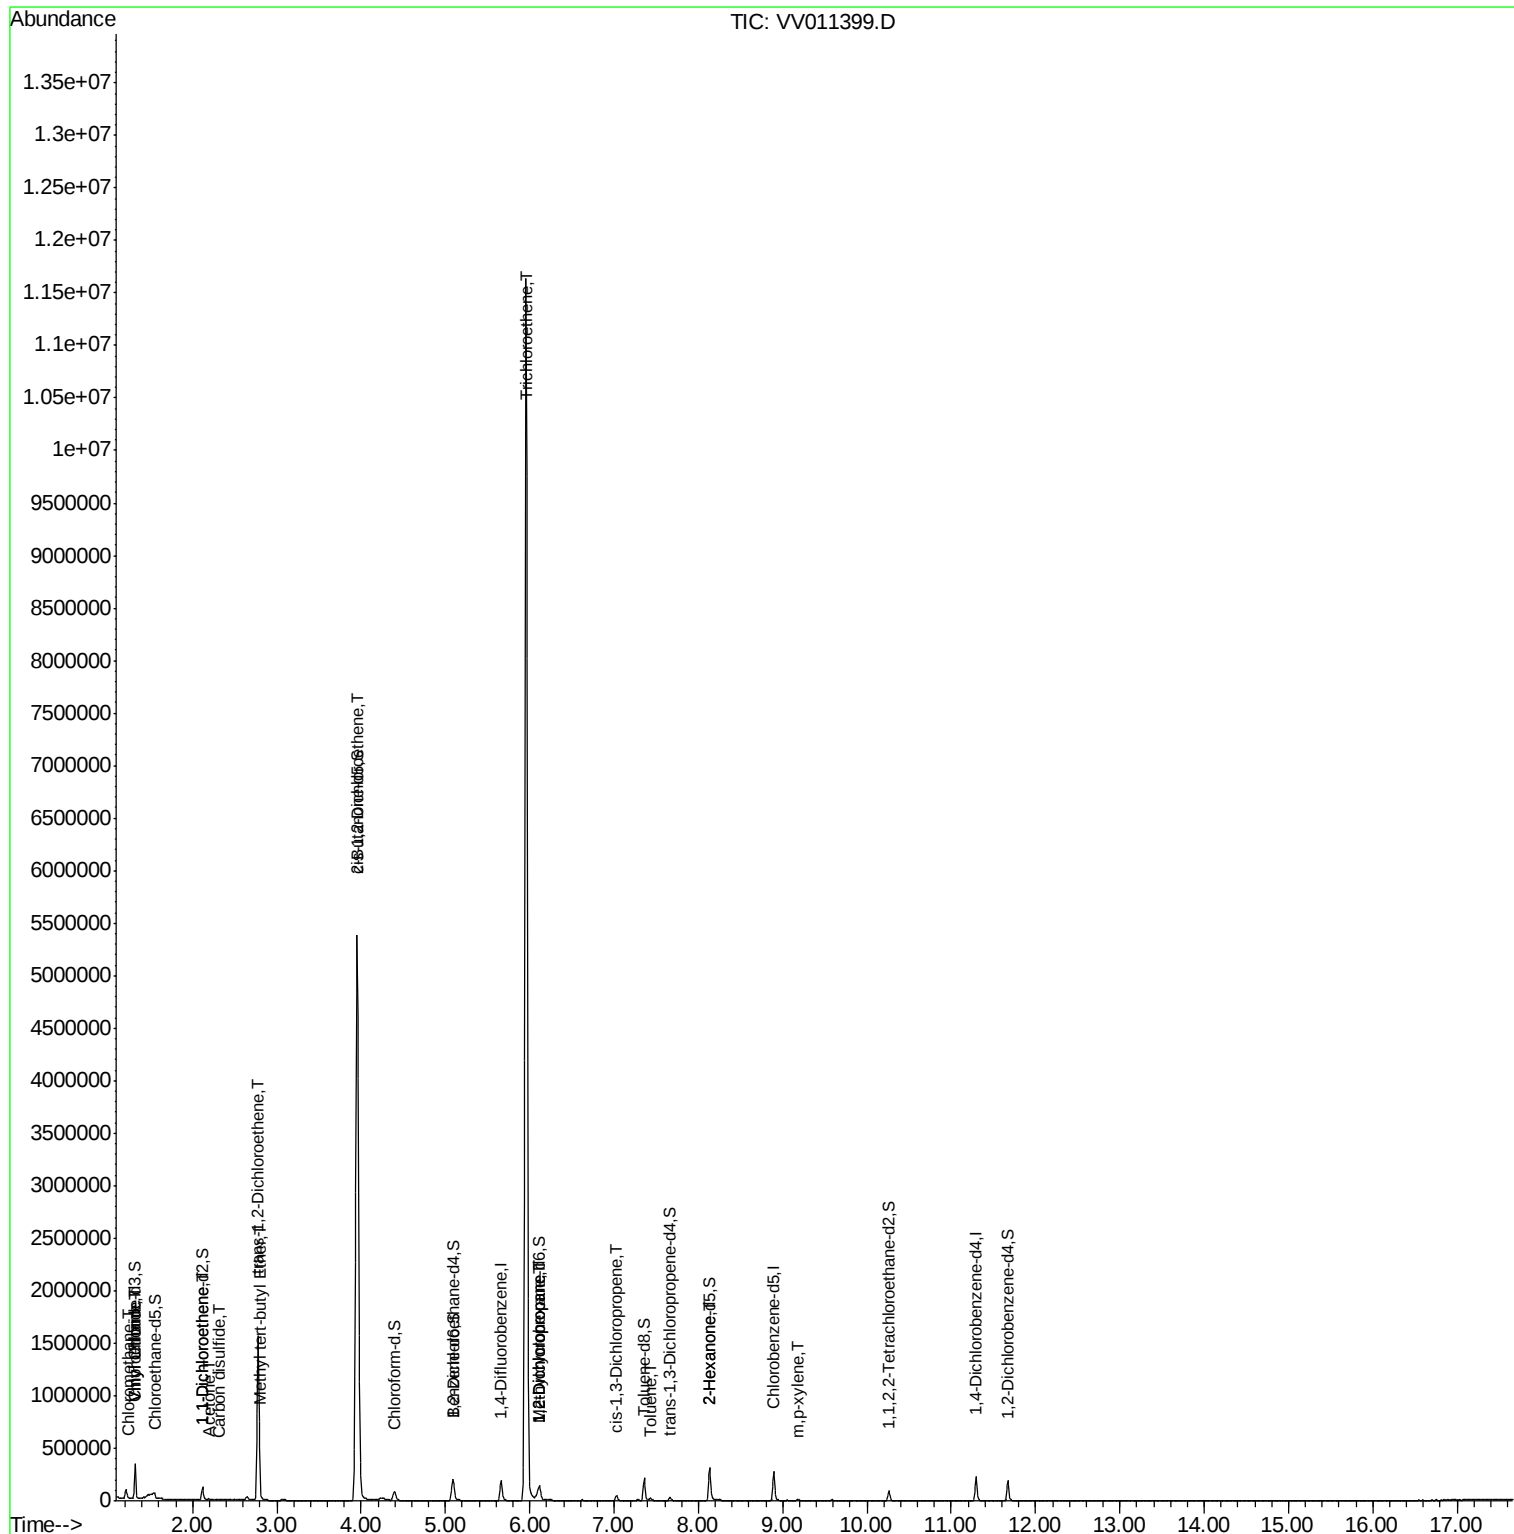

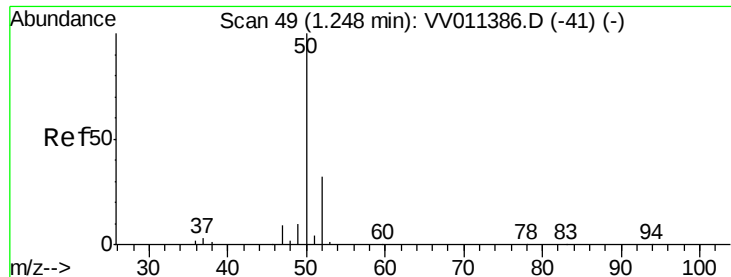

#3

Chloromethane

Concen: 0.125 ug/L

RT: 1.25 min Scan# 50

Delta R.T. 0.00 min

Lab File: VV011399.D

Acq: 11 Jun 2019 17:59

Instrument :

MSVOA_V

ClientSampleId :





BFCP1

Tgt Ion: 50 Resp: 1740

Ion Ratio Lower Upper

50 100

52 27.9 22.3 41.5

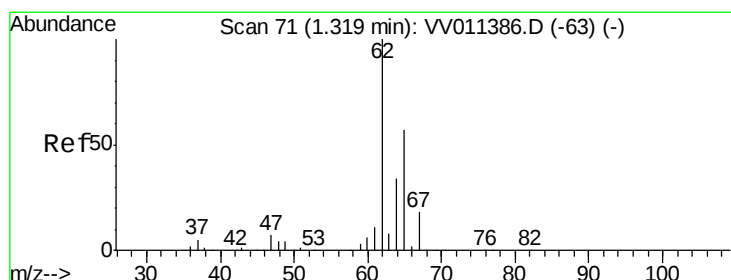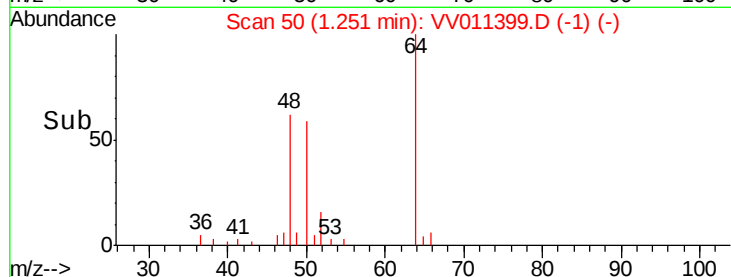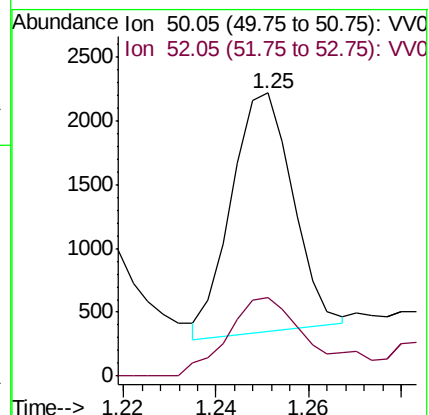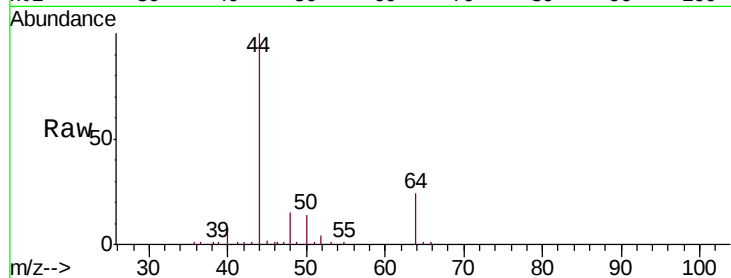

#5

Vinyl chloride

Concen: 10.792 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.00 min

Lab File: VV011399.D




Acq: 11 Jun 2019 17:59


Tgt Ion: 62 Resp: 145318

Ion Ratio Lower Upper

62 100

64 38.2 25.9 48.1

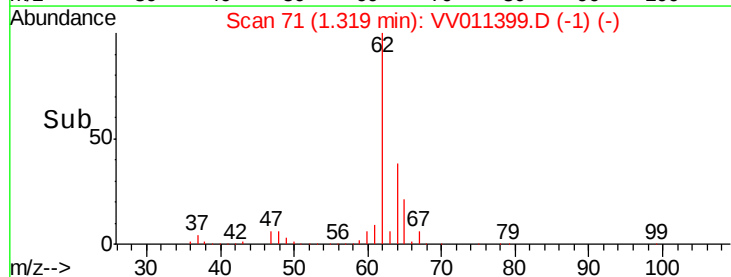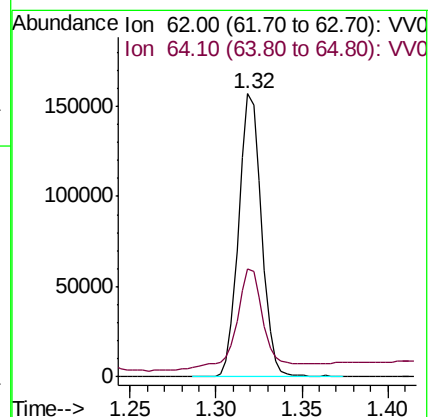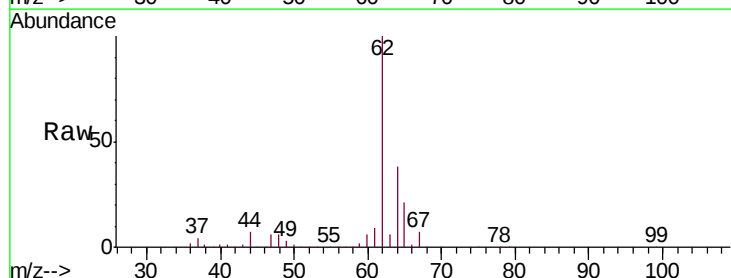

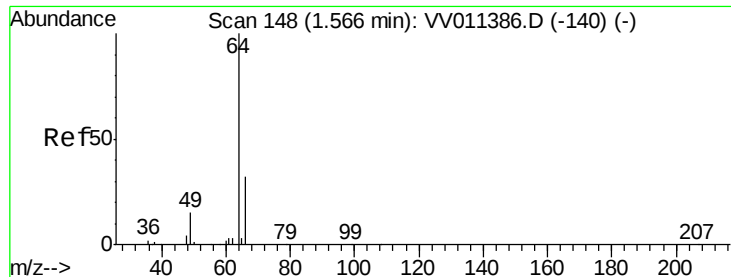

#8

Chloroethane

Concen: 7.248 ug/L

RT: 1.32 min Scan# 71

Delta R.T. -0.25 min

Lab File: VV011399.D

Acq: 11 Jun 2019 17:59

Instrument :

MSVOA_V

ClientSampled :





BFCP1

Tgt Ion: 64 Resp: 62365

Ion Ratio Lower Upper

64 100

66 2.2 19.4 36.0#

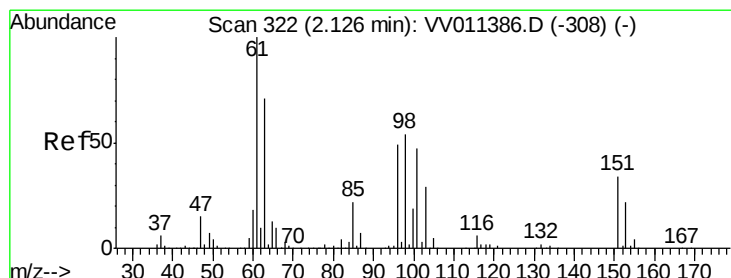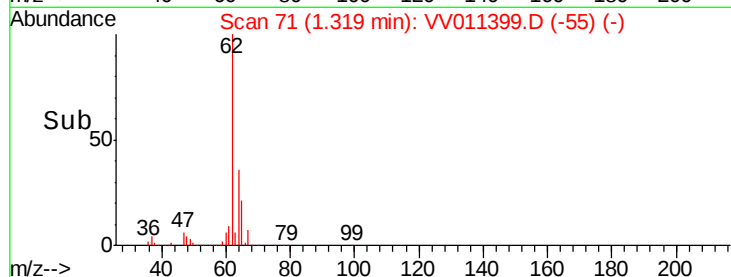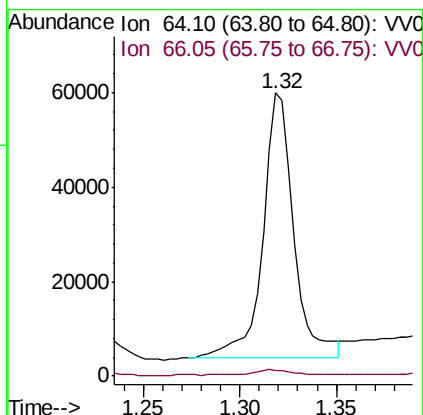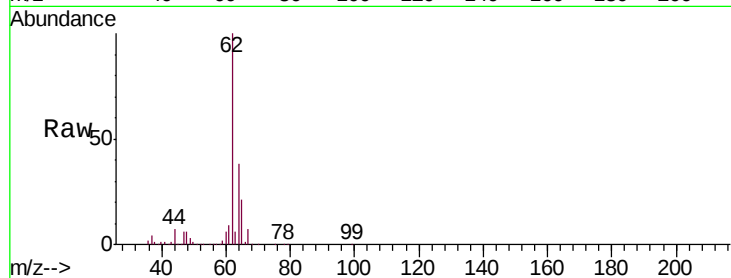

#12

1,1-Dichloroethene

Concen: 0.669 ug/L

RT: 2.13 min Scan# 322

Delta R.T. -0.00 min

Lab File: VV011399.D

Acq: 11 Jun 2019 17:59




Tgt Ion: 96 Resp: 6170


Ion Ratio Lower Upper

96 100

61 263.5 139.8 259.6#

63 622.4 94.3 175.1#

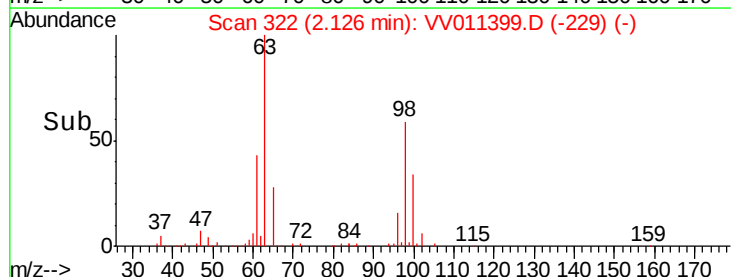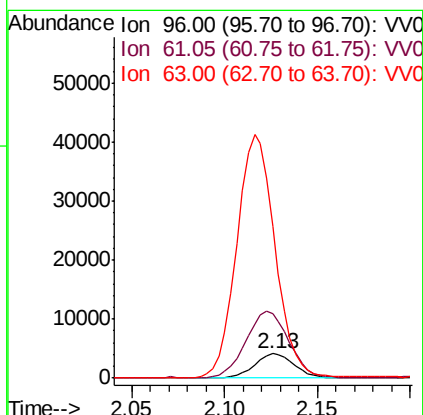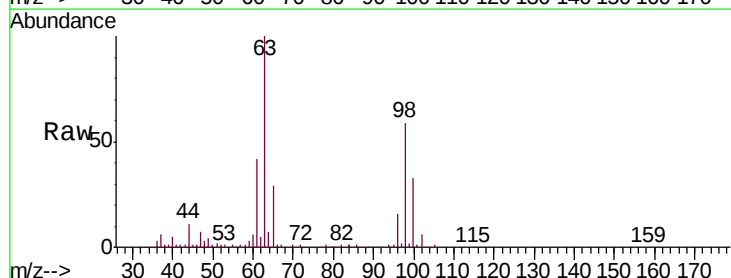



#13

Acetone

Concen: 2.044 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011399.D

Acq: 11 Jun 2019 17:59

Instrument :

MSVOA_V

ClientSampleId :


BFCP1

Tgt Ion: 43 Resp: 3422

Ion Ratio Lower Upper

43 100

58 30.1 0.0 55.2

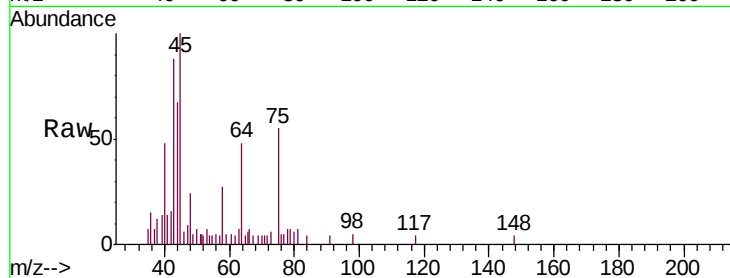

Abundance Ion 43.05 (42.75 to 43.75): VV0

Ion 58.05 (57.75 to 58.75): VV0

2500

2000

1500

1000

500



0

2.15

2.20

2.25

Time-->

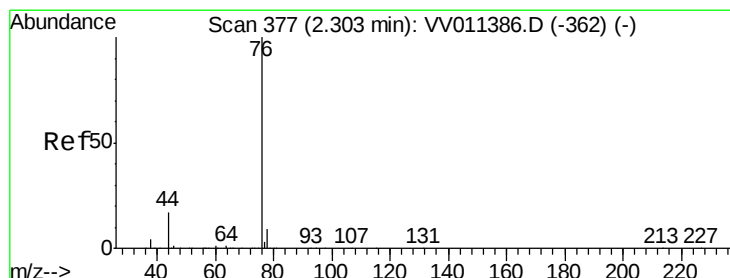

#14

Carbon disulfide

Concen: 0.093 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.01 min

Lab File: VV011399.D


Acq: 11 Jun 2019 17:59

Tgt Ion: 76 Resp: 2601

Ion Ratio Lower Upper

76 100

78 29.8 7.3 10.9#

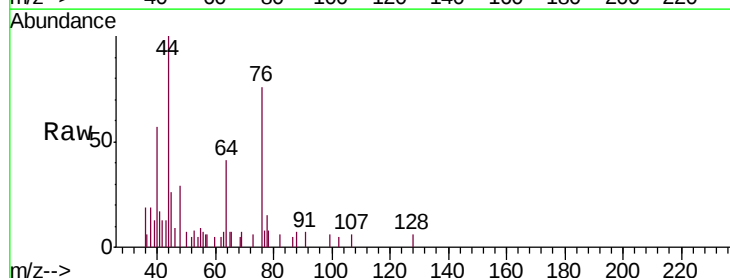

Abundance Ion 76.05 (75.75 to 76.75): VV0

Ion 78.00 (77.70 to 78.70): VV0

1500

1000

500


0


2.25

2.30

2.35

Time-->









#17
Methyl tert-butyl Ether
Concen: 0.235 ug/L
RT: 2.81 min Scan# 534
Delta R.T. -0.00 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59




Instrument :
MSVOA_V
ClientSampleId :
BFCP1


Tgt Ion: 73 Resp: 5796
Ion Ratio Lower Upper
73 100
43 20.8 18.7 28.1
57 31.0 18.1 27.1#

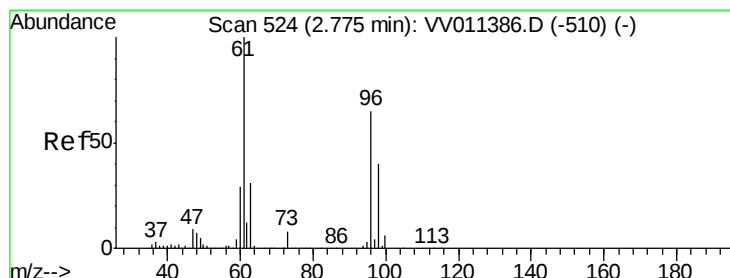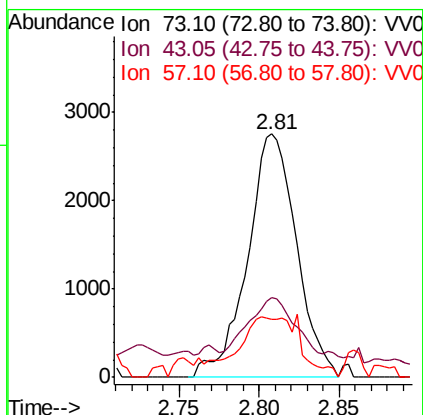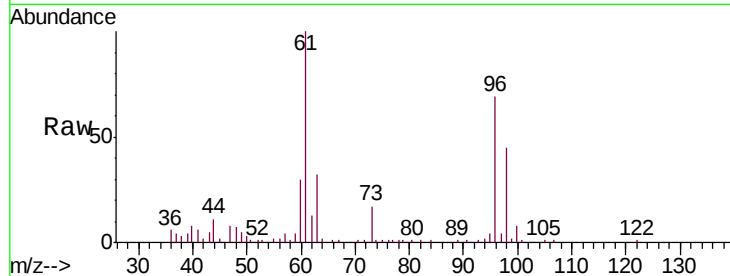

#18
trans-1,2-Dichloroethene
Concen: 48.786 ug/L
RT: 2.78 min Scan# 525
Delta R.T. 0.00 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59

Tgt Ion: 96 Resp: 503694
Ion Ratio Lower Upper
96 100
61 158.0 104.0 193.2
98 63.8 45.7 84.9

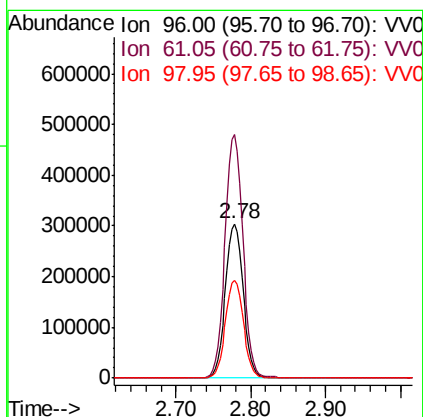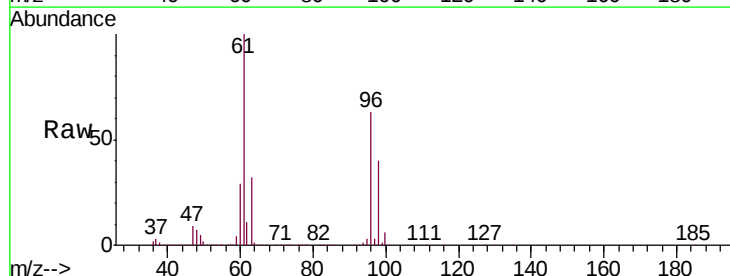




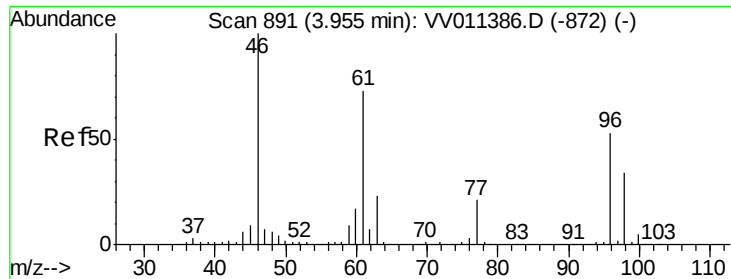


#22

cis-1,2-Dichloroethene
Concen: 236.437 ug/L
RT: 3.95 min Scan# 890
Delta R.T. -0.00 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59

Instrument :
MSVOA_V
ClientSampleId :
BFCP1




Tgt Ion: 96 Resp: 2703432
Ion Ratio Lower Upper
96 100
61 141.8 100.8 187.2
68 0.0 0.0 0.0

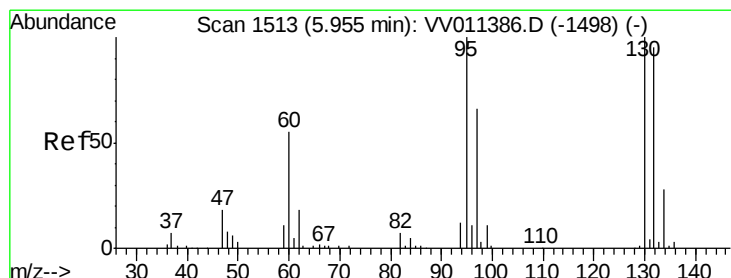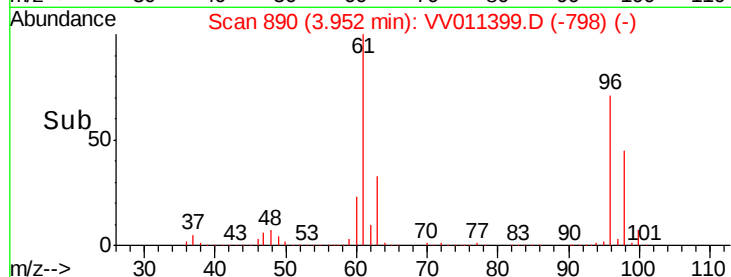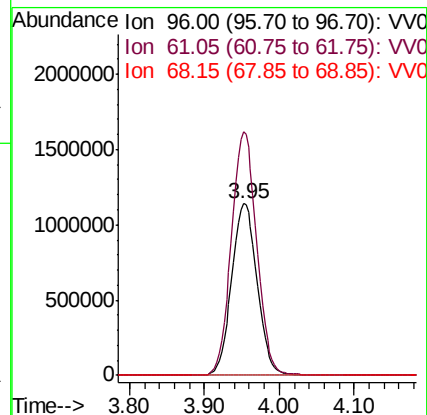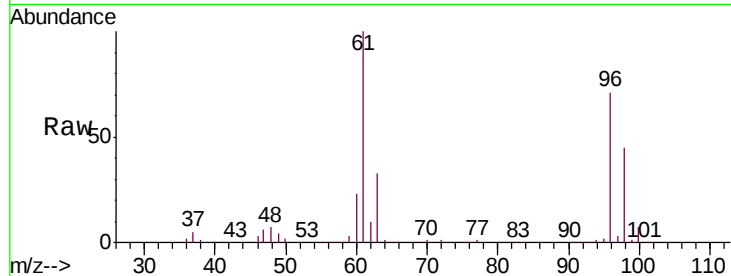


#34

Trichloroethene
Concen: 338.496 ug/L
RT: 5.96 min Scan# 1514
Delta R.T. 0.00 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59

Tgt Ion: 95 Resp: 3845340
Ion Ratio Lower Upper
95 100
97 65.3 45.8 85.2
132 91.3 66.4 123.2
130 95.0 68.3 126.8


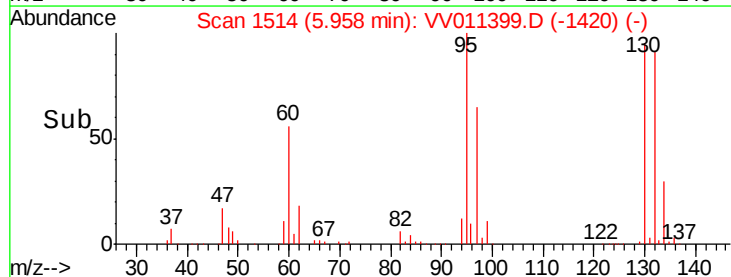
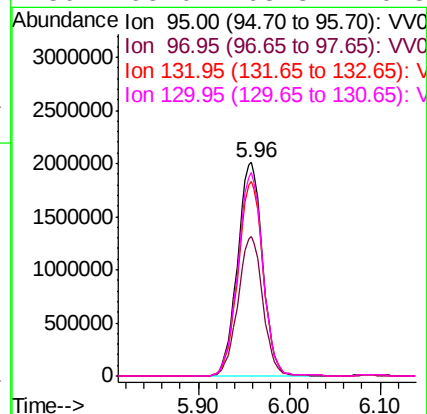
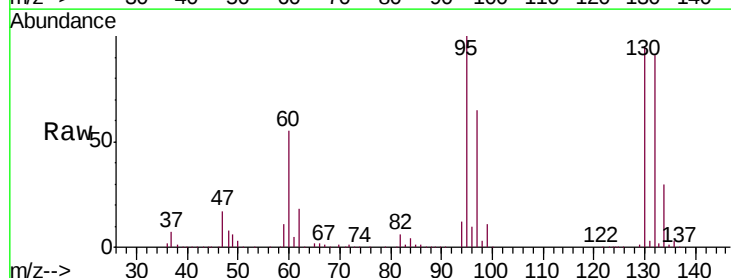




#35
Methylcyclohexane
Concen: 0.702 ug/L
RT: 6.12 min Scan# 1563
Delta R.T. -0.05 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59




Instrument :
MSVOA_V
ClientSampleId :
BFCP1


Tgt Ion: 83 Resp: 13186
Ion Ratio Lower Upper
83 100
55 1.1 67.0 100.6#
98 0.0 40.0 60.0#

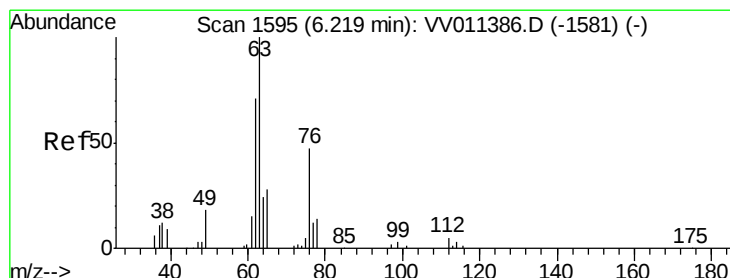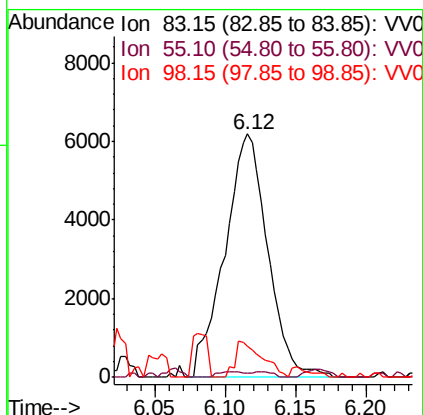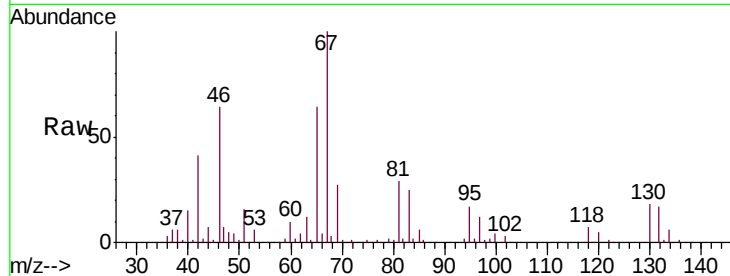

#37
1,2-Dichloropropane
Concen: 0.589 ug/L
RT: 6.12 min Scan# 1563
Delta R.T. -0.10 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59

Tgt Ion: 63 Resp: 6446
Ion Ratio Lower Upper
63 100
112 0.7 3.6 5.4#


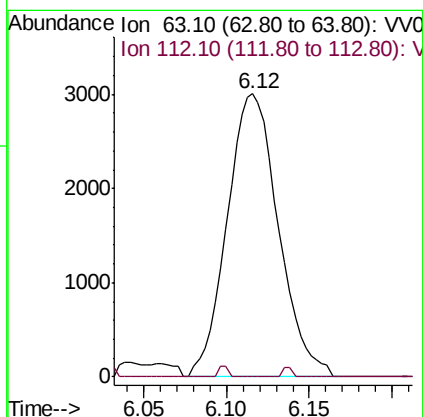

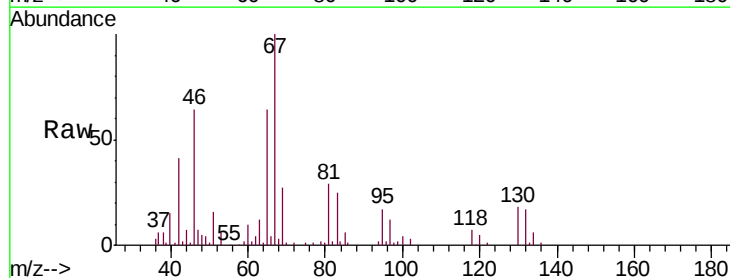


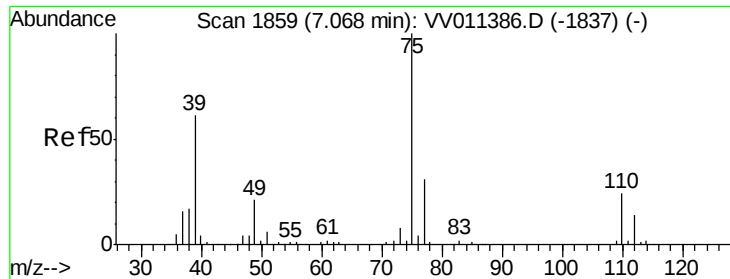

#39
 cis-1,3-Dichloropropene
 Concen: 0.089 ug/L
 RT: 7.03 min Scan# 1846
 Delta R.T. -0.04 min
 Lab File: VV011399.D
 Acq: 11 Jun 2019 17:59




Instrument :
 MSVOA_V
 ClientSampleId :
 BFCP1


Tgt Ion: 75 Resp: 1418
 Ion Ratio Lower Upper
 75 100
 77 78.9 22.2 41.2#

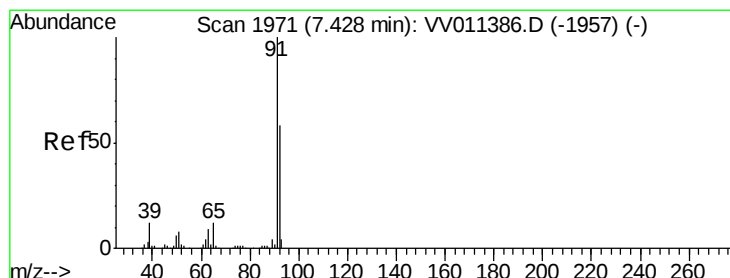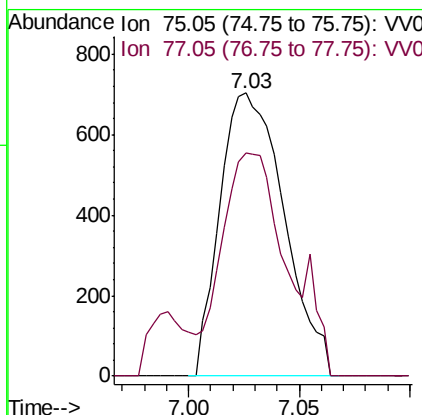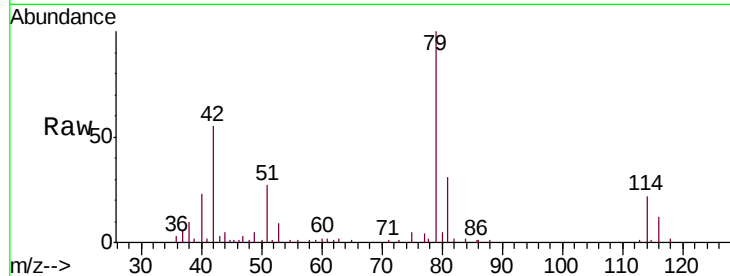

#42
 Toluene
 Concen: 0.255 ug/L
 RT: 7.43 min Scan# 1972
 Delta R.T. 0.00 min
 Lab File: VV011399.D
 Acq: 11 Jun 2019 17:59

Tgt Ion: 91 Resp: 11958
 Ion Ratio Lower Upper
 91 100
 92 55.1 39.9 74.1


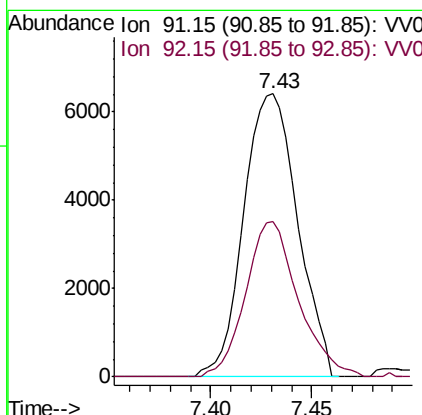

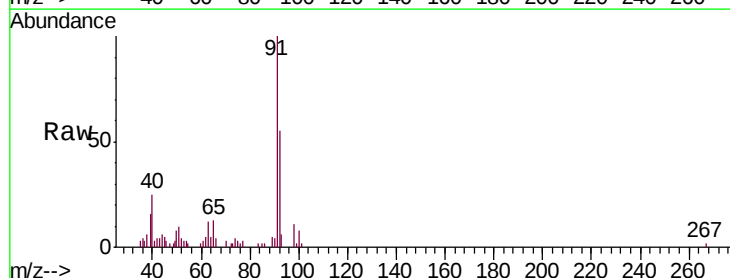


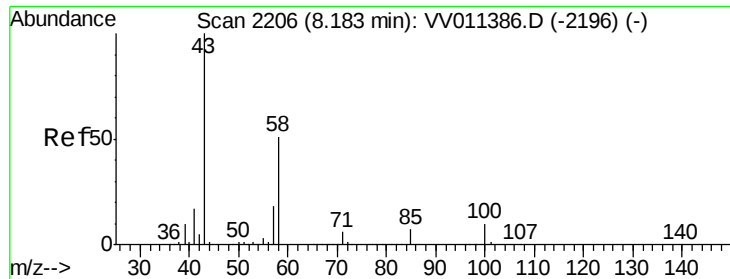

#48
2-Hexanone
Concen: 3.114 ug/L
RT: 8.13 min Scan# 2190
Delta R.T. -0.05 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59

Instrument :
MSVOA_V
ClientSampleId :
BFCP1

Tgt Ion: 43 Resp: 15136
Ion Ratio Lower Upper
43 100
58 26.3 41.4 62.0#
57 26.3 15.0 22.4#
100 0.9 9.0 13.4#

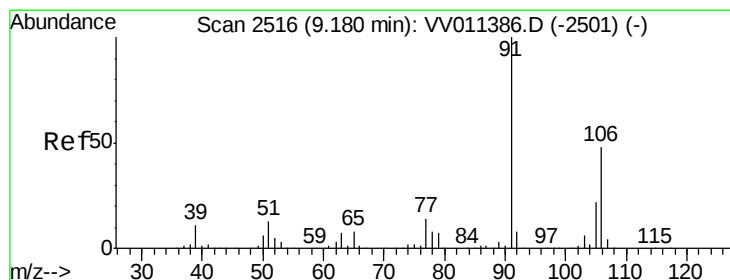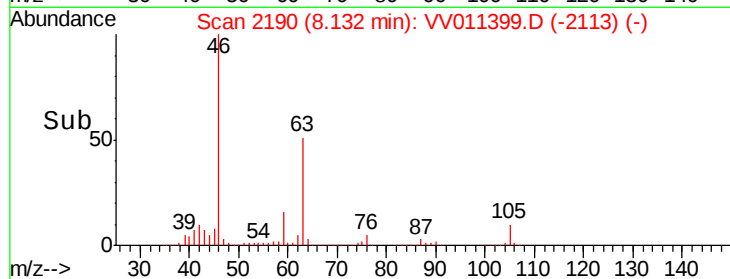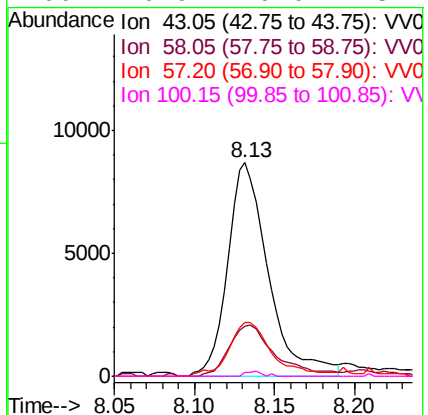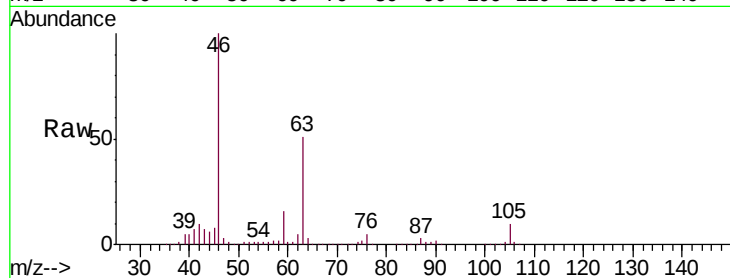

#53
m,p-xylene
Concen: 0.130 ug/L
RT: 9.18 min Scan# 2516
Delta R.T. -0.00 min
Lab File: VV011399.D
Acq: 11 Jun 2019 17:59

Tgt Ion: 106 Resp: 2500
Ion Ratio Lower Upper
106 100
91 169.1 145.5 270.3

