

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011351.D
 Acq On : 10 Jun 2019 15:39
 Operator : SY/MD
 Sample : K3197-16
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Quant Time: Jun 11 02:17:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 11 01:32:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	158827	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	144229	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	56063	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	41398	3.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.80%
7) Chloroethane-d5	1.55	69	37673	3.77	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.40%
11) 1,1-Dichloroethene-d2	2.12	63	71025	2.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.00%#
20) 2-Butanone-d5	3.94	46	134963	49.81	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.62%
24) Chloroform-d	4.40	84	91377	4.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.40%
26) 1,2-Dichloroethane-d4	5.08	65	51256	4.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.60%
32) Benzene-d6	5.09	84	180406	4.18	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.60%
36) 1,2-Dichloropropane-d6	6.11	67	57751	4.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.00%
41) Toluene-d8	7.36	98	156991	3.96	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.20%
43) trans-1,3-Dichloropropene-	7.66	79	17310	3.42	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.40%
46) 2-Hexanone-d5	8.13	63	102151	47.73	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.46%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	40501	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	52286	4.72	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.40%


Target Compounds					Ovalue
13) Acetone	2.19	43	4983	2.743 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011351.D
Acq On : 10 Jun 2019 15:39
Operator : SY/MD
Sample : K3197-16
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Time: Jun 11 02:17:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 11 01:32:35 2019
Response via : Initial Calibration

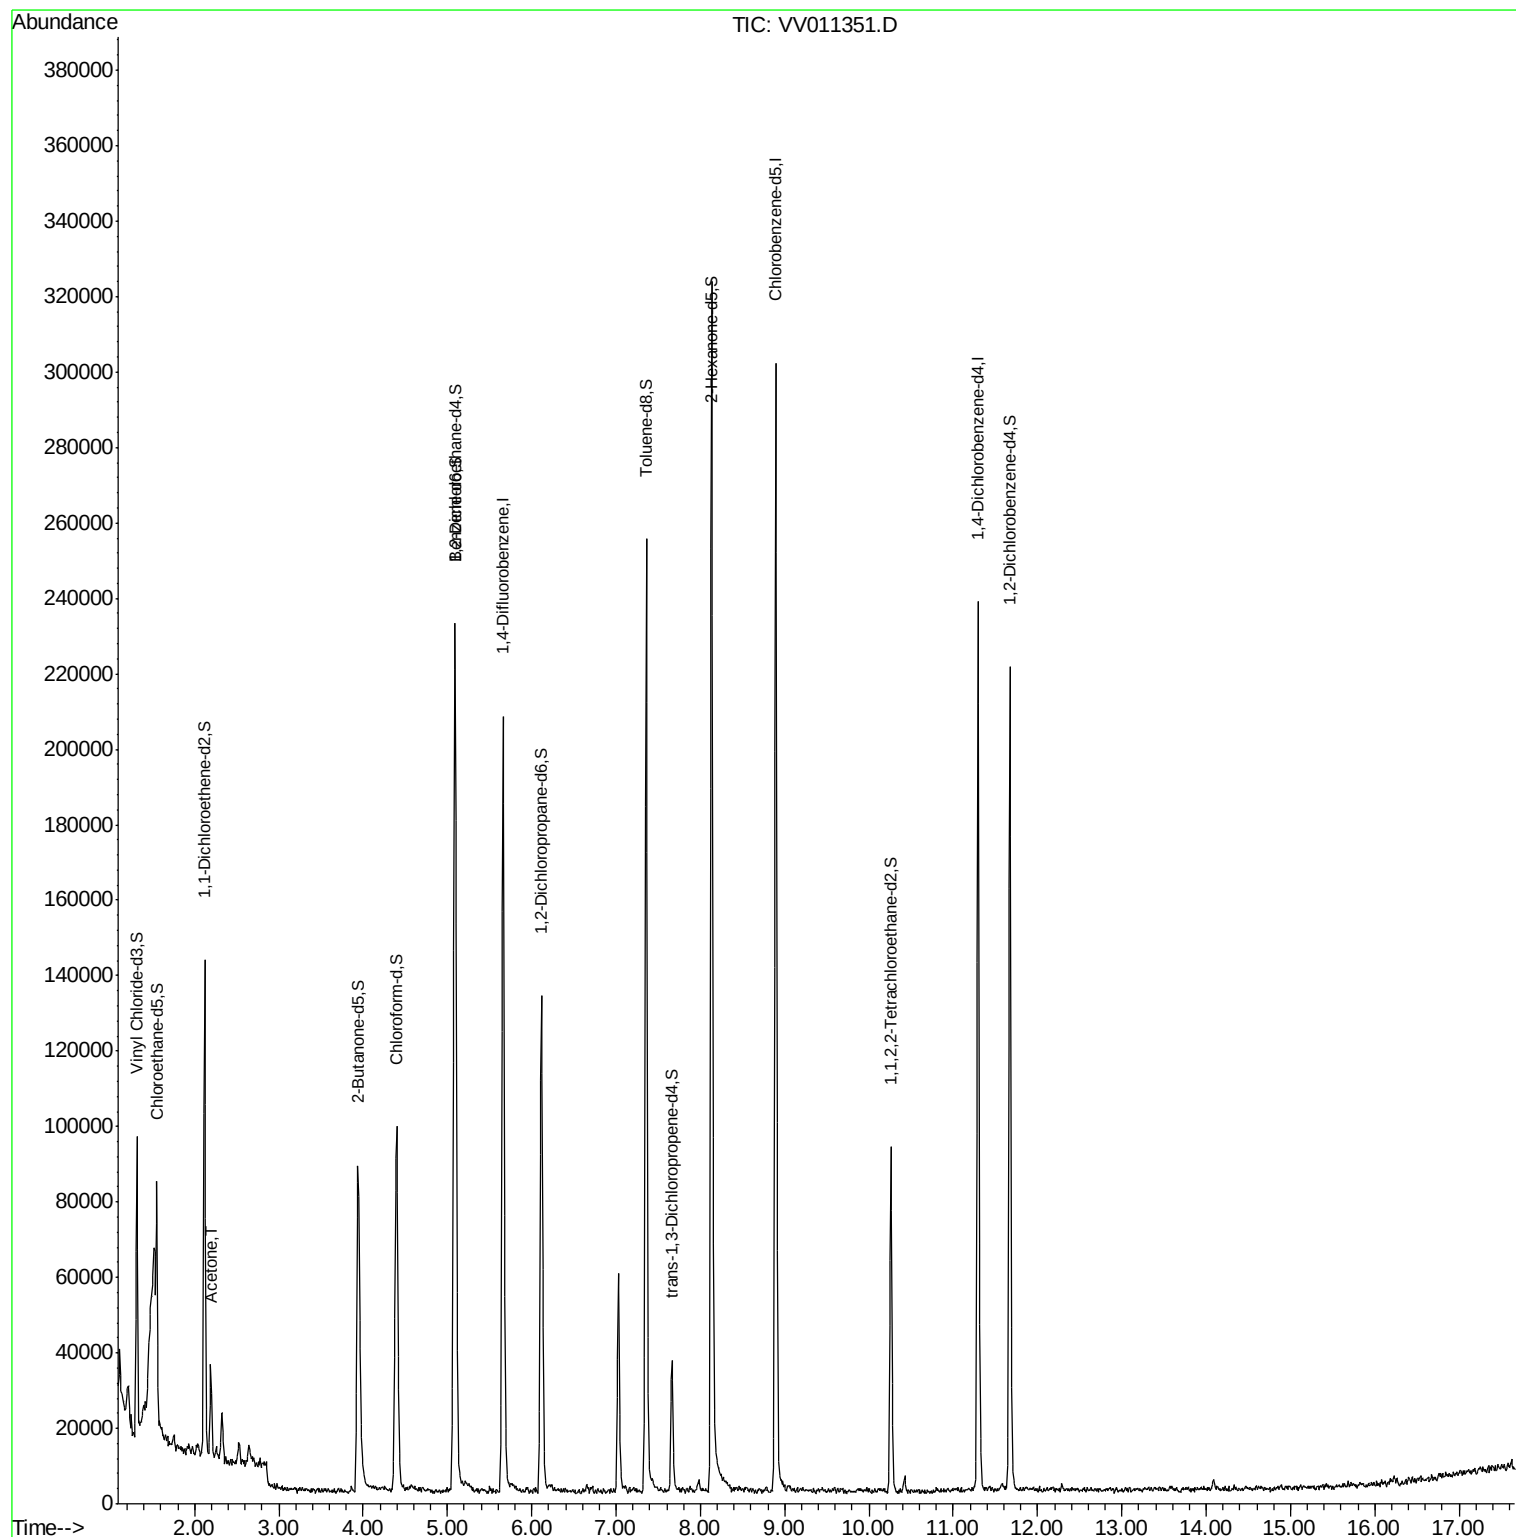

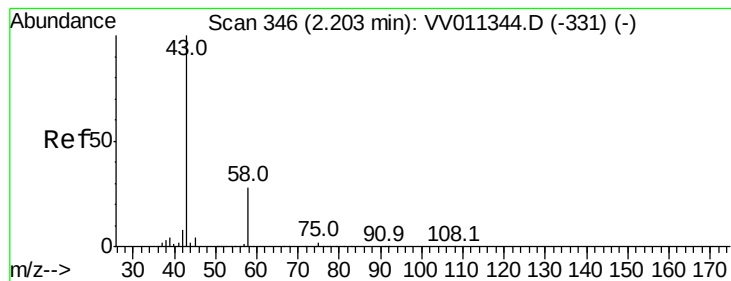

#13

Acetone

Concen: 2.743 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.01 min

Lab File: VV011351.D

Acq: 10 Jun 2019 15:39

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Tot Ion: 43 Resp: 4983

Ion Ratio Lower Upper

43 100

58 31.3 0.0 55.2

