

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011373.D
 Acq On : 11 Jun 2019 04:07
 Operator : SY/MD
 Sample : K3229-08
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P23

Quant Time: Jun 11 04:28:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 11 04:02:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	143694	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	130056	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	50197	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	36982	3.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.00%
7) Chloroethane-d5	1.56	69	34916	3.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.20%
11) 1,1-Dichloroethene-d2	2.12	63	62584	2.88	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.60%#
20) 2-Butanone-d5	3.95	46	123645	50.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.88%
24) Chloroform-d	4.40	84	82205	4.29	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.80%
26) 1,2-Dichloroethane-d4	5.08	65	48366	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
32) Benzene-d6	5.09	84	162286	4.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.40%
36) 1,2-Dichloropropane-d6	6.12	67	51533	4.30	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	86.00%
41) Toluene-d8	7.36	98	136610	3.82	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.40%
43) trans-1,3-Dichloropropene-	7.66	79	12582	2.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	55.00%
46) 2-Hexanone-d5	8.14	63	86050	44.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	89.16%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35375	4.33	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	45571	4.60	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	92.00%


Target Compounds					Ovalue
13) Acetone	2.20	43	7354	4.474 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011373.D
Acq On : 11 Jun 2019 04:07
Operator : SY/MD
Sample : K3229-08
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P23

Quant Time: Jun 11 04:28:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 11 04:02:46 2019
Response via : Initial Calibration

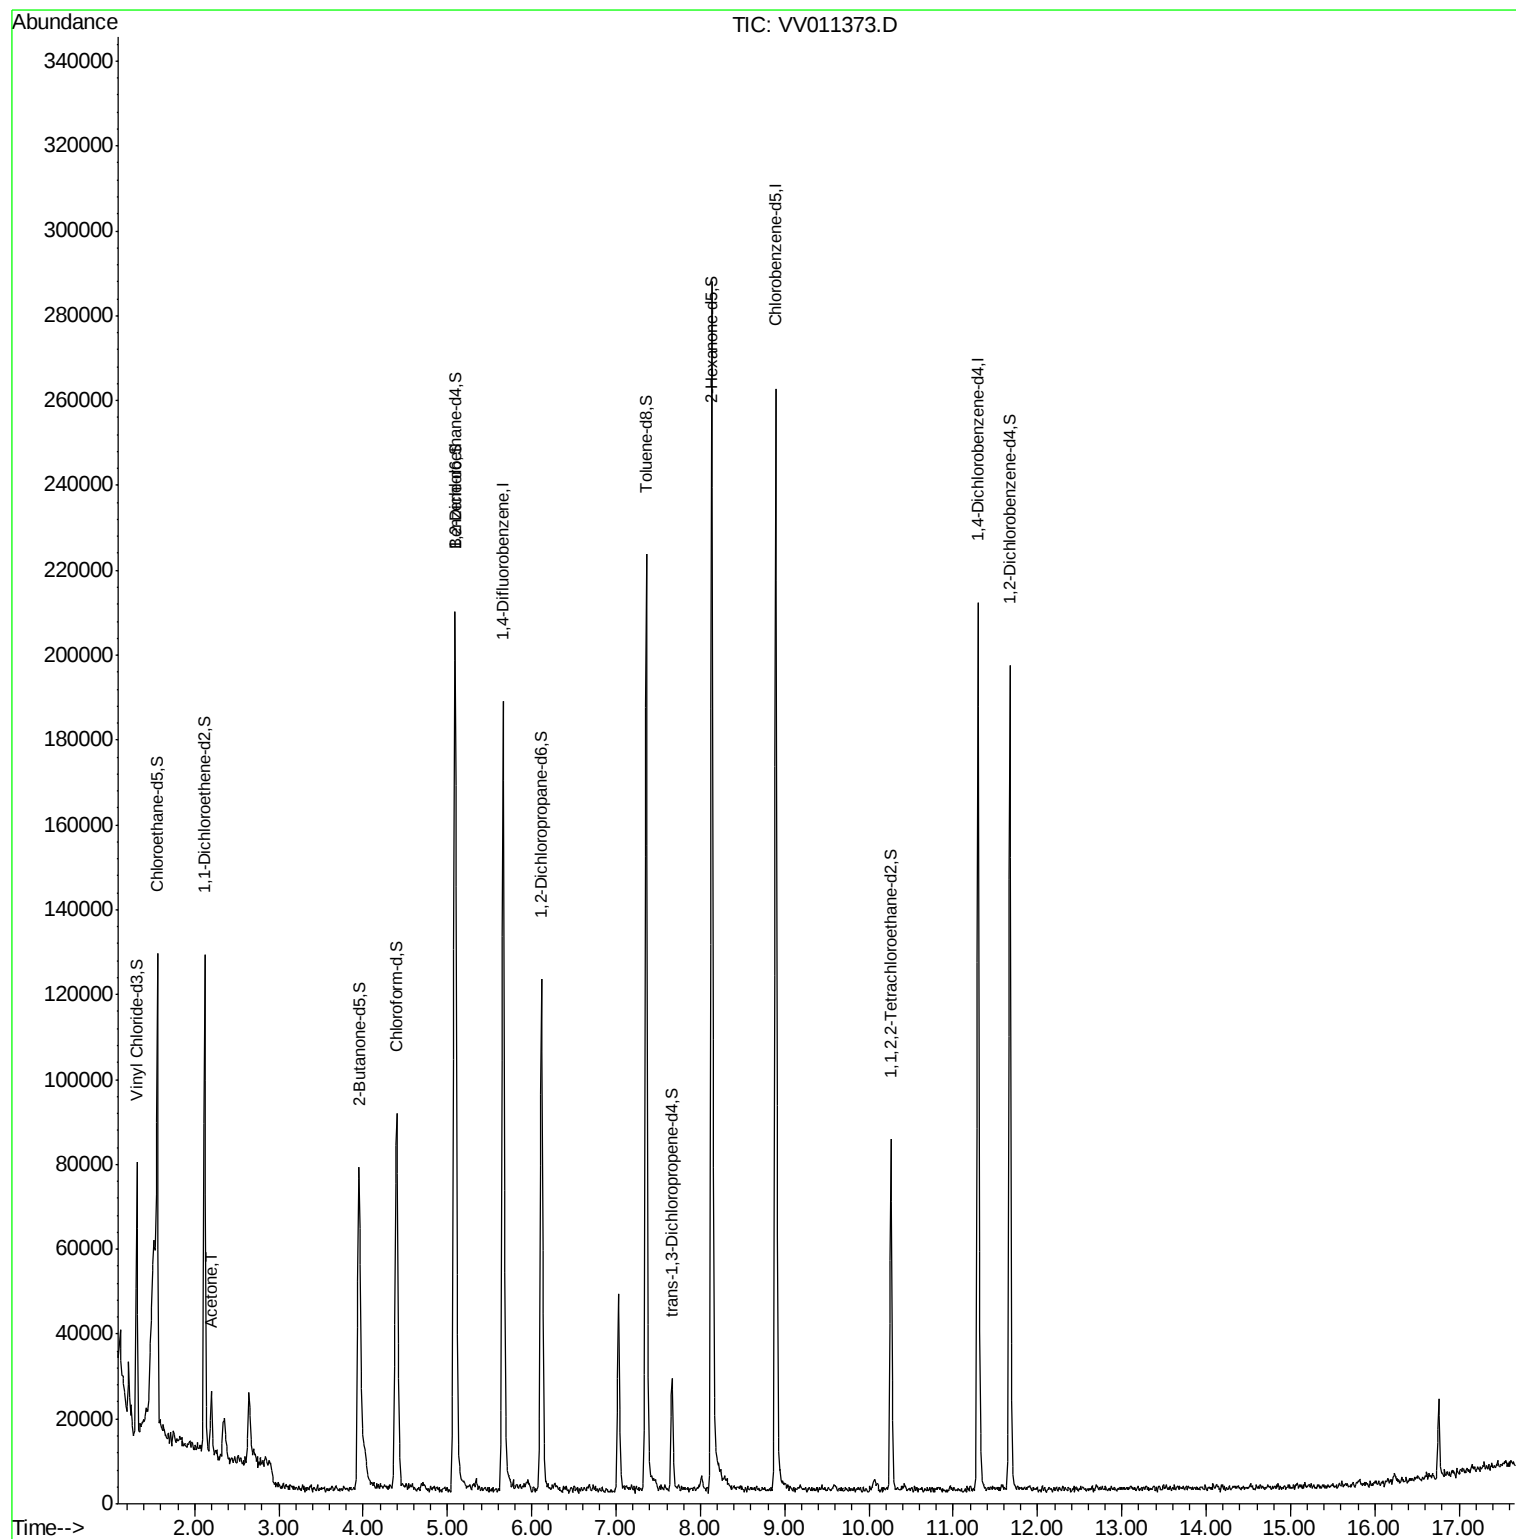

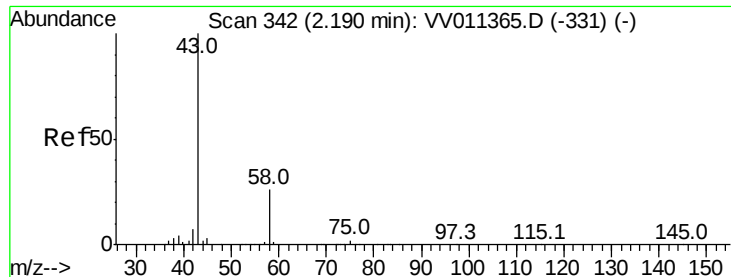

#13

Acetone

Concen: 4.474 ug/L

RT: 2.20 min Scan# 345

Delta R.T. 0.01 min

Lab File: VV011373.D

Acq: 11 Jun 2019 04:07

Instrument :
MSVOA_V
ClientSampleId :
F9P23

Tot Ion: 43 Resp: 7354

Ion Ratio Lower Upper

43 100

58 31.8 0.0 55.2

