

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011375.D
 Acq On : 11 Jun 2019 05:03
 Operator : SY/MD
 Sample : K3229-10
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P30

Quant Time: Jun 11 08:25:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 11 08:01:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	133683	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	122847	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	46633	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	34924	3.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.00%
7) Chloroethane-d5	1.56	69	33967	4.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.60%
11) 1,1-Dichloroethene-d2	2.12	63	59964	2.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	59.20%#
20) 2-Butanone-d5	3.95	46	118274	51.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.72%
24) Chloroform-d	4.40	84	80542	4.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.40%
26) 1,2-Dichloroethane-d4	5.08	65	46929	4.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.40%
32) Benzene-d6	5.09	84	156812	4.27	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.40%
36) 1,2-Dichloropropane-d6	6.12	67	50154	4.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	88.60%
41) Toluene-d8	7.36	98	130405	3.86	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.20%
43) trans-1,3-Dichloropropene-	7.66	79	12641	2.93	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.60%
46) 2-Hexanone-d5	8.14	63	88133	48.34	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.68%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	33990	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	43135	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%


Target Compounds					Ovalue
13) Acetone	2.20	43	8316	5.439 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011375.D
Acq On : 11 Jun 2019 05:03
Operator : SY/MD
Sample : K3229-10
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F9P30

Quant Time: Jun 11 08:25:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 11 08:01:21 2019
Response via : Initial Calibration

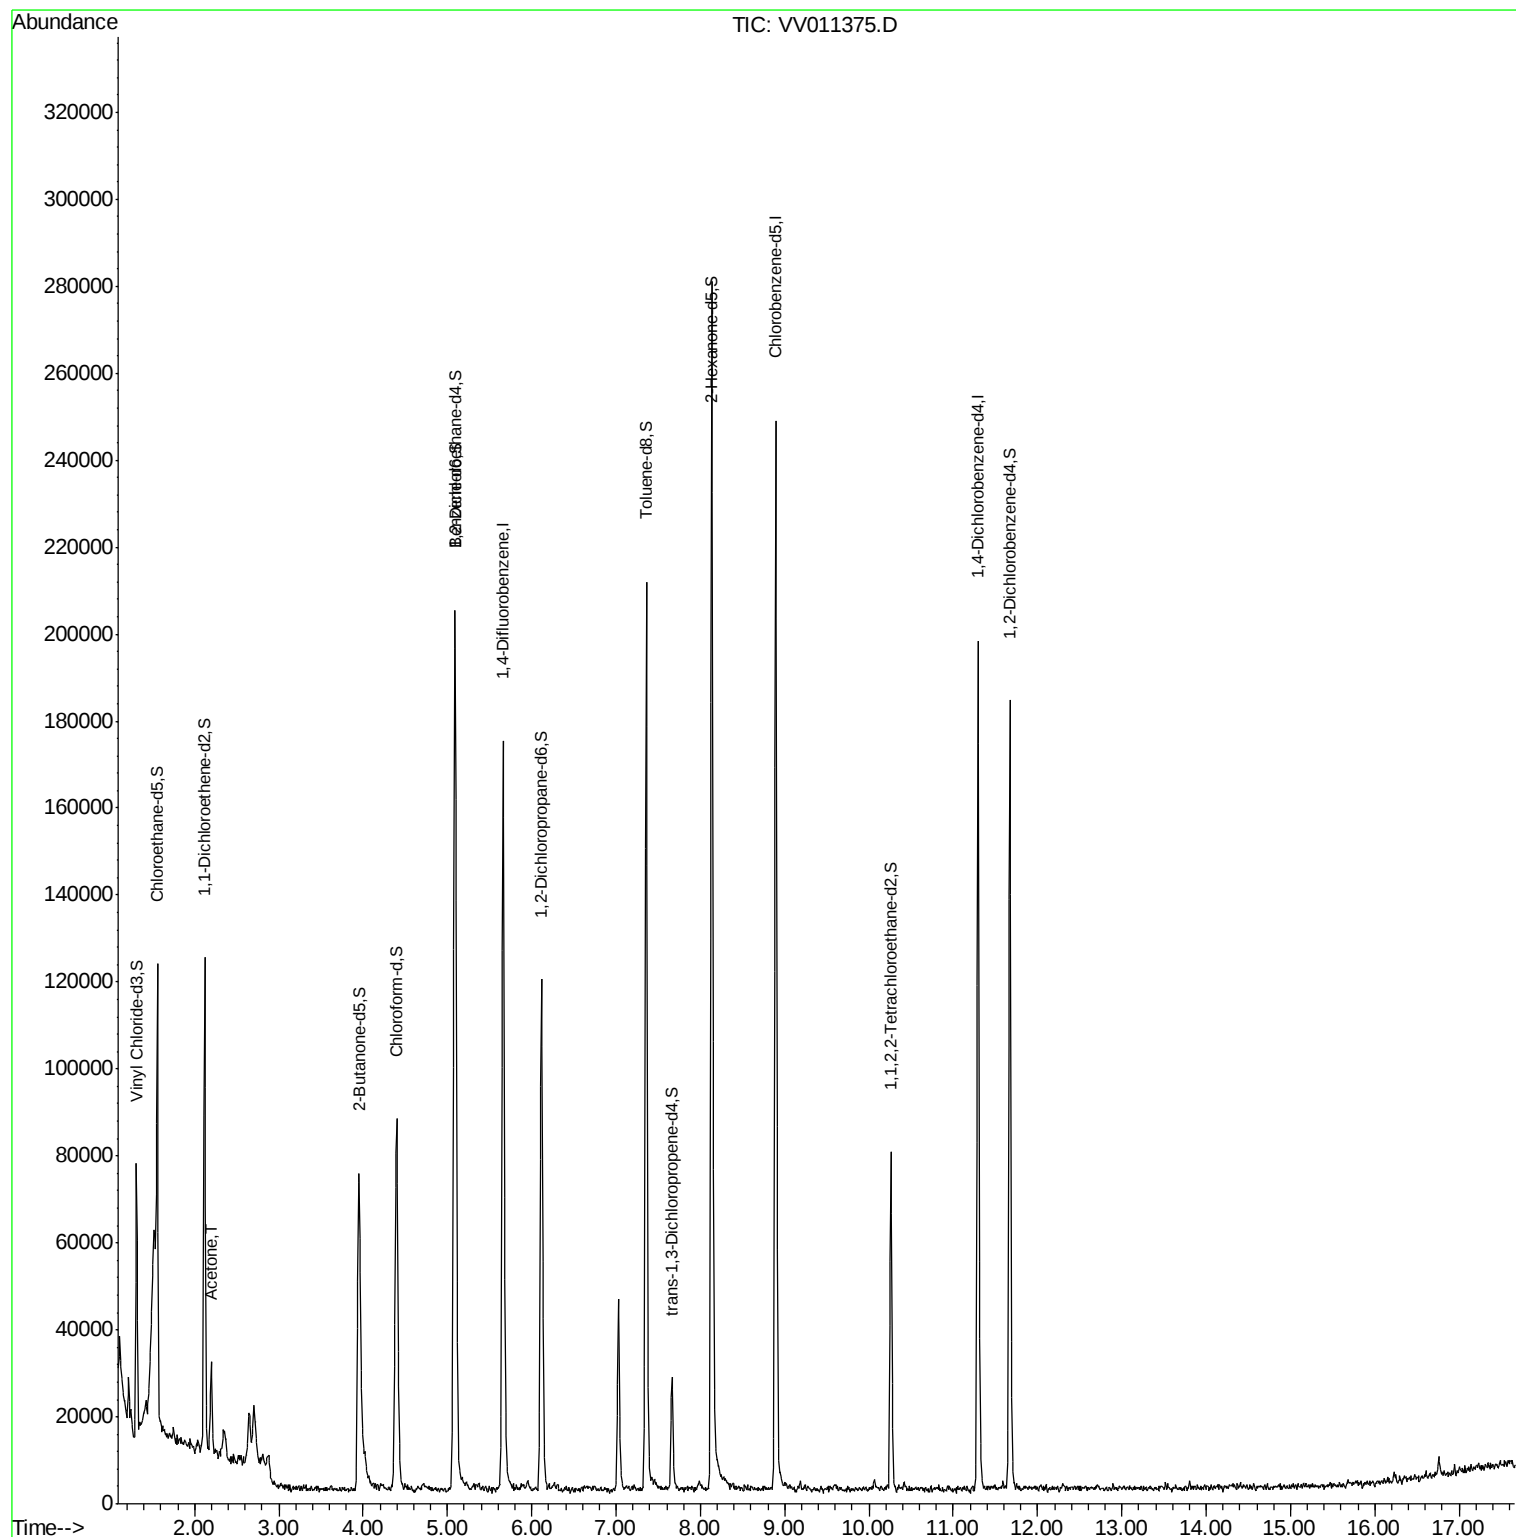

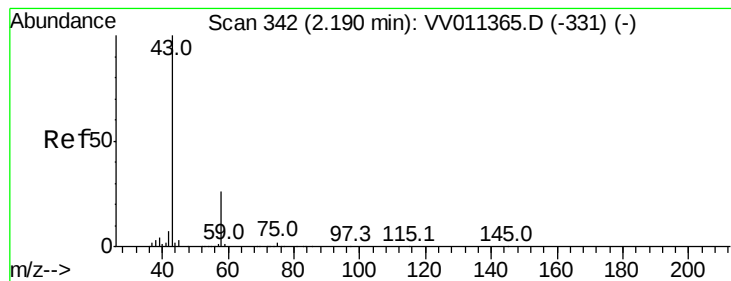

#13
 Acetone
 Concen: 5.439 ug/L
 RT: 2.20 min Scan# 344
 Delta R.T. 0.01 min
 Lab File: VV011375.D
 Acq: 11 Jun 2019 05:03

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P30

Tot Ion: 43 Resp: 8316
 Ion Ratio Lower Upper
 43 100
 58 33.1 0.0 55.2

