

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011379.D
 Acq On : 11 Jun 2019 06:57
 Operator : SY/MD
 Sample : K3229-14
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F9P34

Manual Integrations
 APPROVED

MMDadoda
 6/12/2019 3:04:23 PM

Quant Time: Jun 12 10:58:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Jun 11 08:01:21 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	141957	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	129507	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	53400	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	36933	3.43	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.60%
7) Chloroethane-d5	1.58	69	36384	4.07	ug/L	0.03
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.40%
11) 1,1-Dichloroethene-d2	2.12	63	66128	3.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.60%
20) 2-Butanone-d5	3.98	46	125214	51.71	ug/L	0.04
Spiked Amount	50.000	Range	40 - 130	Recovery	=	103.42%
24) Chloroform-d	4.40	84	86462	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.08	65	49384	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.09	84	165940	4.28	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.60%
36) 1,2-Dichloropropane-d6	6.12	67	52170	4.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.40%
41) Toluene-d8	7.36	98	143804	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.80%
43) trans-1,3-Dichloropropene-	7.67	79	13210	2.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.00%
46) 2-Hexanone-d5	8.14	63	99555	51.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.60%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38182	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	50271	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%

Target Compounds				Ovalue
13) Acetone	2.24	43	16976m	10.455 ug/L
14) Carbon disulfide	2.31	76	4882	0.180 ug/L # 81
47) Tetrachloroethene	8.02	164	1611	0.209 ug/L 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011379.D
Acq On : 11 Jun 2019 06:57
Operator : SY/MD
Sample : K3229-14
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F9P34

Manual Integrations
APPROVED

MMDadoda
6/12/2019 3:04:23 PM

Quant Time: Jun 12 10:58:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Jun 11 08:01:21 2019
Response via : Initial Calibration

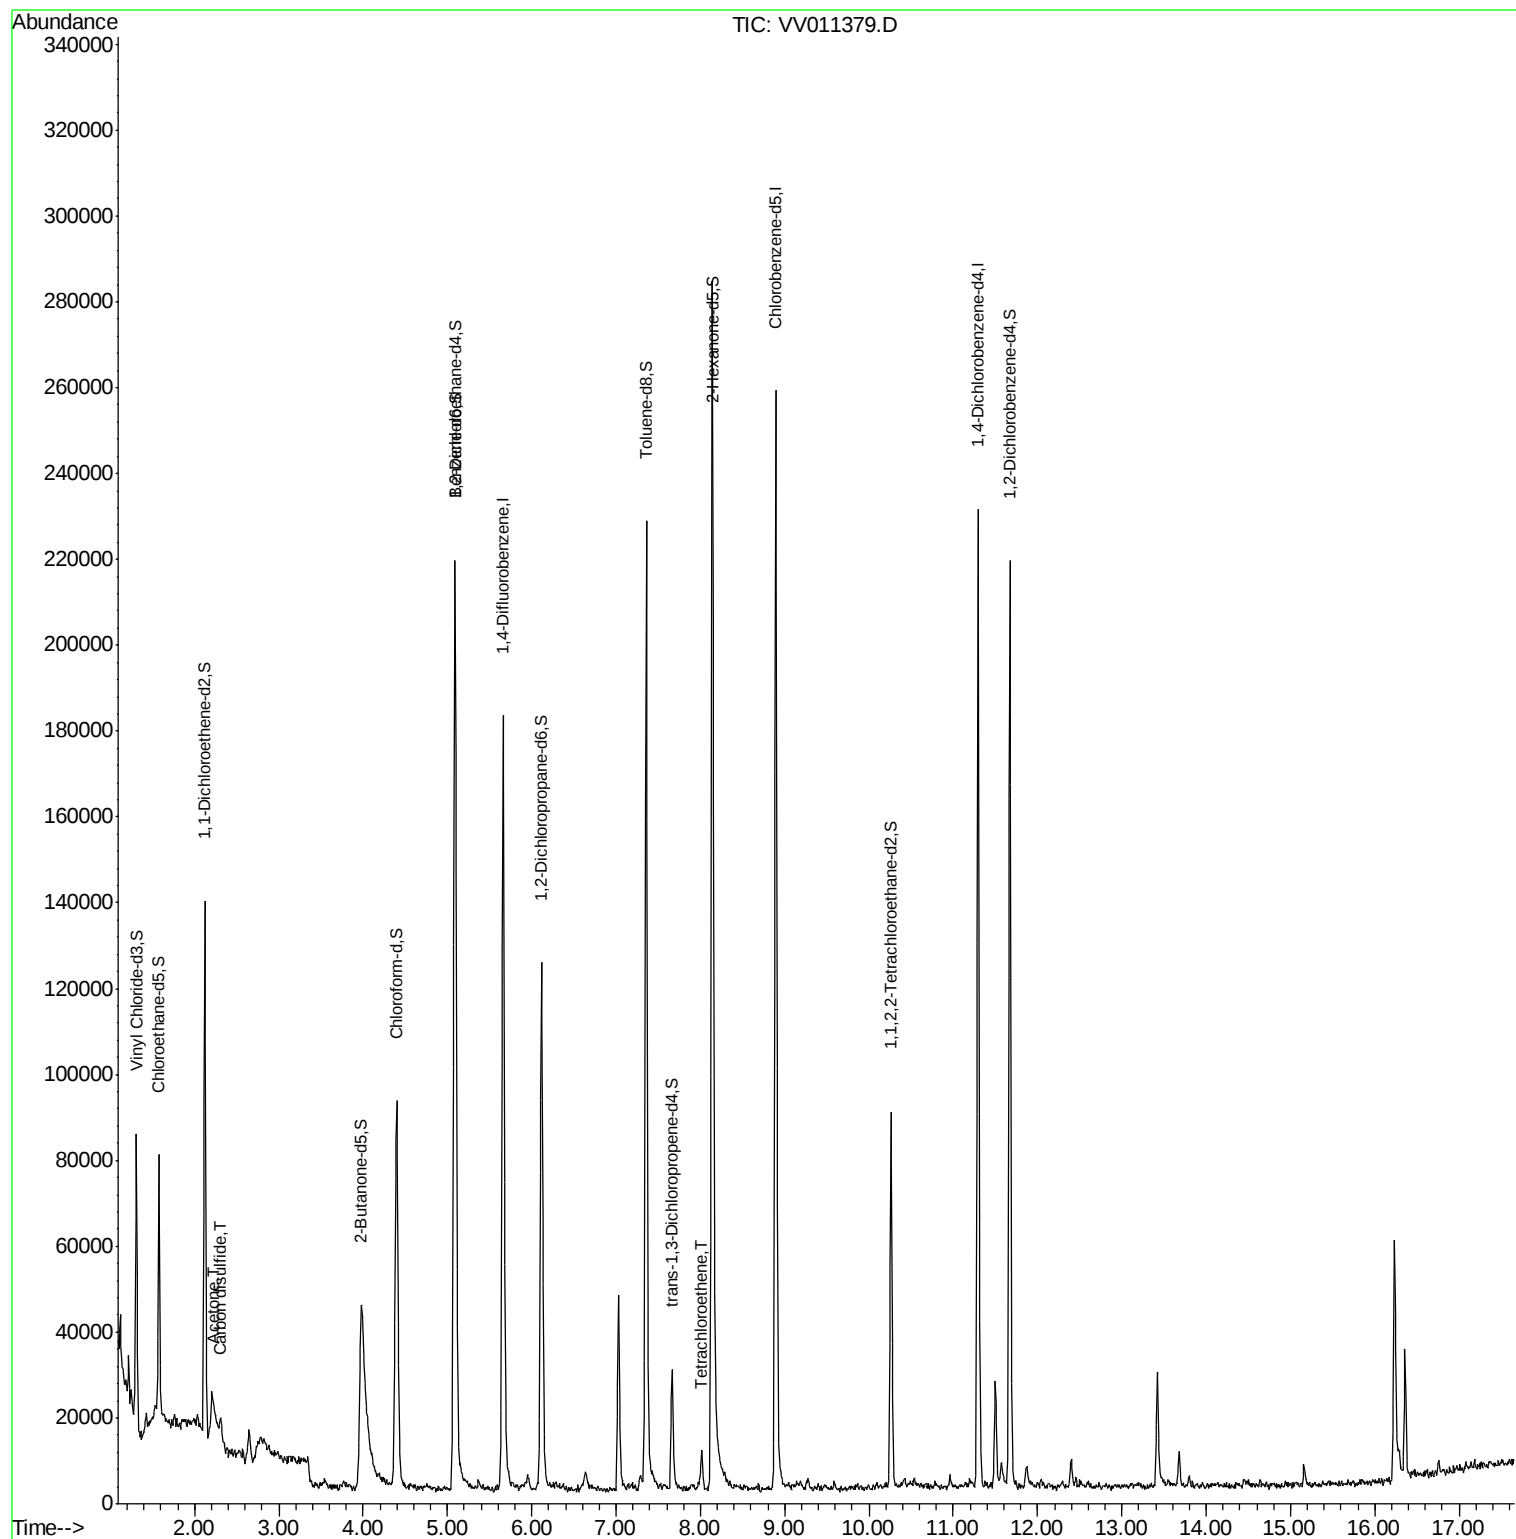

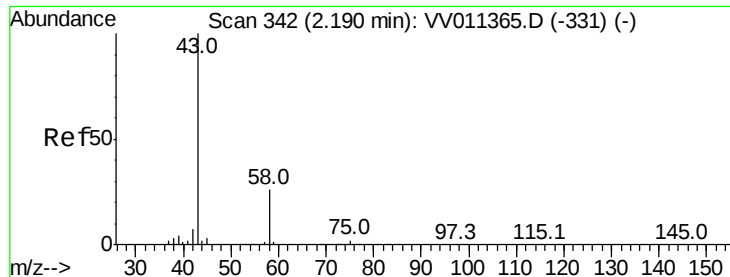

#13

Acetone

Concen: 10.455 ug/L m

RT: 2.24 min Scan# 357

Delta R.T. 0.05 min

Lab File: VV011379.D

Acq: 11 Jun 2019 06:57

Instrument :

MSVOA_V

ClientSampled :

F9P34

Tot Ion: 43 Resp: 16976





Ion Ratio Lower Upper

43 100

58 3.6 0.0 55.2

Manual Integrations
APPROVED

MMDadoda
6/12/2019 3:04:23 PM

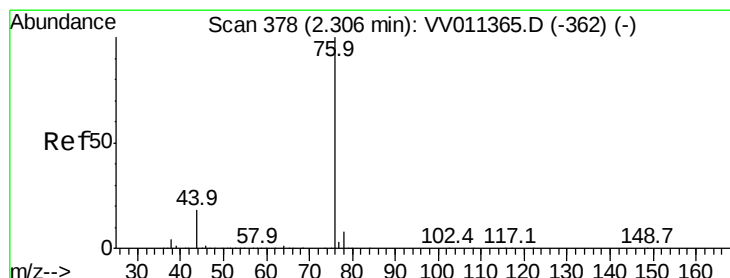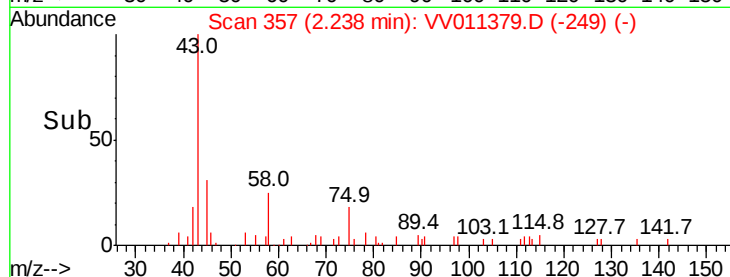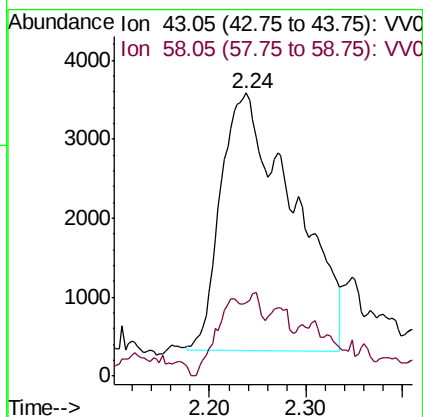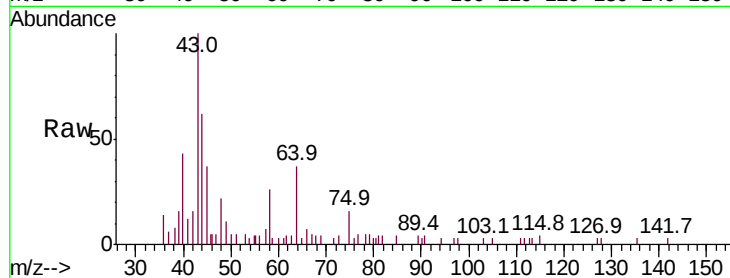

#14

Carbon disulfide

Concen: 0.180 ug/L

RT: 2.31 min Scan# 379

Delta R.T. 0.00 min

Lab File: VV011379.D




Acq: 11 Jun 2019 06:57


Tgt Ion: 76 Resp: 4882

Ion Ratio Lower Upper

76 100

78 15.9 7.3 10.9#

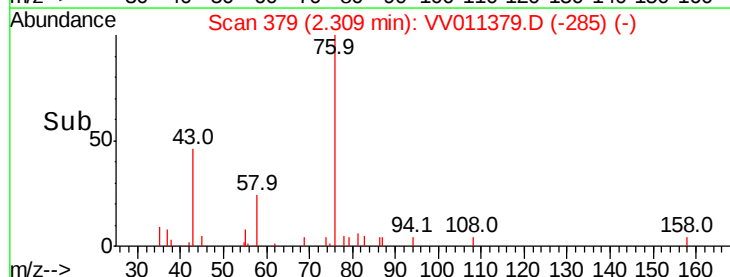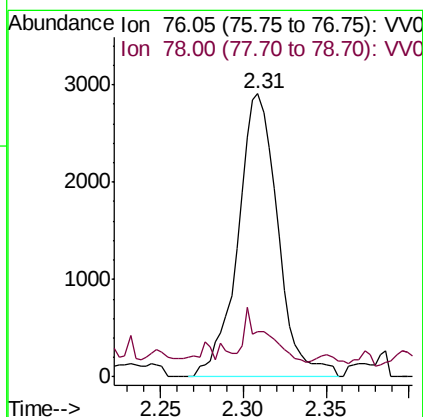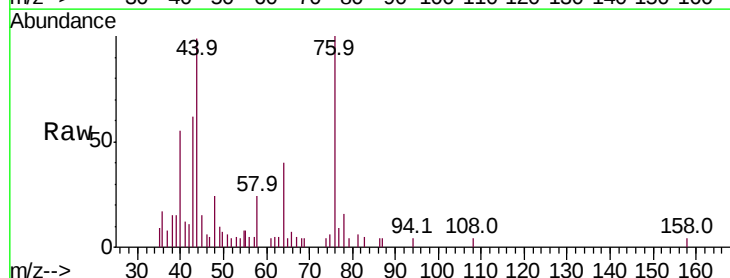

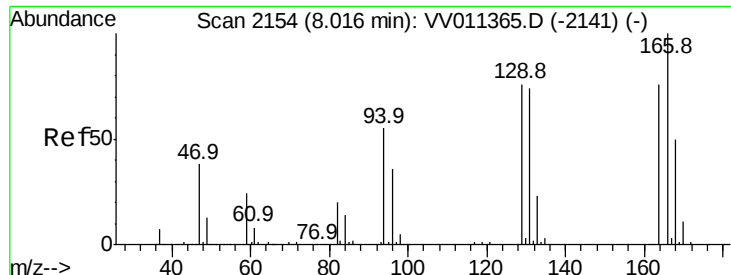

#47

Tetrachloroethene

Concen: 0.209 ug/L


RT: 8.02 min Scan# 2154

Delta R.T. -0.00 min

Lab File: VV011379.D

Acq: 11 Jun 2019 06:57

Instrument :
MSVOA_V
ClientSampleId :
F9P34

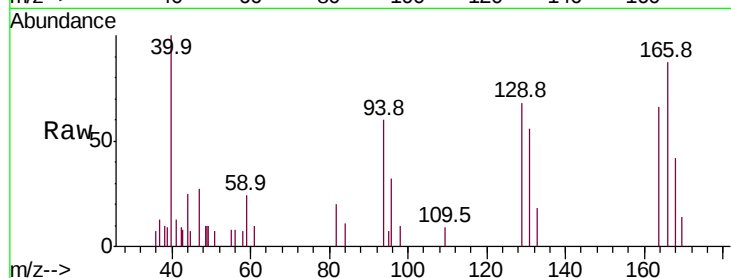

Tot Ion:164 Resp: 1611

Ion Ratio Lower Upper

164 100


129 102.4 69.9 129.9

131 83.9 66.8 124.2

166 130.9 90.2 167.6

Manual Integrations
APPROVED

MMDadoda
6/12/2019 3:04:23 PM

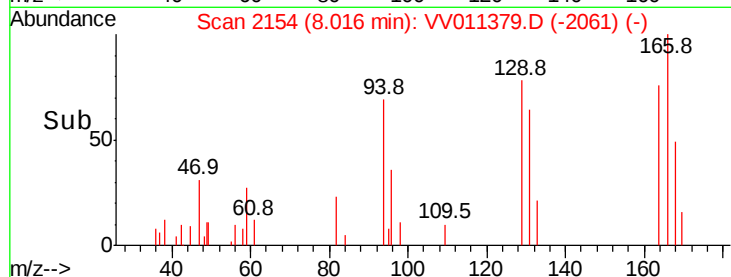

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

