

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011390.D
 Acq On : 11 Jun 2019 13:04
 Operator : SY/MD
 Sample : K3291-01
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8G0

Quant Time: Jun 12 03:41:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 12 02:48:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	148383	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	139397	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	52800	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	36454	3.24	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	64.80%
7) Chloroethane-d5	1.55	69	35194	3.77	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.40%
11) 1,1-Dichloroethene-d2	2.12	63	59405	2.64	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.80%#
20) 2-Butanone-d5	3.94	46	124435	49.16	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.32%
24) Chloroform-d	4.40	84	81473	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.40%
26) 1,2-Dichloroethane-d4	5.08	65	47483	4.44	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.80%
32) Benzene-d6	5.09	84	158437	3.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	76.00%
36) 1,2-Dichloropropane-d6	6.12	67	51342	4.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	80.00%
41) Toluene-d8	7.36	98	137712	3.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.00%
43) trans-1,3-Dichloropropene-	7.66	79	14174	2.89	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	57.80%
46) 2-Hexanone-d5	8.13	63	90731	43.86	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.72%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	36690	4.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	44622	4.28	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	12206	7.192 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011390.D
Acq On : 11 Jun 2019 13:04
Operator : SY/MD
Sample : K3291-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8G0

Quant Time: Jun 12 03:41:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 02:48:56 2019
Response via : Initial Calibration

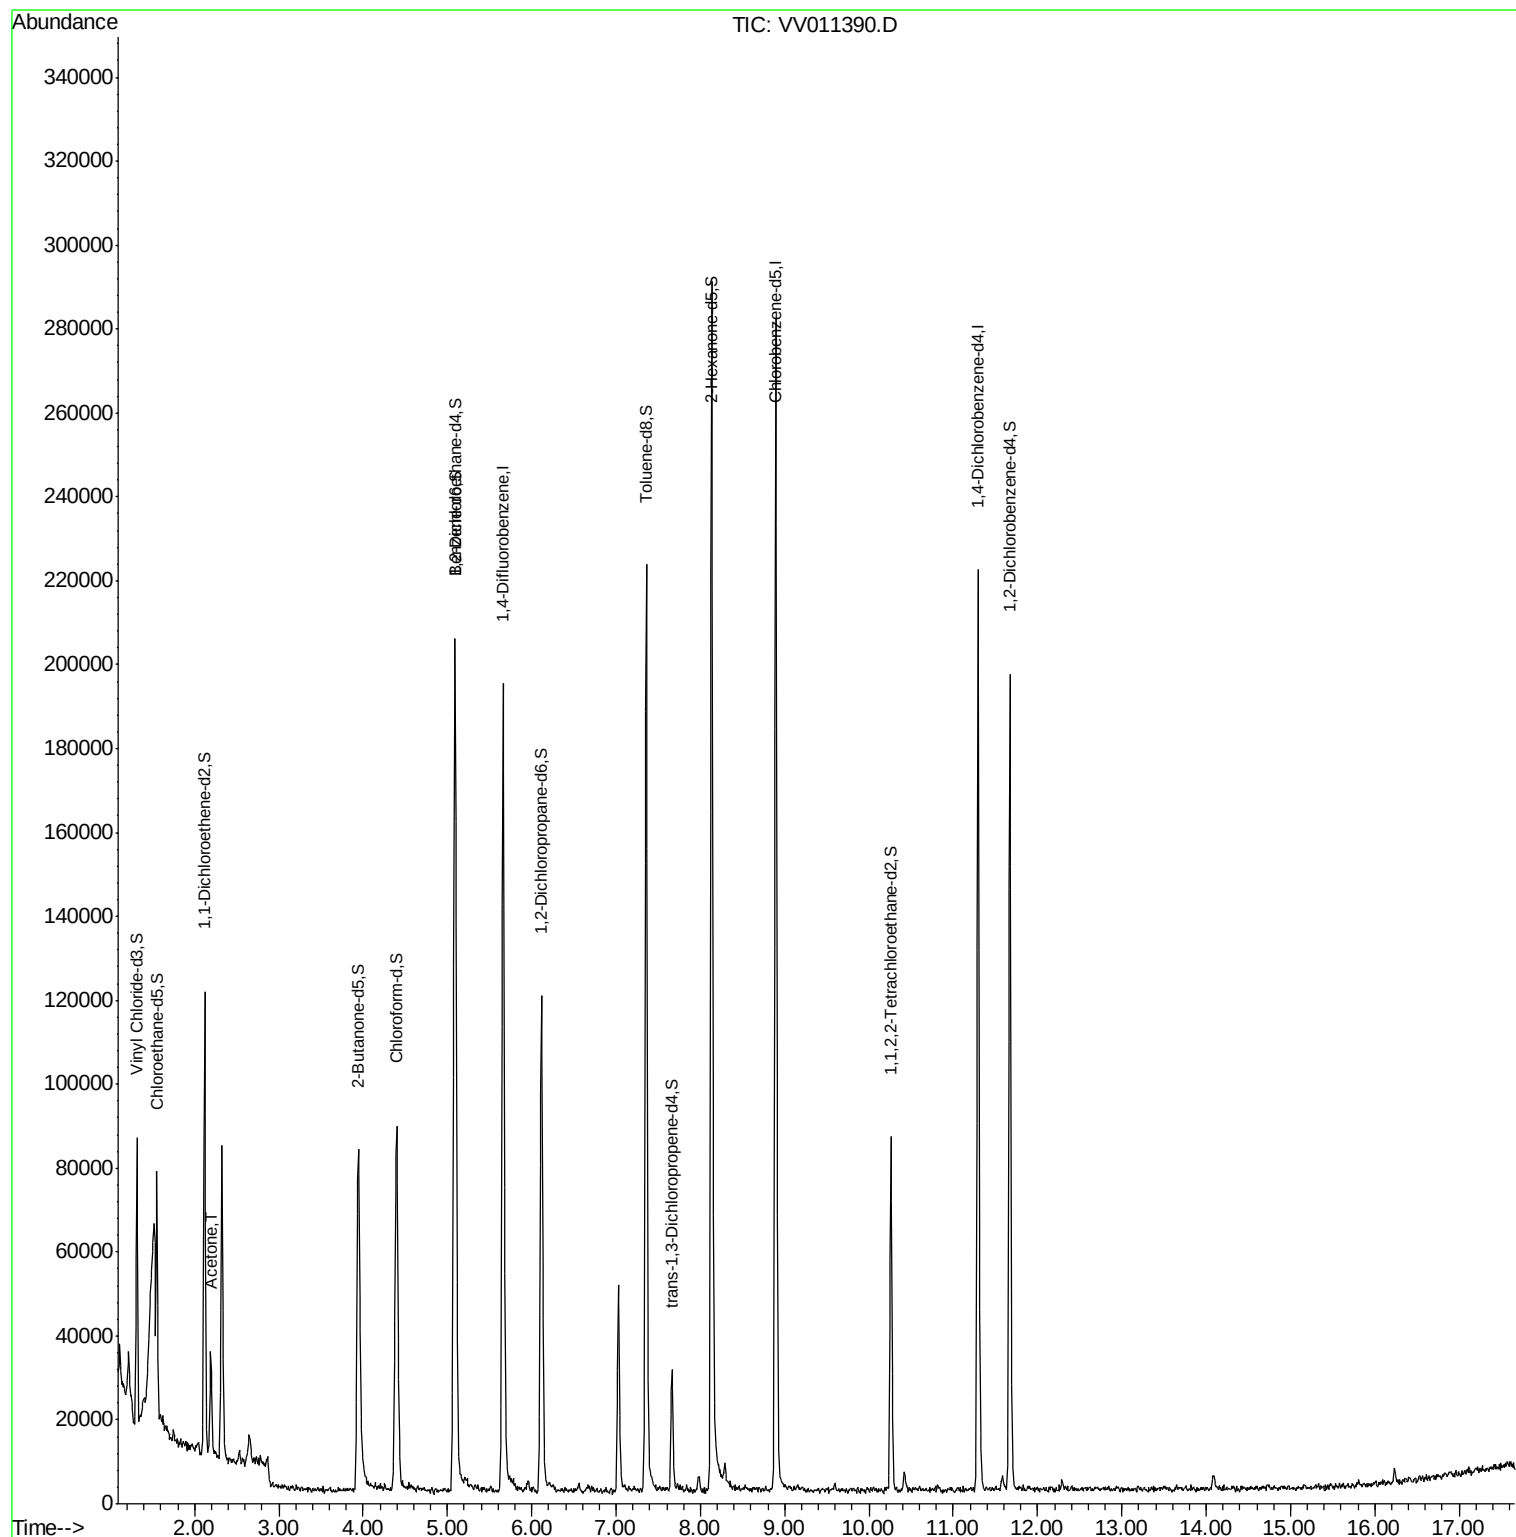

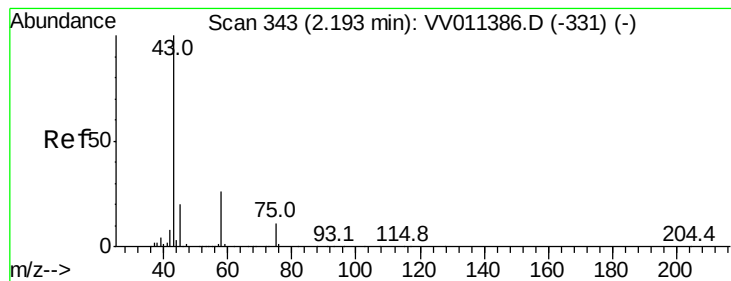

#13
 Acetone
 Concen: 7.192 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. -0.00 min
 Lab File: VV011390.D
 Acq: 11 Jun 2019 13:04

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8G0

Tot Ion: 43 Resp: 12206
 Ion Ratio Lower Upper
 43 100
 58 29.1 0.0 55.2

