

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011401.D
 Acq On : 11 Jun 2019 19:24
 Operator : SY/MD
 Sample : K3291-01
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8G0

Quant Time: Jun 12 04:26:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 12 02:48:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	137390	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	128933	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	49943	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29050	2.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.80%
7) Chloroethane-d5	1.55	69	29562	3.42	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.40%
11) 1,1-Dichloroethene-d2	2.12	63	50583	2.43	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	48.60%#
20) 2-Butanone-d5	3.94	46	135508	57.82	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.64%
24) Chloroform-d	4.40	84	75326	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	82.20%
26) 1,2-Dichloroethane-d4	5.08	65	47080	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	5.09	84	141743	3.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.40%
36) 1,2-Dichloropropane-d6	6.11	67	46906	3.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.00%
41) Toluene-d8	7.36	98	120003	3.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	67.80%#
43) trans-1,3-Dichloropropene-	7.66	79	13156	2.90	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	58.00%
46) 2-Hexanone-d5	8.13	63	100008	52.27	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.54%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38997	4.81	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	43256	4.39	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.80%


Target Compounds					Ovalue
13) Acetone	2.19	43	13540	8.616 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011401.D
Acq On : 11 Jun 2019 19:24
Operator : SY/MD
Sample : K3291-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8G0

Quant Time: Jun 12 04:26:56 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 02:48:56 2019
Response via : Initial Calibration

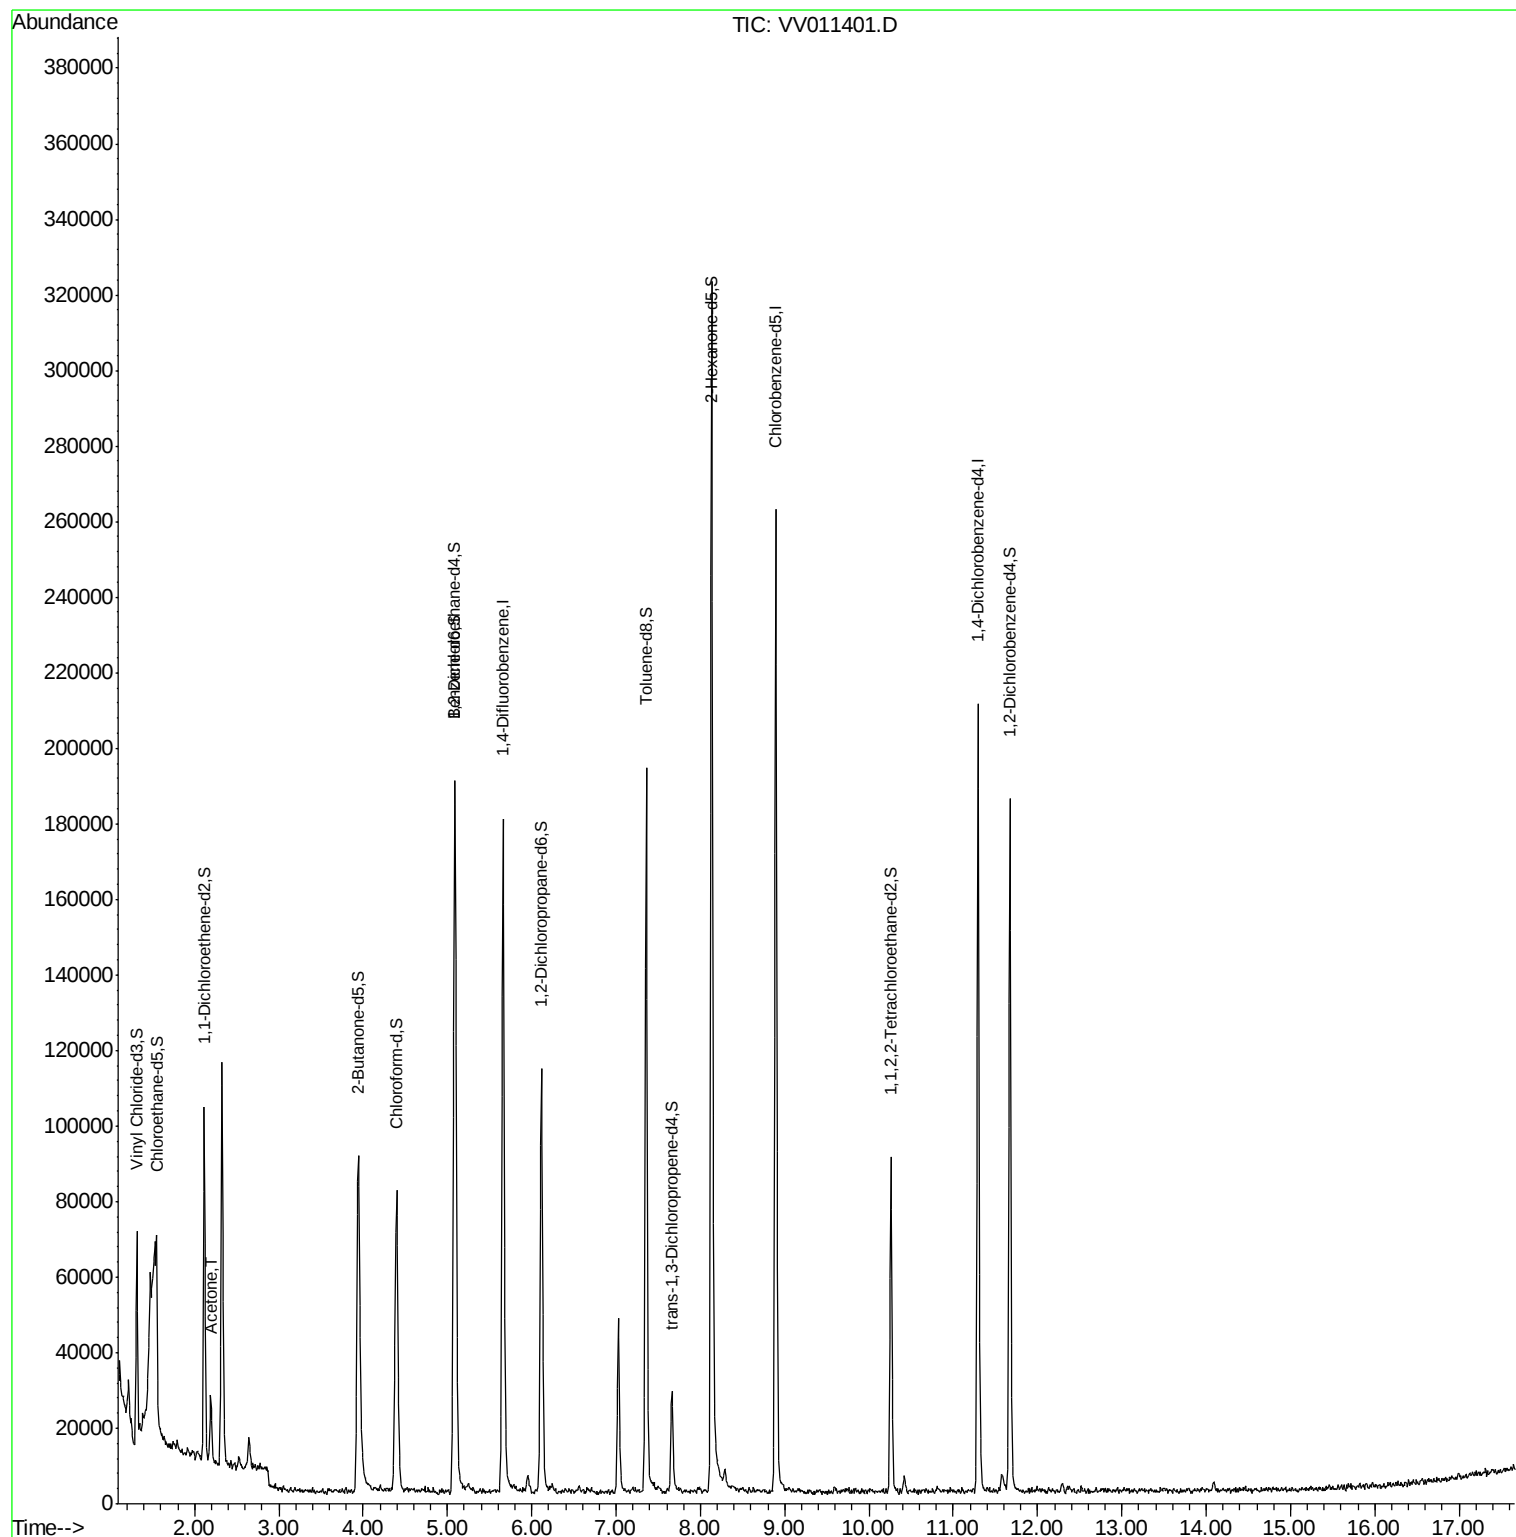

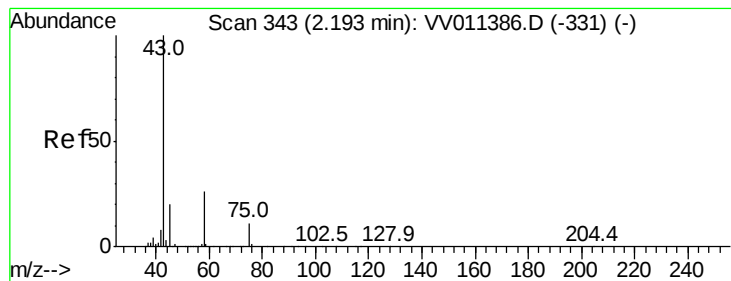

#13

Acetone

Concen: 8.616 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011401.D

Acq: 11 Jun 2019 19:24

Instrument :
MSVOA_V
ClientSampleId :
DB8G0

Tot Ion: 43 Resp: 13540

Ion Ratio Lower Upper

43 100

58 30.5 0.0 55.2

