

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011403.D
 Acq On : 11 Jun 2019 20:20
 Operator : SY/MD
 Sample : K3289-05
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCT5

Quant Time: Jun 12 04:37:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 12 02:48:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	131275	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	121288	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	48095	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27546	2.77	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	55.40%
7) Chloroethane-d5	1.56	69	28341	3.43	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	68.60%
11) 1,1-Dichloroethene-d2	2.12	63	46862	2.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	47.20%#
20) 2-Butanone-d5	3.95	46	127410	56.89	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.78%
24) Chloroform-d	4.40	84	73471	4.20	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	84.00%
26) 1,2-Dichloroethane-d4	5.08	65	43525	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.00%
32) Benzene-d6	5.09	84	133898	3.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.80%
36) 1,2-Dichloropropane-d6	6.12	67	44361	3.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.40%
41) Toluene-d8	7.36	98	110527	3.32	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	66.40%#
43) trans-1,3-Dichloropropene-	7.66	79	11471	2.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	53.80%#
46) 2-Hexanone-d5	8.14	63	91434	50.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.60%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35607	4.67	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	41600	4.38	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.60%


Target Compounds					Ovalue
13) Acetone	2.20	43	3598	2.396 ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011403.D
Acq On : 11 Jun 2019 20:20
Operator : SY/MD
Sample : K3289-05
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFCT5

Quant Time: Jun 12 04:37:58 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 02:48:56 2019
Response via : Initial Calibration

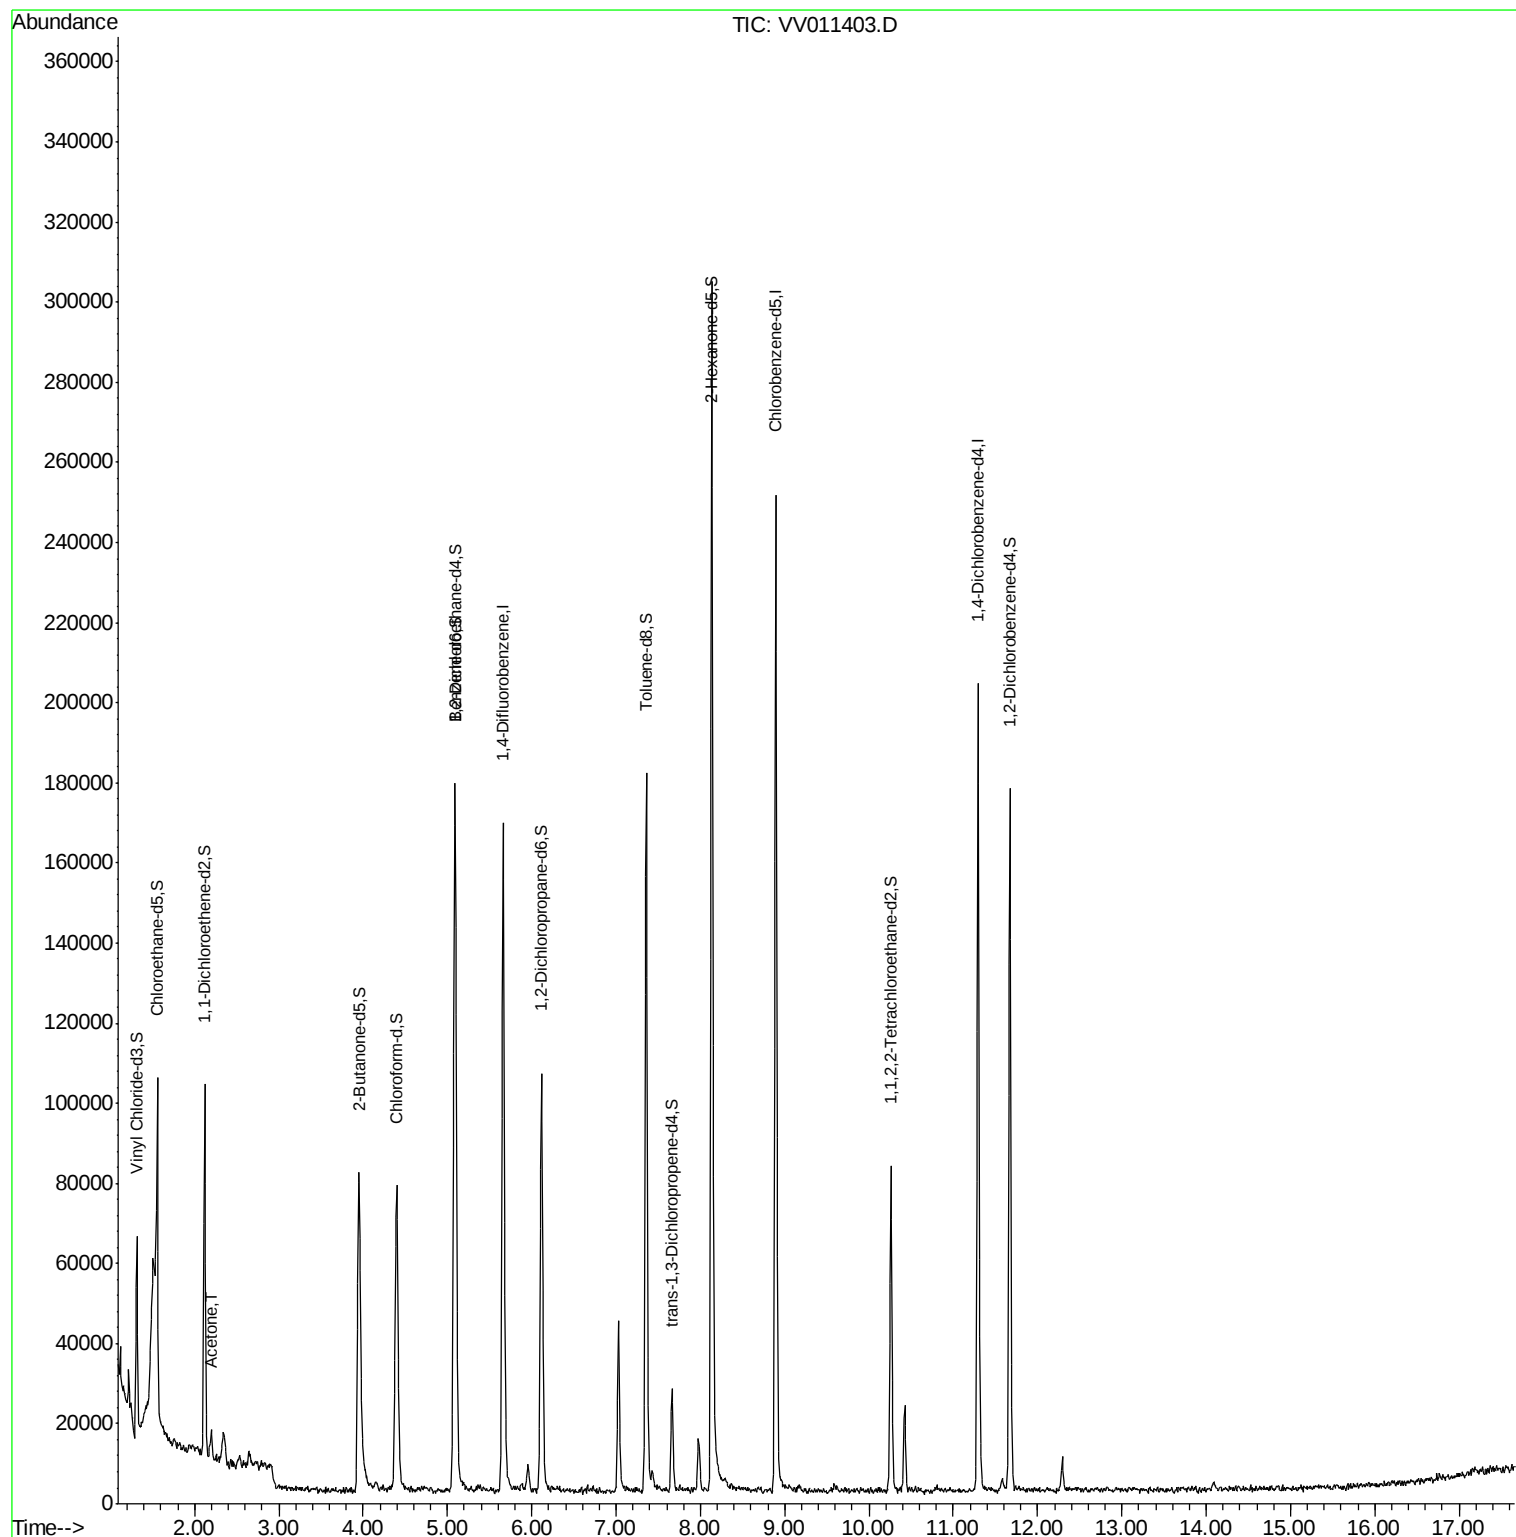

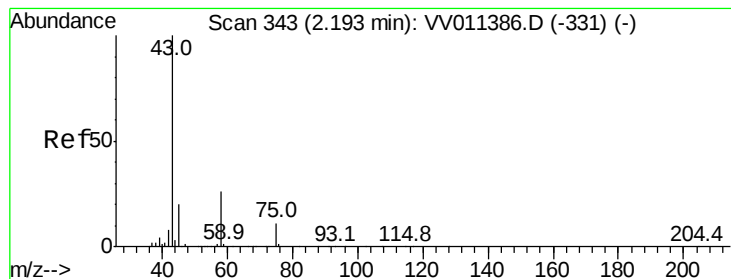

#13
 Acetone
 Concen: 2.396 ug/L
 RT: 2.20 min Scan# 346
 Delta R.T. 0.01 min
 Lab File: VV011403.D
 Acq: 11 Jun 2019 20:20

Instrument :
 MSVOA_V
 ClientSampleId :
 BFCT5

Tot Ion: 43 Resp: 3598
 Ion Ratio Lower Upper
 43 100
 58 38.6 0.0 55.2

