

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
 Data File : VV011406.D
 Acq On : 11 Jun 2019 23:10
 Operator : SY/MD
 Sample : K3286-01
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0JQ4

Quant Time: Jun 12 04:50:40 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Jun 12 04:39:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	141428	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	130484	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	49708	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	29133	2.72	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	54.40%
7) Chloroethane-d5	1.57	69	31659	3.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	71.00%
11) 1,1-Dichloroethene-d2	2.12	63	51648	2.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	48.20%#
20) 2-Butanone-d5	3.96	46	137424	56.96	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.92%
24) Chloroform-d	4.40	84	76244	4.04	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.80%
26) 1,2-Dichloroethane-d4	5.08	65	46025	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.20%
32) Benzene-d6	5.09	84	143774	3.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.60%
36) 1,2-Dichloropropane-d6	6.12	67	47947	3.99	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	79.80%
41) Toluene-d8	7.36	98	123975	3.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	69.20%#
43) trans-1,3-Dichloropropene-	7.66	79	13526	2.95	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	59.00%
46) 2-Hexanone-d5	8.14	63	100431	51.86	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.72%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37802	4.61	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	41889	4.27	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.40%


Target Compounds					Ovalue
13) Acetone	2.21	43	4135	2.556 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011406.D
Acq On : 11 Jun 2019 23:10
Operator : SY/MD
Sample : K3286-01
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0JQ4

Quant Time: Jun 12 04:50:40 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Jun 12 04:39:23 2019
Response via : Initial Calibration

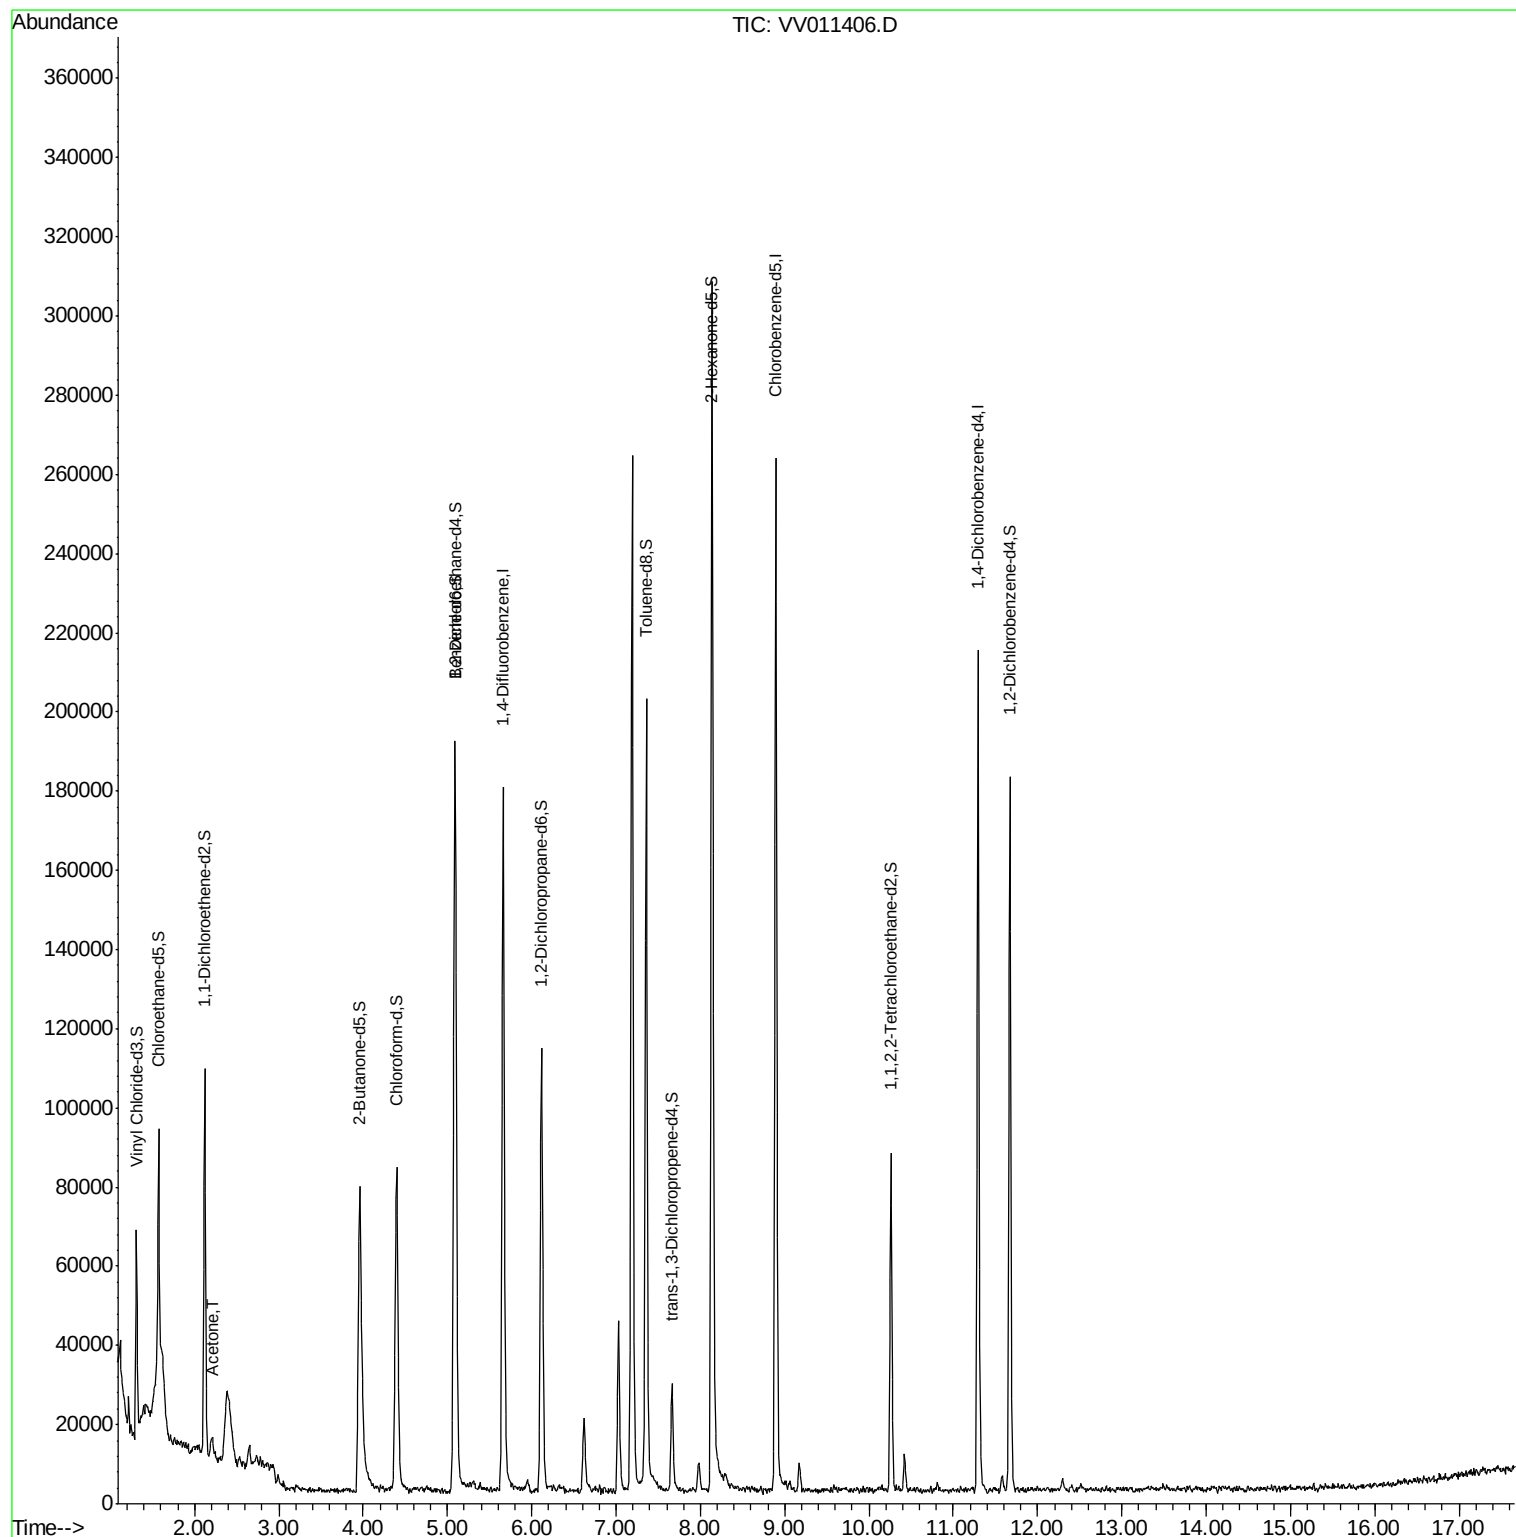

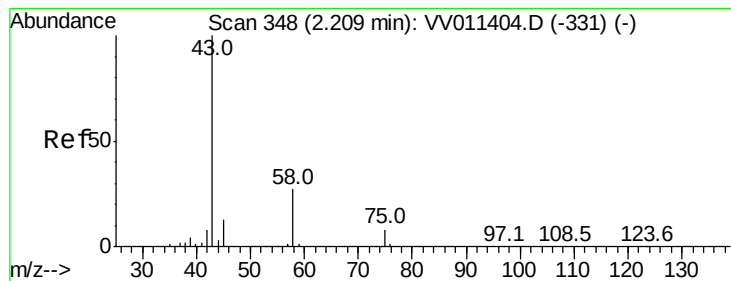

#13

Acetone

Concen: 2.556 ug/L

RT: 2.21 min Scan# 348

Delta R.T. 0.00 min

Lab File: VV011406.D

Acq: 11 Jun 2019 23:10

Instrument :
MSVOA_V
ClientSampleId :
C0JQ4

Tot Ion: 43 Resp: 4135

Ion Ratio Lower Upper

43 100

58 38.2 0.0 55.2

