


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061019\
Data File : VV011343.D
Acq On : 10 Jun 2019 11:29
Operator : SY/MD
Sample : BFB46
Misc : 25ML/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB46

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Jun 12 13:49:01 2019

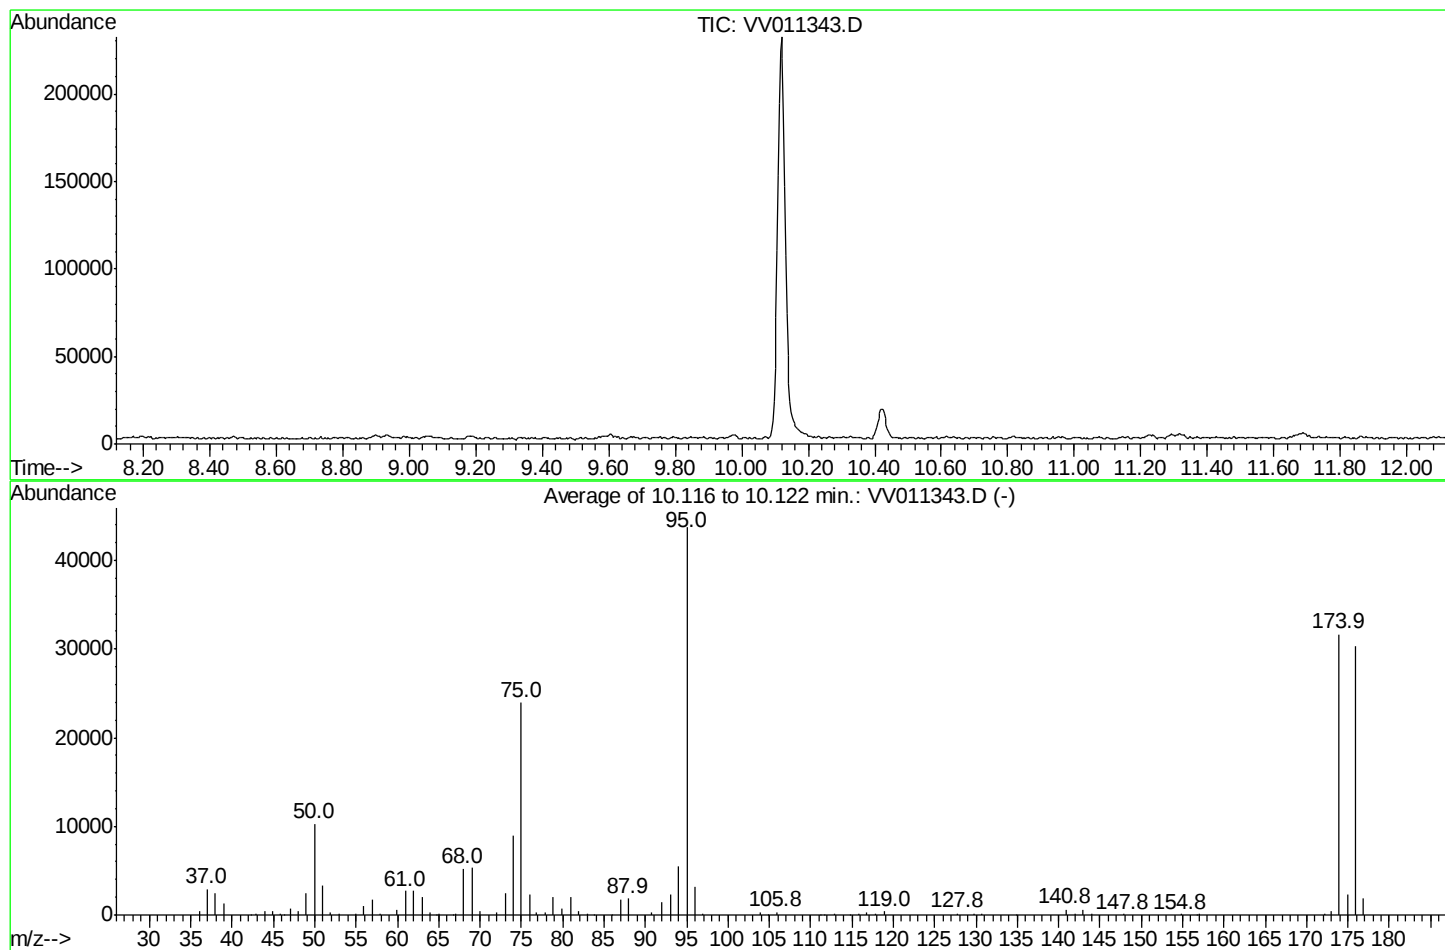

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	10255	PASS
75	95	30	80	54.7	23930	PASS
95	95	100	100	100.0	43738	PASS
96	95	5	9	7.2	3169	PASS
173	174	0.00	2	1.2	395	PASS
174	95	50	120	72.4	31658	PASS
175	174	5	9	7.3	2312	PASS
176	174	95	101	96.0	30392	PASS
177	176	5	9	6.0	1828	PASS

m/z	Abundance
35.40	135.0
36.00	156.0
37.50	164.0
38.00	114.0
38.50	125.0
39.90	1401.0
40.80	203.0
43.10	116.0
43.90	462.0
44.90	119.0
51.60	104.0
55.00	112.0
60.50	105.0
61.20	126.0
63.30	126.0
68.20	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	553.0
36.90	3038.0
37.90	2554.0
39.00	1315.0
39.90	1283.0
41.00	106.0
42.80	205.0
43.90	966.0
45.00	600.0
45.80	139.0
46.30	166.0
47.00	705.0
48.00	484.0
49.00	2508.0
50.00	10353.0
51.00	3250.0
51.90	254.0
54.90	255.0
55.90	1091.0
57.00	1762.0
57.90	137.0
59.90	498.0
60.90	2635.0
62.00	2648.0
63.00	2058.0
64.00	213.0
64.70	161.0
65.10	214.0
66.80	212.0
68.00	5236.0
69.00	5266.0
70.10	416.0
71.90	316.0
73.00	2457.0
74.00	9025.0
75.00	23760.0
76.00	2210.0
76.80	350.0
77.80	313.0
78.80	2068.0
79.90	673.0
80.90	1981.0
81.90	369.0
83.00	123.0
83.70	103.0
87.00	1789.0
87.90	1698.0
90.80	236.0
91.90	1468.0
93.00	2279.0
94.00	5393.0
95.00	44072.0
96.00	3306.0
96.90	110.0
103.90	299.0
104.80	104.0
105.90	289.0
112.80	106.0
114.70	109.0
115.80	232.0
116.80	290.0
117.80	157.0
118.90	434.0
127.80	197.0
129.80	177.0
130.80	102.0
140.80	491.0
142.10	149.0
143.00	445.0
144.00	128.0
147.80	163.0
154.80	164.0
156.70	131.0
172.20	269.0
173.00	549.0
173.90	30496.0
174.90	2288.0
175.90	29344.0
176.90	1794.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	593.0
37.00	3007.0
37.90	2669.0
39.00	1324.0
39.90	1308.0
40.80	124.0
42.80	167.0
43.90	936.0
44.90	602.0
45.90	153.0
47.00	682.0
47.90	516.0
48.90	2500.0
50.00	10570.0
51.00	3403.0
51.90	271.0
53.00	116.0
55.00	244.0
55.90	1085.0
57.00	1757.0
57.90	162.0
59.90	507.0
60.90	2817.0
62.00	2906.0
63.00	2098.0
63.90	246.0
65.10	209.0
67.00	196.0
67.90	5414.0
69.00	5470.0
69.90	399.0
71.90	320.0
73.00	2437.0
74.00	9206.0
75.00	24896.0
76.00	2294.0
76.80	328.0
77.80	264.0
78.80	2101.0
79.90	719.0
80.90	1992.0
81.90	380.0
83.00	115.0
87.00	1748.0
87.90	1876.0
90.80	272.0
91.90	1560.0
93.00	2378.0
94.00	5657.0
95.00	45200.0
95.90	3296.0
96.90	154.0
103.80	289.0
105.90	310.0
112.80	122.0
114.80	107.0
115.80	238.0
116.80	327.0
117.80	197.0
118.90	412.0
127.80	212.0
129.80	168.0
130.70	128.0
140.90	636.0
142.10	160.0
143.00	514.0
144.00	122.0
147.80	139.0
154.80	145.0
156.90	137.0
173.90	32864.0
174.90	2360.0
175.90	31448.0
176.90	1838.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46

m/z	Abundance
36.00	608.0
37.00	2662.0
37.90	2470.0
39.00	1152.0
39.90	1305.0
40.80	129.0
42.30	120.0
42.80	110.0
43.90	822.0
44.90	540.0
45.90	178.0
47.00	604.0
47.90	473.0
48.90	2314.0
50.00	9844.0
51.00	3118.0
51.90	258.0
52.90	130.0
55.00	231.0
55.90	1038.0
57.00	1637.0
57.90	159.0
59.90	553.0
61.00	2651.0
62.00	2698.0
63.00	1932.0
63.90	285.0
64.90	217.0
67.00	207.0
67.90	5005.0
69.00	5163.0
69.90	420.0
72.00	310.0
73.00	2296.0
74.00	8466.0
75.00	23136.0
76.00	2230.0
76.80	287.0
77.80	201.0
78.80	1908.0
79.90	649.0
80.90	1927.0
81.80	423.0
83.00	101.0
86.00	104.0
86.90	1551.0
87.90	1856.0
90.80	252.0
91.90	1456.0
93.00	2162.0
94.00	5464.0
95.00	41944.0
96.00	2905.0
96.90	154.0
103.80	270.0
105.80	299.0
111.10	101.0
111.60	113.0
112.80	133.0
115.90	193.0
116.80	336.0
117.90	254.0
119.00	361.0
127.80	216.0
129.70	159.0
130.80	105.0
134.90	102.0
140.90	670.0
142.00	137.0
142.90	608.0
143.90	116.0
147.90	114.0
157.00	143.0
173.00	636.0
173.90	31616.0
174.90	2289.0
175.90	30384.0
176.90	1852.0

Instrument :
MSVOA_V
ClientSampleId :
BFB46