
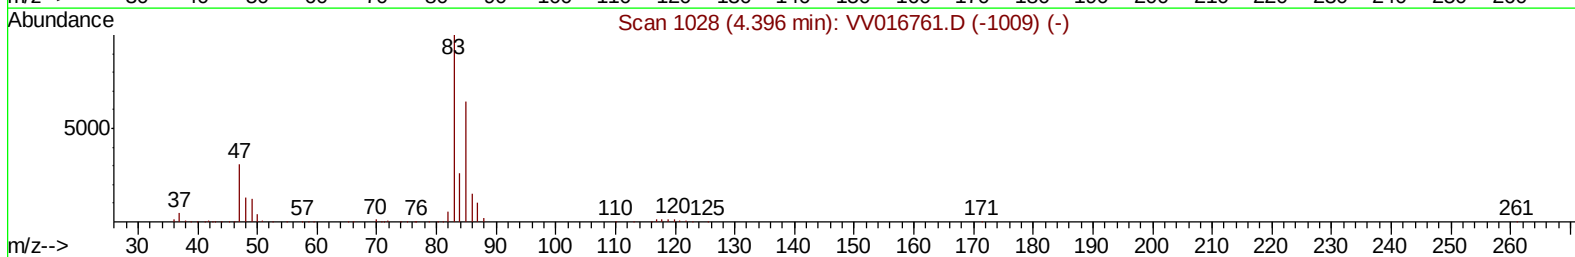
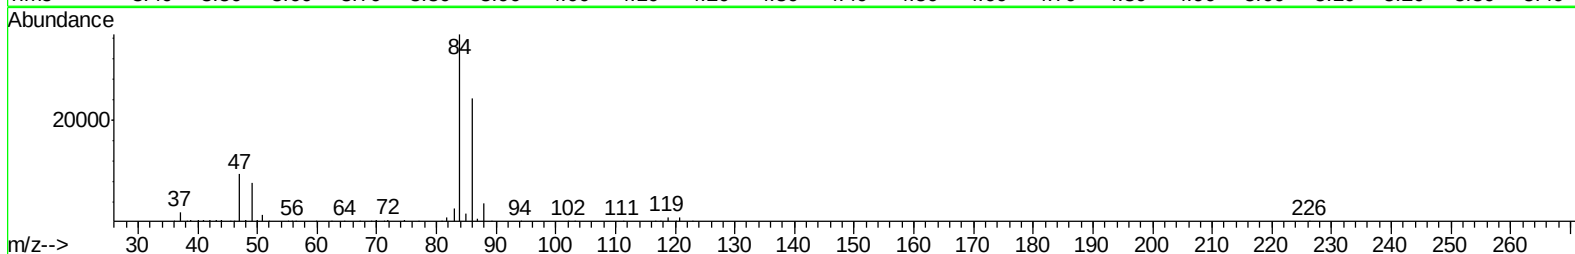


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV061020\
Data File : VV016775.D
Acq On : 10 Jun 2020 17:38
Operator : SY/MD
Sample : L2914-06 20X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Jun 11 01:08:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM060820WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 11 01:04:46 2020
Response via : Initial Calibration

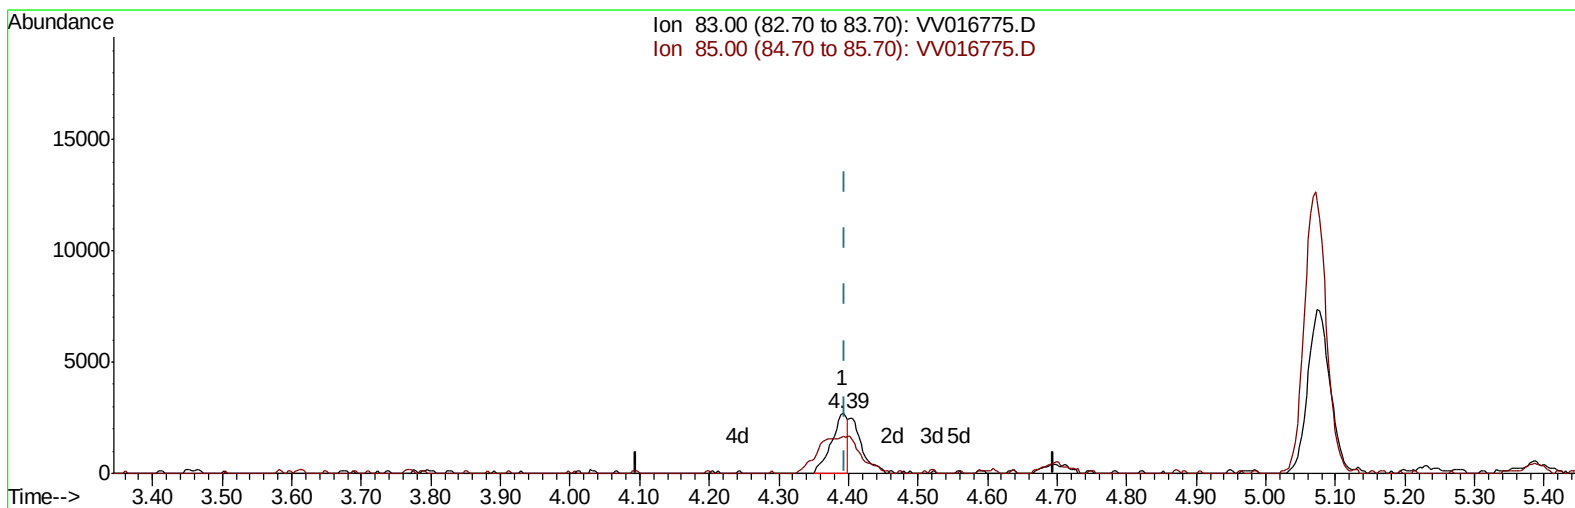

TIC: VV016775.D

(25) Chloroform (T)

4.392min (-0.003) 0.93ug/L

response 4339

Ion	Exp%	Act%
83.00	100	100
85.00	63.00	61.95
0.00	0.00	0.00
0.00	0.00	0.00